

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036827.D
 Acq On : 07 Aug 2024 09:56
 Operator : SY/MD
 Sample : VV0807WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	208936	222297	12.50%	1.650%
2	1.532	146	153	167	rVB	184863	225643	12.69%	1.675%
3	2.060	307	317	331	rBV	362323	524264	29.49%	3.892%
4	3.484	756	760	762	rBB4	680	508	0.03%	0.004%
5	3.587	789	792	793	rBV2	1071	458	0.03%	0.003%
6	3.671	815	818	819	rBV2	730	442	0.02%	0.003%
7	3.796	848	857	891	rBV	113316	324881	18.27%	2.412%
8	4.243	979	996	1023	rBV	279870	717047	40.33%	5.323%
9	4.465	1063	1065	1069	rBV3	676	491	0.03%	0.004%
10	4.526	1081	1084	1086	rBV4	1132	615	0.03%	0.005%
11	4.590	1097	1104	1107	rVB7	1023	1296	0.07%	0.010%
12	4.606	1107	1109	1112	rBV2	677	441	0.02%	0.003%
13	4.732	1145	1148	1155	rVB6	708	823	0.05%	0.006%
14	4.789	1161	1166	1169	rBV5	711	599	0.03%	0.004%
15	4.886	1192	1196	1200	rBV5	688	709	0.04%	0.005%
16	4.950	1200	1216	1245	rBV2	702502	1777833	100.00%	13.197%
17	5.317	1327	1330	1332	rBV3	959	671	0.04%	0.005%
18	5.416	1357	1361	1364	rBV4	575	576	0.03%	0.004%
19	5.474	1377	1379	1385	rVV5	717	649	0.04%	0.005%
20	5.529	1385	1396	1431	rBV	561408	1143934	64.34%	8.492%
21	5.732	1457	1459	1462	rBV3	778	507	0.03%	0.004%
22	5.825	1479	1488	1505	rBV3	22369	51769	2.91%	0.384%
23	5.986	1523	1538	1572	rBV	402881	835610	47.00%	6.203%
24	6.368	1653	1657	1663	rBV5	790	703	0.04%	0.005%
25	6.404	1663	1668	1671	rBV6	772	722	0.04%	0.005%
26	6.474	1688	1690	1693	rVB3	1287	700	0.04%	0.005%
27	6.641	1739	1742	1744	rBV2	919	617	0.03%	0.005%
28	6.664	1746	1749	1750	rVB3	1006	504	0.03%	0.004%
29	6.789	1784	1788	1790	rBV4	707	434	0.02%	0.003%
30	6.912	1815	1826	1853	rBV	227801	437228	24.59%	3.246%
31	7.195	1910	1914	1916	rBV3	1185	968	0.05%	0.007%
32	7.240	1917	1928	1951	rBV	776198	1371083	77.12%	10.178%
33	7.551	2014	2025	2053	rBV	150225	284130	15.98%	2.109%
34	7.912	2130	2137	2146	rVB10	1901	2809	0.16%	0.021%
35	7.953	2146	2150	2154	rBV4	860	644	0.04%	0.005%
36	7.973	2154	2156	2161	rBV5	797	837	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036827.D
 Acq On : 07 Aug 2024 09:56
 Operator : SY/MD
 Sample : VV0807WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.024	2164	2172	2214	rBV2	308947	661076	37.18%	4.907%
38	8.301	2256	2258	2261	rVB4	989	588	0.03%	0.004%
39	8.445	2299	2303	2305	rVB4	667	482	0.03%	0.004%
40	8.461	2305	2308	2310	rVB2	949	579	0.03%	0.004%
41	8.477	2310	2313	2315	rBV4	872	487	0.03%	0.004%
42	8.648	2364	2366	2372	rBV6	644	522	0.03%	0.004%
43	8.693	2377	2380	2385	rBV5	846	488	0.03%	0.004%
44	8.780	2393	2407	2443	rBV	835050	1383716	77.83%	10.272%
45	9.329	2574	2578	2580	rBV3	1308	1213	0.07%	0.009%
46	9.362	2583	2588	2590	rBV3	1275	1054	0.06%	0.008%
47	9.497	2621	2630	2631	rBV6	1003	1064	0.06%	0.008%
48	9.522	2634	2638	2641	rBV4	708	714	0.04%	0.005%
49	9.680	2684	2687	2689	rBV2	765	441	0.02%	0.003%
50	9.802	2722	2725	2728	rVB5	672	463	0.03%	0.003%
51	9.837	2732	2736	2738	rVB4	645	493	0.03%	0.004%
52	9.992	2780	2784	2788	rBV3	577	473	0.03%	0.004%
53	10.056	2798	2804	2808	rBV5	584	651	0.04%	0.005%
54	10.149	2821	2833	2857	rBV	476136	760547	42.78%	5.646%
55	10.368	2898	2901	2905	rBV3	726	563	0.03%	0.004%
56	10.387	2905	2907	2910	rVV4	820	579	0.03%	0.004%
57	10.481	2934	2936	2942	rVV5	848	736	0.04%	0.005%
58	10.754	3017	3021	3023	rBV3	864	594	0.03%	0.004%
59	10.857	3048	3053	3054	rBV4	887	638	0.04%	0.005%
60	10.934	3075	3077	3081	rVB2	738	472	0.03%	0.004%
61	10.995	3092	3096	3099	rBV5	1206	979	0.06%	0.007%
62	11.127	3131	3137	3140	rBV6	2041	2459	0.14%	0.018%
63	11.178	3143	3153	3183	rBV	858485	1369964	77.06%	10.170%
64	11.355	3206	3208	3214	rVB6	1112	677	0.04%	0.005%
65	11.554	3255	3270	3299	rBV	821952	1308120	73.58%	9.711%
66	11.709	3315	3318	3325	rVB7	1105	1157	0.07%	0.009%
67	11.831	3354	3356	3359	rVB4	839	469	0.03%	0.003%
68	11.863	3364	3366	3371	rVB5	1051	869	0.05%	0.006%
69	11.892	3371	3375	3376	rBV3	1083	706	0.04%	0.005%
70	11.937	3384	3389	3390	rBV5	548	450	0.03%	0.003%
71	12.017	3411	3414	3417	rVB3	1341	745	0.04%	0.006%
72	12.146	3449	3454	3456	rBV4	541	476	0.03%	0.004%
73	12.194	3465	3469	3475	rVB4	654	786	0.04%	0.006%
74	12.223	3475	3478	3483	rBV6	559	463	0.03%	0.003%
75	12.291	3494	3499	3501	rBV6	701	564	0.03%	0.004%
76	12.345	3512	3516	3518	rBV4	846	634	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036827.D
 Acq On : 07 Aug 2024 09:56
 Operator : SY/MD
 Sample : VV0807WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK362

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.458	3548	3551	3553	rBV2	984	562	0.03%	0.004%
78	12.583	3586	3590	3593	rBV6	1622	1621	0.09%	0.012%
79	12.644	3603	3609	3613	rBV4	838	1005	0.06%	0.007%
80	12.831	3661	3667	3669	rBV4	782	793	0.04%	0.006%
81	12.844	3669	3671	3673	rVV3	969	506	0.03%	0.004%
82	12.924	3693	3696	3702	rBV3	745	826	0.05%	0.006%
83	13.079	3741	3744	3749	rBV6	1008	801	0.05%	0.006%
84	13.217	3777	3787	3794	rBV7	2681	4789	0.27%	0.036%
85	13.304	3812	3814	3819	rVV5	750	525	0.03%	0.004%
86	13.352	3825	3829	3832	rVB4	807	530	0.03%	0.004%
87	13.451	3854	3860	3862	rBV4	4388	4721	0.27%	0.035%
88	13.535	3882	3886	3890	rBV4	629	519	0.03%	0.004%
89	13.574	3896	3898	3901	rVB2	973	592	0.03%	0.004%
90	13.622	3910	3913	3915	rBV2	691	531	0.03%	0.004%
91	13.689	3924	3934	3942	rVB2	2777	5086	0.29%	0.038%
92	13.725	3942	3945	3950	rVB5	1324	1284	0.07%	0.010%
93	13.757	3950	3955	3956	rBV4	1100	899	0.05%	0.007%
94	13.828	3974	3977	3980	rBV3	767	507	0.03%	0.004%
95	13.931	4006	4009	4011	rBV4	847	487	0.03%	0.004%
96	14.146	4073	4076	4078	rBV2	746	512	0.03%	0.004%
97	14.419	4158	4161	4164	rBV2	725	525	0.03%	0.004%
98	14.622	4221	4224	4228	rBV6	745	547	0.03%	0.004%
99	14.677	4239	4241	4244	rBV3	1032	661	0.04%	0.005%
100	15.635	4537	4539	4540	rBV2	1340	642	0.04%	0.005%




Sum of corrected areas: 13471064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036827.D
Acq On : 07 Aug 2024 09:56
Operator : SY/MD
Sample : VV0807WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

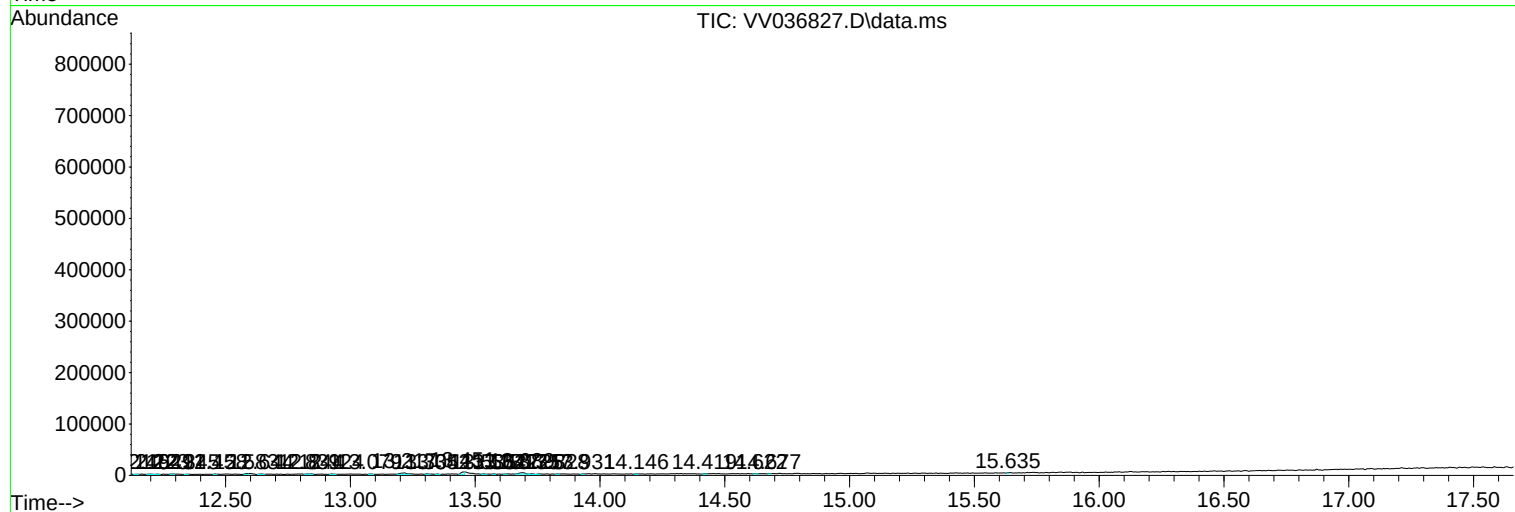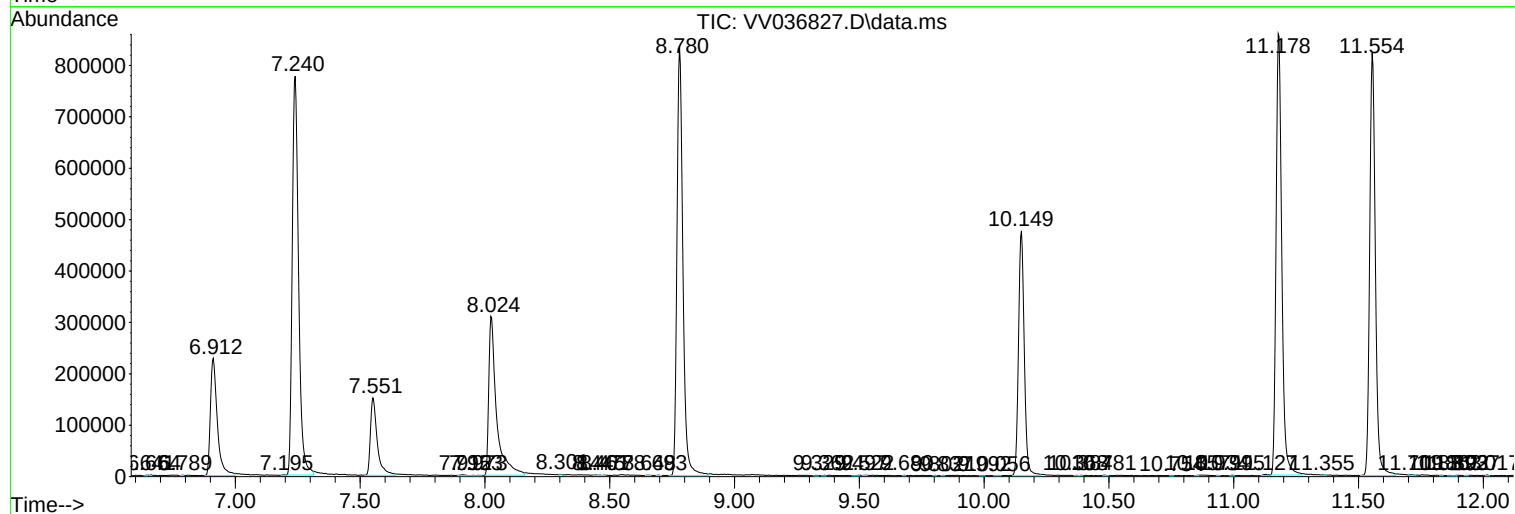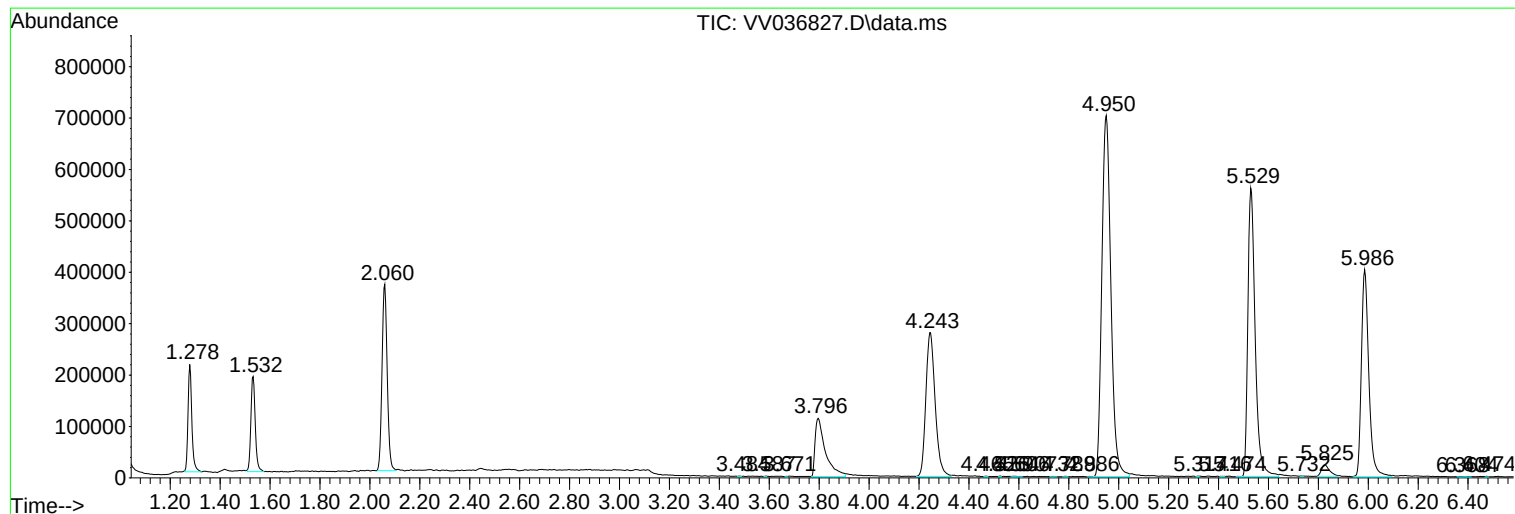

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036827.D
Acq On : 07 Aug 2024 09:56
Operator : SY/MD
Sample : VV0807WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036827.D
Acq On : 07 Aug 2024 09:56
Operator : SY/MD
Sample : VV0807WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK362

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc