

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036828.D
 Acq On : 07 Aug 2024 10:43
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	52	56	60	rBV3	5140	5689	0.33%	0.042%
2	1.278	68	74	90	rVB	227962	245233	14.10%	1.797%
3	1.532	146	153	166	rVB	199547	235149	13.52%	1.723%
4	2.056	307	316	331	rBV	386517	549486	31.60%	4.027%
5	3.568	782	786	789	rVB5	829	698	0.04%	0.005%
6	3.738	834	839	841	rBV4	1007	856	0.05%	0.006%
7	3.793	847	856	891	rBV	95027	261164	15.02%	1.914%
8	4.240	976	995	1023	rBV	277927	706300	40.61%	5.176%
9	4.545	1086	1090	1093	rBV4	1009	863	0.05%	0.006%
10	4.683	1129	1133	1134	rBV3	727	516	0.03%	0.004%
11	4.947	1200	1215	1246	rBV2	686648	1739073	100.00%	12.746%
12	5.172	1283	1285	1293	rVB8	787	631	0.04%	0.005%
13	5.404	1354	1357	1360	rBV4	986	689	0.04%	0.005%
14	5.526	1384	1395	1423	rBV	624370	1273215	73.21%	9.331%
15	5.744	1461	1463	1466	rBV2	815	464	0.03%	0.003%
16	5.822	1476	1487	1501	rBV3	19712	44814	2.58%	0.328%
17	5.982	1525	1537	1570	rBV	383471	799825	45.99%	5.862%
18	6.297	1628	1635	1638	rVB8	662	776	0.04%	0.006%
19	6.375	1657	1659	1663	rVB4	1070	536	0.03%	0.004%
20	6.439	1673	1679	1680	rBV5	767	679	0.04%	0.005%
21	6.513	1700	1702	1706	rVV5	863	680	0.04%	0.005%
22	6.600	1726	1729	1732	rBV3	816	758	0.04%	0.006%
23	6.777	1780	1784	1788	rVB3	1028	710	0.04%	0.005%
24	6.802	1788	1792	1795	rVB5	951	615	0.04%	0.005%
25	6.825	1795	1799	1801	rBV4	604	460	0.03%	0.003%
26	6.908	1815	1825	1861	rBV	222212	430358	24.75%	3.154%
27	7.137	1894	1896	1902	rBV5	1394	1158	0.07%	0.008%
28	7.175	1905	1908	1912	rBV4	946	794	0.05%	0.006%
29	7.236	1916	1927	1951	rBV	768823	1353757	77.84%	9.922%
30	7.548	2015	2024	2057	rBV	147403	276190	15.88%	2.024%
31	7.873	2122	2125	2126	rBV2	758	496	0.03%	0.004%
32	7.912	2134	2137	2144	rVB7	1790	1705	0.10%	0.012%
33	8.024	2163	2172	2217	rBV2	268248	585865	33.69%	4.294%
34	8.297	2253	2257	2259	rVB4	1291	837	0.05%	0.006%
35	8.519	2324	2326	2331	rBV5	581	598	0.03%	0.004%
36	8.558	2336	2338	2342	rVV5	850	645	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036828.D
 Acq On : 07 Aug 2024 10:43
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.654	2366	2368	2373	rVB3	888	668	0.04%	0.005%
38	8.690	2373	2379	2382	rBV5	1151	1208	0.07%	0.009%
39	8.780	2395	2407	2438	rBV	931174	1547212	88.97%	11.340%
40	9.220	2541	2544	2547	rBV4	1043	857	0.05%	0.006%
41	9.339	2575	2581	2585	rVV6	511	708	0.04%	0.005%
42	9.365	2585	2589	2592	rVV3	849	704	0.04%	0.005%
43	9.381	2592	2594	2598	rVB5	702	485	0.03%	0.004%
44	9.432	2607	2610	2613	rBV3	837	642	0.04%	0.005%
45	9.452	2613	2616	2619	rBV3	557	468	0.03%	0.003%
46	9.484	2623	2626	2629	rBV3	704	604	0.03%	0.004%
47	9.590	2656	2659	2661	rBV2	1075	584	0.03%	0.004%
48	9.651	2674	2678	2681	rBV4	662	597	0.03%	0.004%
49	9.683	2685	2688	2690	rBV2	734	570	0.03%	0.004%
50	9.696	2690	2692	2694	rVV2	880	462	0.03%	0.003%
51	9.715	2694	2698	2703	rVB5	836	953	0.05%	0.007%
52	9.744	2703	2707	2709	rBV2	676	468	0.03%	0.003%
53	10.005	2784	2788	2791	rBV3	824	785	0.05%	0.006%
54	10.149	2817	2833	2858	rBV	429404	695850	40.01%	5.100%
55	10.320	2881	2886	2893	rVB7	1297	1442	0.08%	0.011%
56	10.420	2915	2917	2921	rVB3	766	525	0.03%	0.004%
57	10.455	2925	2928	2934	rBV4	615	646	0.04%	0.005%
58	10.484	2934	2937	2940	rBV4	690	579	0.03%	0.004%
59	10.612	2974	2977	2979	rVV3	817	505	0.03%	0.004%
60	10.664	2988	2993	2995	rBV4	1038	999	0.06%	0.007%
61	10.677	2995	2997	3001	rVV4	677	543	0.03%	0.004%
62	10.783	3024	3030	3033	rBV5	515	488	0.03%	0.004%
63	10.976	3087	3090	3092	rBV3	868	500	0.03%	0.004%
64	11.063	3109	3117	3121	rBV5	1137	1140	0.07%	0.008%
65	11.130	3133	3138	3143	rBV7	2018	2108	0.12%	0.015%
66	11.178	3143	3153	3189	rVV	977246	1544776	88.83%	11.322%
67	11.555	3257	3270	3300	rBV	797209	1280331	73.62%	9.384%
68	11.738	3323	3327	3333	rVB6	1321	1450	0.08%	0.011%
69	11.767	3334	3336	3343	rVB6	939	868	0.05%	0.006%
70	11.844	3357	3360	3363	rBV4	699	558	0.03%	0.004%
71	11.860	3363	3365	3369	rVV4	772	518	0.03%	0.004%
72	12.034	3415	3419	3420	rBV2	673	493	0.03%	0.004%
73	12.053	3423	3425	3427	rVV3	979	557	0.03%	0.004%
74	12.082	3430	3434	3438	rVB3	904	637	0.04%	0.005%
75	12.117	3443	3445	3451	rVB4	803	704	0.04%	0.005%
76	12.210	3471	3474	3480	rVB6	626	701	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036828.D
 Acq On : 07 Aug 2024 10:43
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.323	3506	3509	3513	rVB4	788	502	0.03%	0.004%
78	12.439	3543	3545	3547	rBV2	1255	699	0.04%	0.005%
79	12.481	3554	3558	3560	rBV3	927	738	0.04%	0.005%
80	12.519	3565	3570	3574	rVB7	538	501	0.03%	0.004%
81	12.583	3586	3590	3591	rBV3	1227	732	0.04%	0.005%
82	12.821	3661	3664	3672	rVB6	856	1088	0.06%	0.008%
83	12.860	3672	3676	3680	rBV4	761	758	0.04%	0.006%
84	12.924	3693	3696	3700	rBV4	567	464	0.03%	0.003%
85	13.011	3717	3723	3725	rBV4	470	467	0.03%	0.003%
86	13.191	3776	3779	3780	rBV3	967	520	0.03%	0.004%
87	13.220	3780	3788	3796	rVB10	2343	4100	0.24%	0.030%
88	13.294	3808	3811	3815	rBV5	762	558	0.03%	0.004%
89	13.458	3854	3862	3871	rBV5	4162	7916	0.46%	0.058%
90	13.577	3894	3899	3901	rVB4	702	482	0.03%	0.004%
91	13.654	3919	3923	3926	rBV3	686	547	0.03%	0.004%
92	13.731	3943	3947	3948	rBV3	1003	741	0.04%	0.005%
93	13.767	3955	3958	3962	rBV4	964	575	0.03%	0.004%
94	13.876	3990	3992	3997	rBV3	908	737	0.04%	0.005%
95	14.021	4034	4037	4039	rBV3	605	489	0.03%	0.004%
96	14.172	4081	4084	4087	rBV2	965	835	0.05%	0.006%
97	14.307	4123	4126	4130	rBV5	1057	1121	0.06%	0.008%
98	14.542	4196	4199	4205	rVB6	1179	1362	0.08%	0.010%
99	14.841	4290	4292	4296	rVB3	933	584	0.03%	0.004%
100	15.194	4400	4402	4406	rVB3	1334	712	0.04%	0.005%




Sum of corrected areas: 13644403

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036828.D
Acq On : 07 Aug 2024 10:43
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

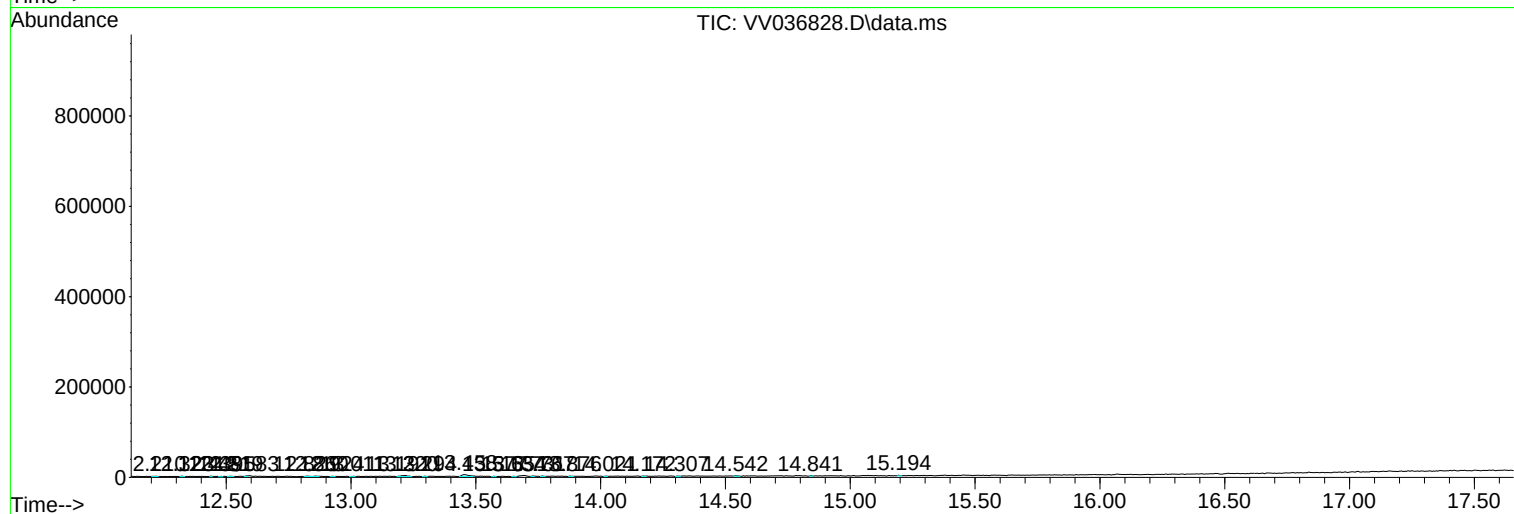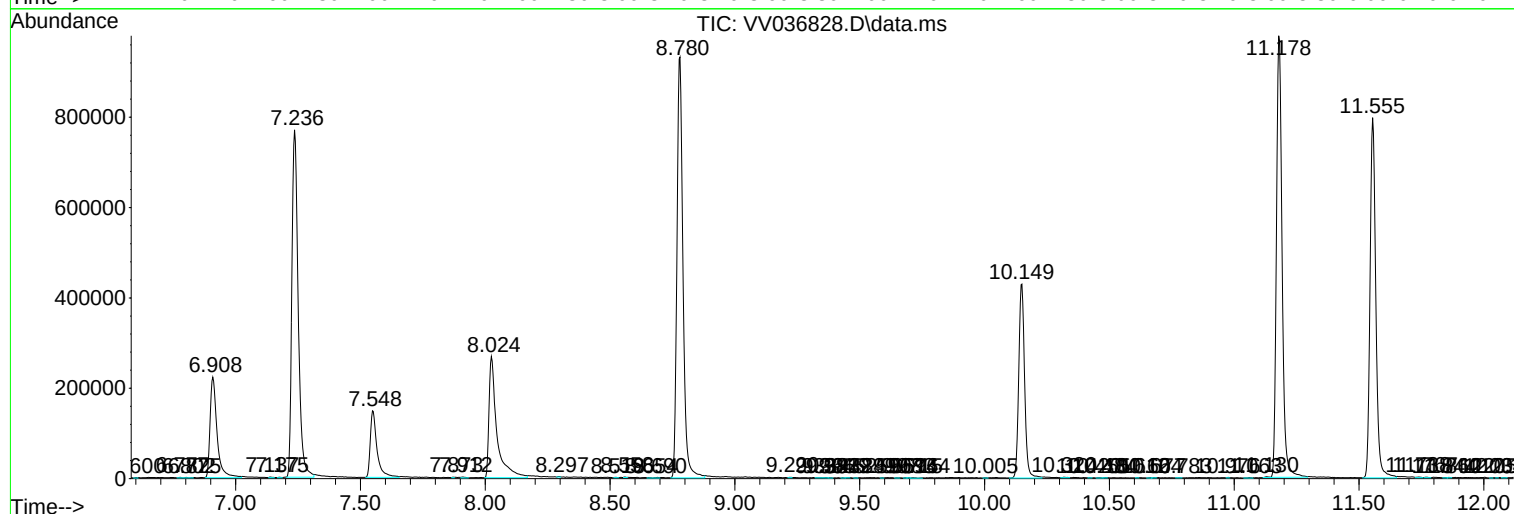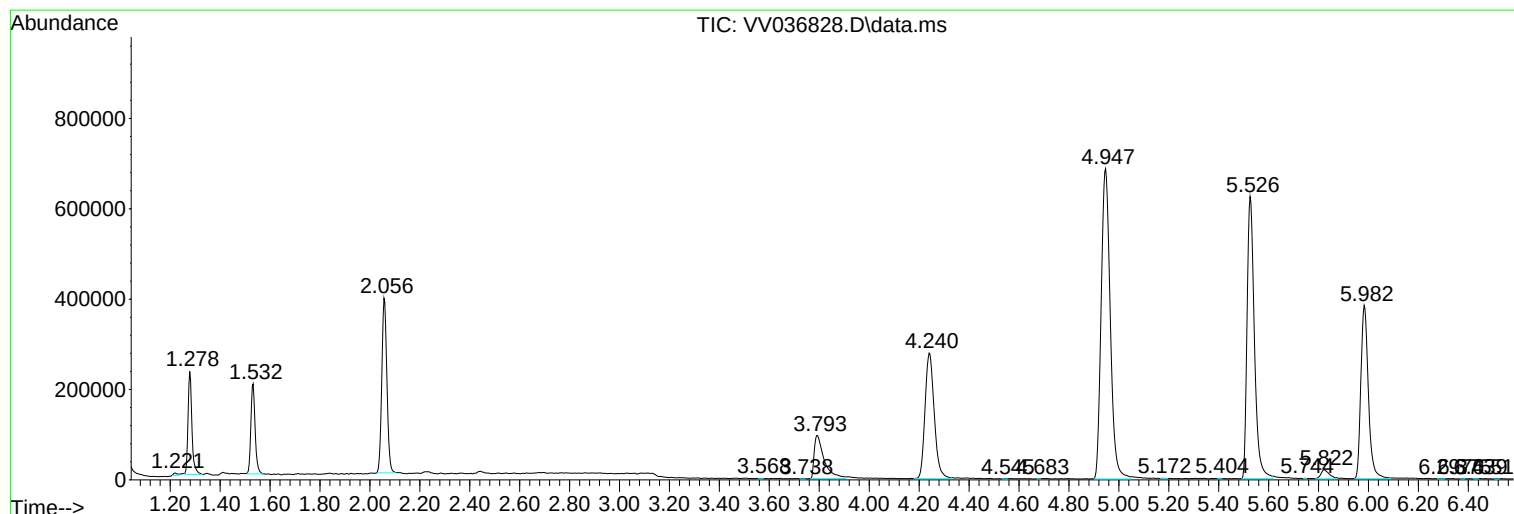

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036828.D
Acq On : 07 Aug 2024 10:43
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036828.D
Acq On : 07 Aug 2024 10:43
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc