

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036832.D
 Acq On : 07 Aug 2024 12:09
 Operator : SY/MD
 Sample : P3480-08
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	228460	246848	14.02%	1.857%
2	1.532	146	153	170	rVB	203055	239993	13.63%	1.805%
3	2.059	307	317	328	rBV	378817	545145	30.96%	4.101%
4	3.432	741	744	747	rBV4	708	547	0.03%	0.004%
5	3.587	788	792	796	rBV5	766	719	0.04%	0.005%
6	3.625	801	804	806	rBV3	761	455	0.03%	0.003%
7	3.731	832	837	838	rBV4	591	457	0.03%	0.003%
8	3.796	848	857	881	rBV	100389	265013	15.05%	1.994%
9	4.246	979	997	1023	rBV	273699	707768	40.20%	5.324%
10	4.487	1067	1072	1076	rBV6	1213	1166	0.07%	0.009%
11	4.535	1085	1087	1091	rVB2	845	553	0.03%	0.004%
12	4.567	1095	1097	1100	rVV2	818	468	0.03%	0.004%
13	4.950	1198	1216	1247	rBV2	694813	1760660	100.00%	13.244%
14	5.198	1290	1293	1297	rVB2	1061	688	0.04%	0.005%
15	5.220	1297	1300	1303	rBV4	754	466	0.03%	0.004%
16	5.317	1327	1330	1333	rBV4	1102	587	0.03%	0.004%
17	5.484	1375	1382	1384	rBV5	1241	1499	0.09%	0.011%
18	5.532	1385	1397	1428	rVV	565026	1149723	65.30%	8.649%
19	5.821	1476	1487	1509	rBV2	37521	82682	4.70%	0.622%
20	5.985	1522	1538	1571	rBV2	393204	815275	46.31%	6.133%
21	6.333	1644	1646	1651	rVB5	744	499	0.03%	0.004%
22	6.362	1653	1655	1658	rVB2	1005	475	0.03%	0.004%
23	6.384	1658	1662	1663	rBV3	822	558	0.03%	0.004%
24	6.448	1678	1682	1683	rBV2	828	501	0.03%	0.004%
25	6.596	1724	1728	1731	rVB4	899	681	0.04%	0.005%
26	6.622	1731	1736	1738	rBV4	683	689	0.04%	0.005%
27	6.751	1773	1776	1781	rVB4	801	566	0.03%	0.004%
28	6.911	1815	1826	1857	rBV	219630	428001	24.31%	3.220%
29	7.239	1917	1928	1950	rBV	778131	1362652	77.39%	10.250%
30	7.551	2016	2025	2052	rVV	144749	269767	15.32%	2.029%
31	7.834	2110	2113	2119	rVV7	899	915	0.05%	0.007%
32	7.886	2126	2129	2131	rVV2	856	474	0.03%	0.004%
33	7.908	2131	2136	2140	rVV7	994	999	0.06%	0.008%
34	8.027	2164	2173	2217	rBV2	263065	594161	33.75%	4.470%
35	8.313	2260	2262	2264	rBV2	801	464	0.03%	0.003%
36	8.558	2334	2338	2342	rBV6	1423	1179	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036832.D
 Acq On : 07 Aug 2024 12:09
 Operator : SY/MD
 Sample : P3480-08
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.606	2351	2353	2357	rVB3	804	631	0.04%	0.005%
38	8.635	2357	2362	2365	rBV5	1011	839	0.05%	0.006%
39	8.779	2396	2407	2438	rBV	845757	1406853	79.90%	10.583%
40	9.040	2485	2488	2490	rBV3	891	566	0.03%	0.004%
41	9.085	2496	2502	2508	rBV8	2437	3900	0.22%	0.029%
42	9.185	2530	2533	2535	rVB4	824	519	0.03%	0.004%
43	9.268	2554	2559	2562	rBV5	958	800	0.05%	0.006%
44	9.484	2620	2626	2637	rBV9	1555	3414	0.19%	0.026%
45	9.918	2759	2761	2764	rVV2	1234	645	0.04%	0.005%
46	9.979	2777	2780	2782	rBV4	559	449	0.03%	0.003%
47	10.014	2787	2791	2794	rBV5	680	563	0.03%	0.004%
48	10.037	2795	2798	2802	rVB4	725	514	0.03%	0.004%
49	10.078	2809	2811	2815	rVB4	920	516	0.03%	0.004%
50	10.149	2821	2833	2854	rBV	411007	651112	36.98%	4.898%
51	10.313	2878	2884	2891	rVB6	994	1511	0.09%	0.011%
52	10.345	2891	2894	2895	rBV2	978	593	0.03%	0.004%
53	10.603	2972	2974	2981	rVB5	713	531	0.03%	0.004%
54	10.651	2986	2989	2993	rVB3	626	575	0.03%	0.004%
55	10.683	2993	2999	3005	rVB6	952	1073	0.06%	0.008%
56	10.715	3005	3009	3012	rBV5	528	549	0.03%	0.004%
57	10.847	3047	3050	3053	rBV3	917	783	0.04%	0.006%
58	11.017	3101	3103	3112	rVB5	1076	1308	0.07%	0.010%
59	11.072	3112	3120	3123	rBV4	1147	1414	0.08%	0.011%
60	11.117	3130	3134	3135	rBV3	729	539	0.03%	0.004%
61	11.181	3142	3154	3178	rBV	881370	1390702	78.99%	10.461%
62	11.377	3212	3215	3218	rVV4	734	595	0.03%	0.004%
63	11.400	3220	3222	3225	rVB4	957	524	0.03%	0.004%
64	11.448	3234	3237	3242	rBV5	798	973	0.06%	0.007%
65	11.493	3242	3251	3259	rBV4	9043	19463	1.11%	0.146%
66	11.554	3260	3270	3303	rVB	804366	1290635	73.30%	9.709%
67	11.844	3358	3360	3363	rBV4	811	492	0.03%	0.004%
68	11.889	3372	3374	3377	rVB4	865	454	0.03%	0.003%
69	11.911	3377	3381	3383	rBV5	612	489	0.03%	0.004%
70	11.995	3405	3407	3411	rBV5	860	644	0.04%	0.005%
71	12.017	3411	3414	3419	rVB6	827	716	0.04%	0.005%
72	12.072	3427	3431	3433	rBV3	730	498	0.03%	0.004%
73	12.258	3485	3489	3490	rBV2	566	454	0.03%	0.003%
74	12.268	3490	3492	3496	rVV3	876	586	0.03%	0.004%
75	12.291	3496	3499	3504	rVB4	756	621	0.04%	0.005%
76	12.316	3504	3507	3509	rBV3	928	645	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036832.D
 Acq On : 07 Aug 2024 12:09
 Operator : SY/MD
 Sample : P3480-08
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.342	3512	3515	3518	rVV3	852	562	0.03%	0.004%
78	12.361	3518	3521	3523	rVV5	799	498	0.03%	0.004%
79	12.384	3523	3528	3532	rVB5	861	805	0.05%	0.006%
80	12.435	3537	3544	3546	rBV4	981	1007	0.06%	0.008%
81	12.512	3565	3568	3574	rBV5	1716	1569	0.09%	0.012%
82	12.545	3574	3578	3580	rVV4	550	454	0.03%	0.003%
83	12.577	3584	3588	3591	rVV4	534	536	0.03%	0.004%
84	12.741	3634	3639	3642	rBV4	864	790	0.04%	0.006%
85	13.210	3782	3785	3791	rVV7	1657	1496	0.08%	0.011%
86	13.400	3842	3844	3849	rBV6	613	449	0.03%	0.003%
87	13.454	3856	3861	3862	rBV4	2055	1741	0.10%	0.013%
88	13.538	3880	3887	3891	rBV6	702	900	0.05%	0.007%
89	13.628	3909	3915	3916	rBV4	805	721	0.04%	0.005%
90	13.683	3927	3932	3937	rBV7	1298	1510	0.09%	0.011%
91	13.766	3955	3958	3961	rBV3	841	624	0.04%	0.005%
92	13.889	3993	3996	3997	rBV3	1103	630	0.04%	0.005%
93	13.969	4016	4021	4027	rBV7	1141	1539	0.09%	0.012%
94	13.998	4027	4030	4033	rVB2	615	444	0.03%	0.003%
95	14.094	4056	4060	4065	rBV5	933	837	0.05%	0.006%
96	14.136	4069	4073	4079	rBV6	957	930	0.05%	0.007%
97	14.348	4135	4139	4142	rBV3	1347	1465	0.08%	0.011%
98	14.535	4195	4197	4201	rVB4	865	504	0.03%	0.004%
99	15.136	4381	4384	4389	rBV5	1082	808	0.05%	0.006%
100	15.229	4410	4413	4415	rBV3	1206	818	0.05%	0.006%




Sum of corrected areas: 13293618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036832.D
Acq On : 07 Aug 2024 12:09
Operator : SY/MD
Sample : P3480-08
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

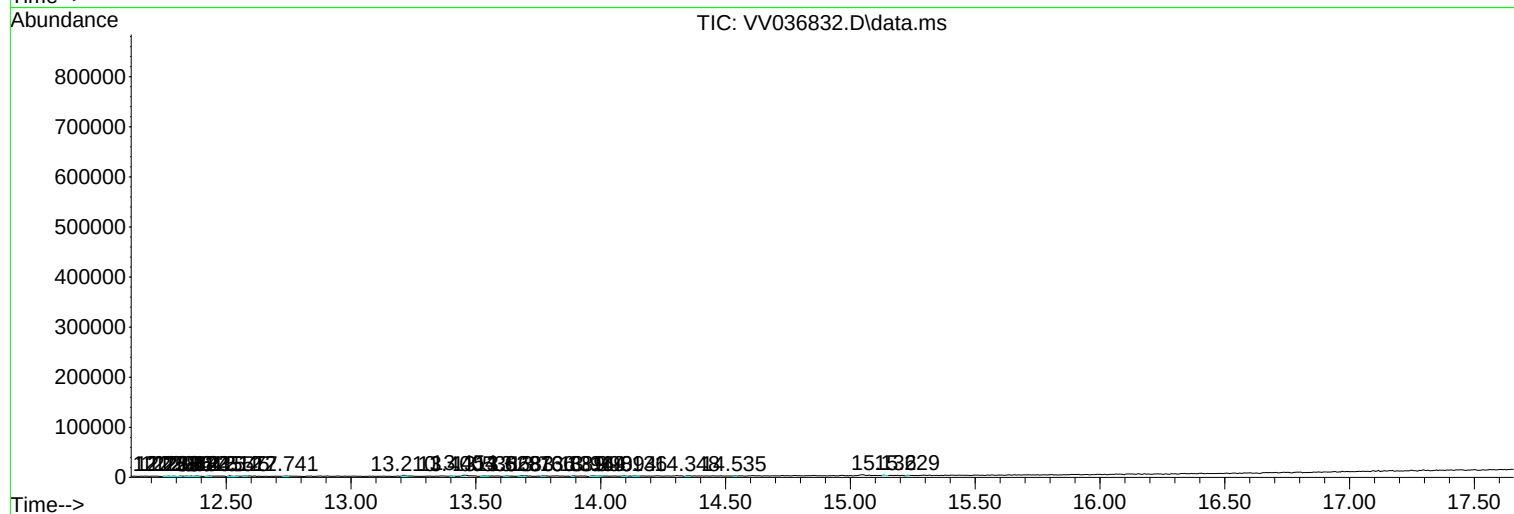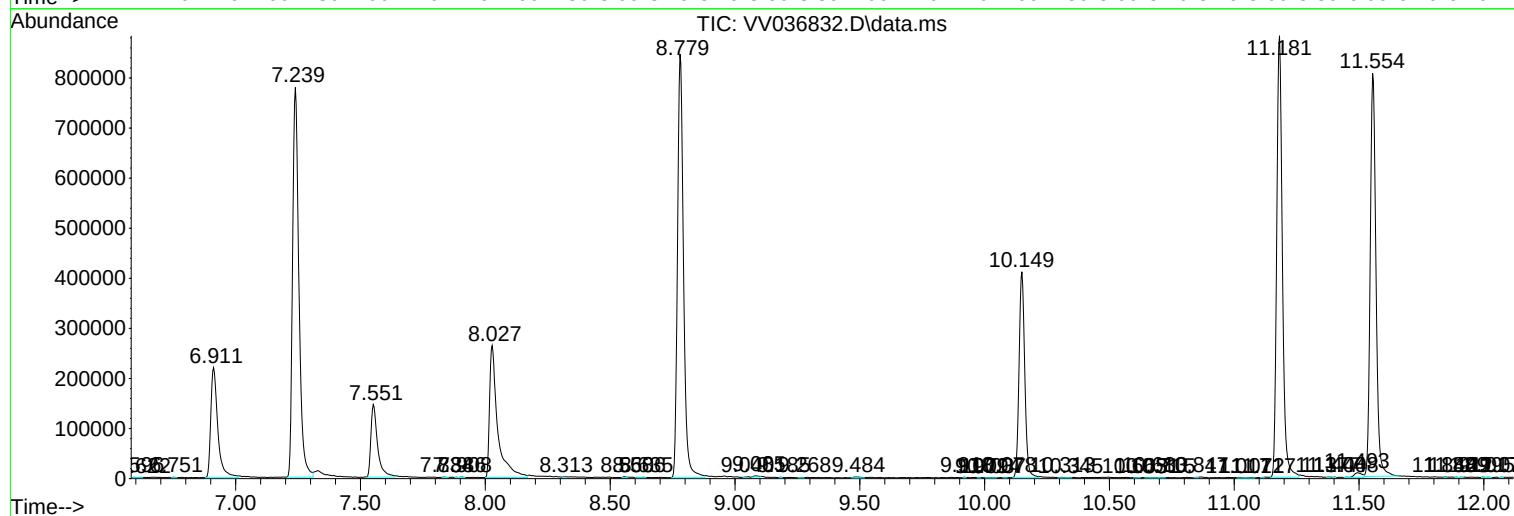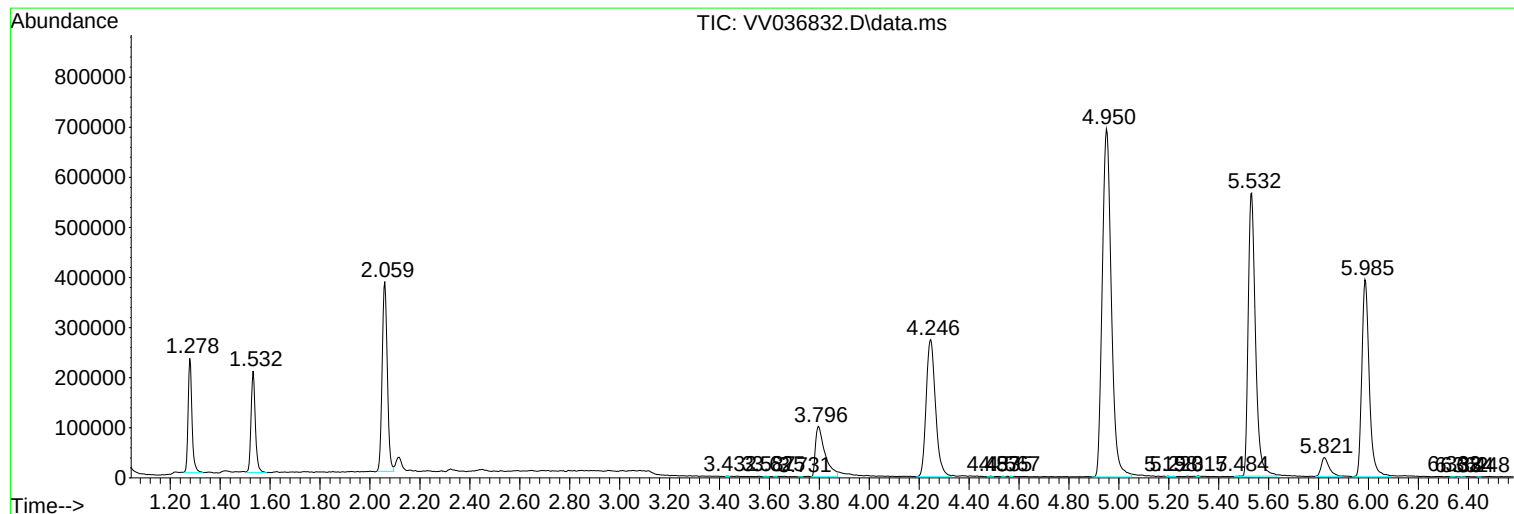

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036832.D
Acq On : 07 Aug 2024 12:09
Operator : SY/MD
Sample : P3480-08
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036832.D
Acq On : 07 Aug 2024 12:09
Operator : SY/MD
Sample : P3480-08
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------