

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036834.D
 Acq On : 07 Aug 2024 12:53
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	228692	246459	13.84%	1.804%
2	1.532	146	153	167	rVB	201374	237651	13.34%	1.739%
3	2.060	307	317	332	rBV	384472	554549	31.13%	4.059%
4	3.471	752	756	760	rBV4	1085	1150	0.06%	0.008%
5	3.722	830	834	837	rBV4	928	749	0.04%	0.005%
6	3.799	849	858	886	rBV	99483	276319	15.51%	2.022%
7	4.063	938	940	946	rVB5	695	569	0.03%	0.004%
8	4.246	977	997	1031	rBV3	296077	883623	49.61%	6.467%
9	4.410	1046	1048	1052	rVB4	1518	867	0.05%	0.006%
10	4.571	1095	1098	1102	rVB5	1172	687	0.04%	0.005%
11	4.613	1108	1111	1112	rBV2	762	466	0.03%	0.003%
12	4.799	1166	1169	1174	rVB6	652	598	0.03%	0.004%
13	4.825	1174	1177	1179	rBV4	817	434	0.02%	0.003%
14	4.834	1179	1180	1184	rVB3	949	519	0.03%	0.004%
15	4.860	1184	1188	1189	rBV2	799	535	0.03%	0.004%
16	4.950	1199	1216	1247	rBV2	713324	1781209	100.00%	13.036%
17	5.294	1321	1323	1327	rVB5	864	519	0.03%	0.004%
18	5.330	1332	1334	1338	rBV3	605	444	0.02%	0.003%
19	5.423	1361	1363	1365	rVB3	816	442	0.02%	0.003%
20	5.529	1381	1396	1431	rBV	581470	1181630	66.34%	8.648%
21	5.715	1452	1454	1458	rVB4	1378	848	0.05%	0.006%
22	5.773	1467	1472	1475	rBV5	975	863	0.05%	0.006%
23	5.822	1475	1487	1510	rVV	49254	109363	6.14%	0.800%
24	5.985	1525	1538	1568	rBV	397729	828232	46.50%	6.062%
25	6.214	1606	1609	1612	rVB4	893	606	0.03%	0.004%
26	6.320	1638	1642	1643	rBV3	855	518	0.03%	0.004%
27	6.439	1667	1679	1696	rBV2	16429	36321	2.04%	0.266%
28	6.609	1728	1732	1733	rBV3	726	443	0.02%	0.003%
29	6.693	1755	1758	1761	rBV2	868	598	0.03%	0.004%
30	6.709	1761	1763	1766	rVB3	826	518	0.03%	0.004%
31	6.735	1767	1771	1773	rBV4	906	793	0.04%	0.006%
32	6.912	1816	1826	1856	rBV	227590	436451	24.50%	3.194%
33	7.130	1892	1894	1899	rVB4	1120	921	0.05%	0.007%
34	7.172	1899	1907	1909	rBV6	968	1261	0.07%	0.009%
35	7.239	1917	1928	1950	rBV	793694	1384465	77.73%	10.133%
36	7.551	2016	2025	2057	rVV	147276	275860	15.49%	2.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036834.D
 Acq On : 07 Aug 2024 12:53
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	7.911	2133	2137	2139	rBV4	1365	1190	0.07%	0.009%
38	7.953	2145	2150	2151	rBV5	669	522	0.03%	0.004%
39	8.027	2164	2173	2208	rBV2	263011	601046	33.74%	4.399%
40	8.493	2317	2318	2327	rVB6	1384	1246	0.07%	0.009%
41	8.677	2372	2375	2377	rBV4	737	453	0.03%	0.003%
42	8.780	2393	2407	2431	rBV	858764	1419395	79.69%	10.388%
43	9.050	2489	2491	2496	rBV5	701	626	0.04%	0.005%
44	9.079	2496	2500	2502	rBV3	1805	1404	0.08%	0.010%
45	9.220	2541	2544	2550	rBV4	1099	883	0.05%	0.006%
46	9.329	2576	2578	2580	rBV	937	516	0.03%	0.004%
47	9.490	2624	2628	2632	rBV5	771	605	0.03%	0.004%
48	9.670	2680	2684	2688	rBV6	1062	903	0.05%	0.007%
49	9.696	2688	2692	2696	rBV7	1293	1140	0.06%	0.008%
50	9.728	2697	2702	2704	rVB5	574	408	0.02%	0.003%
51	9.802	2723	2725	2728	rBV3	971	641	0.04%	0.005%
52	9.873	2744	2747	2750	rVB3	883	542	0.03%	0.004%
53	9.902	2750	2756	2761	rBV7	878	1413	0.08%	0.010%
54	10.011	2786	2790	2793	rBV5	746	607	0.03%	0.004%
55	10.050	2799	2802	2805	rVB2	753	467	0.03%	0.003%
56	10.149	2817	2833	2858	rBV	403213	642797	36.09%	4.704%
57	10.345	2890	2894	2896	rVB3	722	485	0.03%	0.004%
58	10.410	2910	2914	2918	rVB5	959	861	0.05%	0.006%
59	10.435	2918	2922	2924	rBV4	627	634	0.04%	0.005%
60	10.471	2930	2933	2935	rBV3	692	472	0.03%	0.003%
61	10.545	2954	2956	2959	rBV3	810	549	0.03%	0.004%
62	10.661	2988	2992	2995	rVB3	980	781	0.04%	0.006%
63	10.683	2995	2999	3000	rBV2	796	585	0.03%	0.004%
64	10.744	3014	3018	3021	rBV3	1104	870	0.05%	0.006%
65	10.796	3031	3034	3036	rVB2	905	505	0.03%	0.004%
66	10.866	3047	3056	3063	rBV6	1534	2391	0.13%	0.017%
67	10.940	3074	3079	3080	rBV3	814	663	0.04%	0.005%
68	11.030	3104	3107	3109	rVB3	826	508	0.03%	0.004%
69	11.050	3109	3113	3115	rVB3	940	686	0.04%	0.005%
70	11.111	3129	3132	3133	rBV2	810	449	0.03%	0.003%
71	11.181	3143	3154	3174	rBV	892296	1407125	79.00%	10.298%
72	11.365	3208	3211	3213	rBV4	872	531	0.03%	0.004%
73	11.513	3248	3257	3259	rBV5	2953	4063	0.23%	0.030%
74	11.554	3259	3270	3303	rVB	809215	1299191	72.94%	9.508%
75	11.783	3339	3341	3344	rVB4	1019	434	0.02%	0.003%
76	11.863	3362	3366	3369	rBV4	500	443	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036834.D
 Acq On : 07 Aug 2024 12:53
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	11.976	3399	3401	3406	rBV5	618	488	0.03%	0.004%
78	12.120	3444	3446	3451	rVB5	664	544	0.03%	0.004%
79	12.378	3519	3526	3529	rBV7	978	1007	0.06%	0.007%
80	12.519	3569	3570	3576	rVB3	620	451	0.03%	0.003%
81	12.596	3590	3594	3597	rVB3	909	753	0.04%	0.006%
82	12.959	3704	3707	3710	rBV3	746	650	0.04%	0.005%
83	12.988	3713	3716	3719	rVB3	764	470	0.03%	0.003%
84	13.008	3719	3722	3724	rBV3	869	488	0.03%	0.004%
85	13.024	3724	3727	3733	rVB4	838	674	0.04%	0.005%
86	13.165	3767	3771	3774	rBV5	649	490	0.03%	0.004%
87	13.214	3781	3786	3788	rBV4	1642	1395	0.08%	0.010%
88	13.252	3795	3798	3800	rBV4	866	535	0.03%	0.004%
89	13.432	3851	3854	3857	rBV3	815	698	0.04%	0.005%
90	13.689	3926	3934	3937	rBV8	1586	1987	0.11%	0.015%
91	14.037	4038	4042	4045	rBV4	651	709	0.04%	0.005%
92	14.149	4074	4077	4080	rBV5	698	459	0.03%	0.003%
93	14.165	4080	4082	4086	rBV5	764	466	0.03%	0.003%
94	14.230	4100	4102	4106	rVB4	903	609	0.03%	0.004%
95	14.262	4108	4112	4114	rBV3	757	585	0.03%	0.004%
96	14.316	4127	4129	4132	rBV3	803	441	0.02%	0.003%
97	14.361	4140	4143	4146	rVB3	880	437	0.02%	0.003%
98	14.648	4230	4232	4236	rVB4	1058	580	0.03%	0.004%
99	14.673	4236	4240	4242	rBV2	708	576	0.03%	0.004%
100	15.271	4421	4426	4428	rBV5	1514	1578	0.09%	0.012%




Sum of corrected areas: 13663580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036834.D
Acq On : 07 Aug 2024 12:53
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

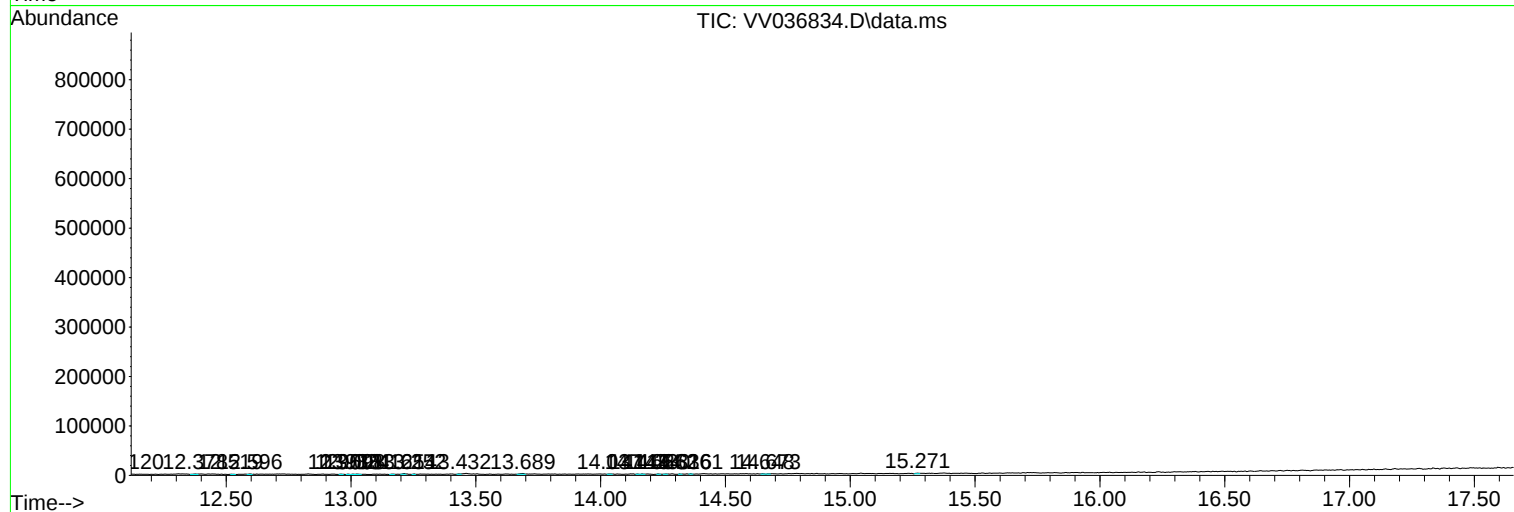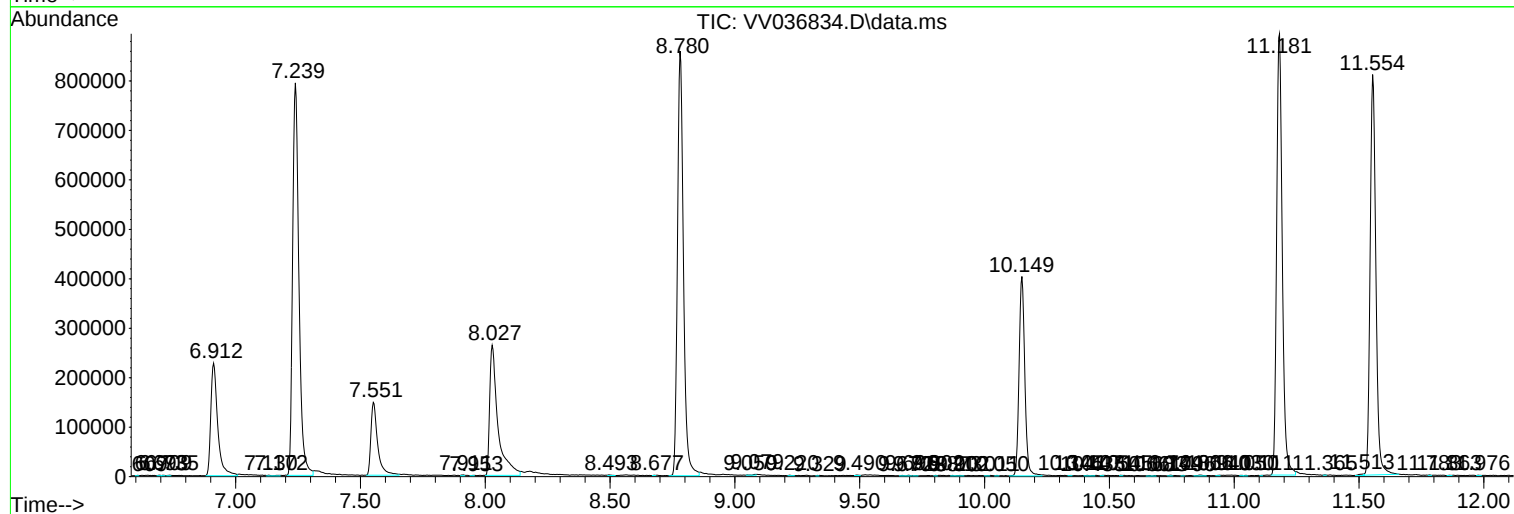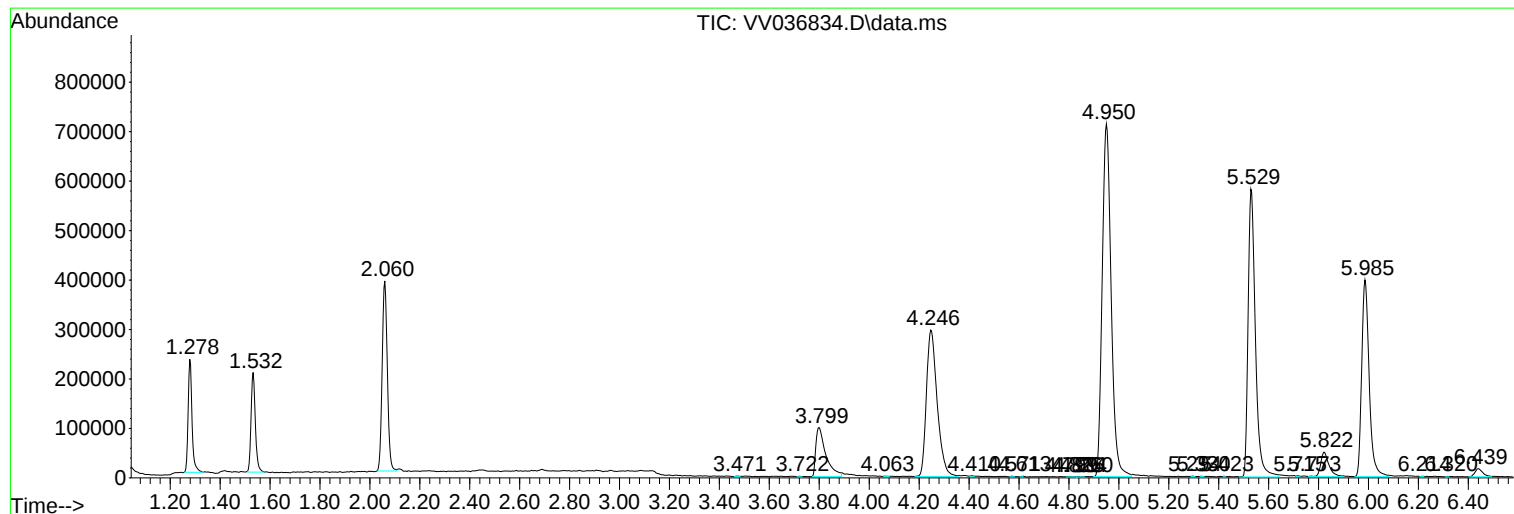

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036834.D
Acq On : 07 Aug 2024 12:53
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036834.D
Acq On : 07 Aug 2024 12:53
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------