

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036835.D
 Acq On : 07 Aug 2024 13:15
 Operator : SY/MD
 Sample : P3498-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.088	11	15	29	rVB	19301	22338	1.27%	0.169%
2	1.191	43	47	52	rBV	13092	12030	0.68%	0.091%
3	1.278	68	74	91	rVB	236077	255913	14.57%	1.935%
4	1.532	146	153	164	rVB	189527	222688	12.68%	1.684%
5	2.059	307	317	330	rBV	368726	537014	30.58%	4.061%
6	3.622	800	803	808	rBV4	734	773	0.04%	0.006%
7	3.657	811	814	817	rVV4	971	857	0.05%	0.006%
8	3.799	849	858	892	rBV	98515	295099	16.80%	2.232%
9	4.108	950	954	957	rBV6	775	848	0.05%	0.006%
10	4.246	978	997	1021	rBV	278525	706826	40.25%	5.345%
11	4.513	1078	1080	1085	rBV4	593	445	0.03%	0.003%
12	4.567	1090	1097	1108	rVB10	2059	4354	0.25%	0.033%
13	4.635	1114	1118	1120	rBV3	575	468	0.03%	0.004%
14	4.805	1167	1171	1173	rBV4	775	591	0.03%	0.004%
15	4.863	1185	1189	1195	rVB6	772	636	0.04%	0.005%
16	4.889	1195	1197	1200	rBV3	831	429	0.02%	0.003%
17	4.950	1201	1216	1250	rBV2	692020	1756285	100.00%	13.281%
18	5.400	1353	1356	1357	rBV3	1182	540	0.03%	0.004%
19	5.419	1360	1362	1368	rVB5	1320	954	0.05%	0.007%
20	5.493	1378	1385	1386	rBV5	1140	1125	0.06%	0.009%
21	5.529	1386	1396	1431	rVV	573581	1172561	66.76%	8.867%
22	5.825	1478	1488	1508	rBV4	22380	49534	2.82%	0.375%
23	5.985	1525	1538	1579	rBV	389822	824519	46.95%	6.235%
24	6.300	1634	1636	1641	rVB6	738	502	0.03%	0.004%
25	6.416	1669	1672	1676	rBV4	883	467	0.03%	0.004%
26	6.644	1739	1743	1746	rBV4	817	701	0.04%	0.005%
27	6.831	1798	1801	1803	rBV3	665	473	0.03%	0.004%
28	6.911	1814	1826	1856	rBV	222997	424612	24.18%	3.211%
29	7.239	1917	1928	1952	rBV	767312	1336347	76.09%	10.106%
30	7.503	2008	2010	2016	rBV6	719	514	0.03%	0.004%
31	7.551	2016	2025	2048	rBV	141650	261100	14.87%	1.975%
32	7.866	2117	2123	2126	rBV6	949	805	0.05%	0.006%
33	7.918	2135	2139	2142	rVB4	1065	682	0.04%	0.005%
34	7.979	2153	2158	2160	rBV4	631	539	0.03%	0.004%
35	8.027	2164	2173	2215	rBV2	282760	613137	34.91%	4.637%
36	8.525	2326	2328	2330	rBV3	698	462	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036835.D
 Acq On : 07 Aug 2024 13:15
 Operator : SY/MD
 Sample : P3498-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.603	2349	2352	2357	rVB4	671	617	0.04%	0.005%
38	8.779	2396	2407	2441	rBV	847878	1400268	79.73%	10.589%
39	9.017	2478	2481	2484	rBV4	769	545	0.03%	0.004%
40	9.140	2517	2519	2523	rBV4	761	492	0.03%	0.004%
41	9.172	2527	2529	2532	rVB2	817	494	0.03%	0.004%
42	9.191	2532	2535	2537	rBV3	1007	446	0.03%	0.003%
43	9.242	2545	2551	2557	rVB6	864	772	0.04%	0.006%
44	9.271	2557	2560	2565	rVB5	792	684	0.04%	0.005%
45	9.442	2610	2613	2616	rVB3	1004	649	0.04%	0.005%
46	9.458	2616	2618	2621	rBV	704	541	0.03%	0.004%
47	9.490	2626	2628	2634	rVB4	1118	874	0.05%	0.007%
48	9.516	2634	2636	2639	rVB3	945	510	0.03%	0.004%
49	9.532	2639	2641	2645	rBV3	850	635	0.04%	0.005%
50	9.789	2717	2721	2723	rBV4	776	657	0.04%	0.005%
51	9.853	2738	2741	2743	rBV4	602	439	0.02%	0.003%
52	9.918	2758	2761	2763	rBV3	669	512	0.03%	0.004%
53	9.959	2771	2774	2778	rVB4	900	554	0.03%	0.004%
54	10.040	2796	2799	2806	rVB7	677	703	0.04%	0.005%
55	10.149	2822	2833	2849	rBV	441651	694781	39.56%	5.254%
56	10.371	2899	2902	2905	rBV4	578	476	0.03%	0.004%
57	10.458	2924	2929	2931	rBV6	727	540	0.03%	0.004%
58	10.484	2931	2937	2938	rBV6	783	707	0.04%	0.005%
59	10.657	2986	2991	2994	rBV6	659	628	0.04%	0.005%
60	10.709	3005	3007	3010	rVB3	664	470	0.03%	0.004%
61	10.763	3021	3024	3027	rBV4	939	693	0.04%	0.005%
62	10.834	3042	3046	3049	rBV4	725	589	0.03%	0.004%
63	10.876	3056	3059	3065	rVB4	1616	1316	0.07%	0.010%
64	10.927	3070	3075	3079	rBV4	691	779	0.04%	0.006%
65	10.982	3089	3092	3097	rBV3	723	519	0.03%	0.004%
66	11.033	3104	3108	3113	rVB7	1156	1082	0.06%	0.008%
67	11.062	3113	3117	3119	rBV5	844	672	0.04%	0.005%
68	11.114	3127	3133	3134	rBV4	2241	1974	0.11%	0.015%
69	11.181	3142	3154	3184	rBV	829822	1334872	76.01%	10.095%
70	11.554	3258	3270	3297	rBV	763208	1224894	69.74%	9.263%
71	11.783	3338	3341	3344	rBV5	827	709	0.04%	0.005%
72	11.815	3348	3351	3353	rBV3	706	502	0.03%	0.004%
73	11.853	3360	3363	3365	rVB3	1108	547	0.03%	0.004%
74	12.233	3478	3481	3486	rBV5	733	690	0.04%	0.005%
75	12.291	3491	3499	3509	rBV8	10730	21374	1.22%	0.162%
76	12.590	3588	3592	3593	rBV2	1218	915	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036835.D
 Acq On : 07 Aug 2024 13:15
 Operator : SY/MD
 Sample : P3498-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.885	3681	3684	3687	rBV4	955	792	0.05%	0.006%
78	12.992	3714	3717	3719	rBV3	582	431	0.02%	0.003%
79	13.040	3730	3732	3734	rVB2	1009	473	0.03%	0.004%
80	13.053	3734	3736	3740	rBV4	567	455	0.03%	0.003%
81	13.136	3759	3762	3765	rBV4	924	613	0.03%	0.005%
82	13.184	3773	3777	3779	rBV4	543	423	0.02%	0.003%
83	13.303	3811	3814	3817	rBV4	545	455	0.03%	0.003%
84	13.361	3829	3832	3835	rVB2	844	475	0.03%	0.004%
85	13.409	3843	3847	3848	rBV2	1179	956	0.05%	0.007%
86	13.551	3888	3891	3895	rBV4	795	718	0.04%	0.005%
87	13.635	3911	3917	3919	rBV6	868	925	0.05%	0.007%
88	13.692	3932	3935	3940	rVB4	1628	1589	0.09%	0.012%
89	13.763	3953	3957	3958	rBV4	796	540	0.03%	0.004%
90	13.863	3985	3988	3993	rBV3	850	653	0.04%	0.005%
91	13.885	3993	3995	3999	rBV4	541	421	0.02%	0.003%
92	13.940	4008	4012	4013	rBV3	720	514	0.03%	0.004%
93	13.966	4017	4020	4026	rBV6	1218	1417	0.08%	0.011%
94	14.136	4069	4073	4075	rBV4	883	701	0.04%	0.005%
95	14.168	4079	4083	4088	rVB4	650	727	0.04%	0.005%
96	14.393	4150	4153	4157	rBV5	725	548	0.03%	0.004%
97	14.467	4172	4176	4178	rBV4	1031	849	0.05%	0.006%
98	14.557	4202	4204	4207	rBV	877	518	0.03%	0.004%
99	15.155	4387	4390	4393	rBV3	865	441	0.03%	0.003%
100	15.175	4393	4396	4399	rBV3	936	671	0.04%	0.005%




Sum of corrected areas: 13223594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036835.D
Acq On : 07 Aug 2024 13:15
Operator : SY/MD
Sample : P3498-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

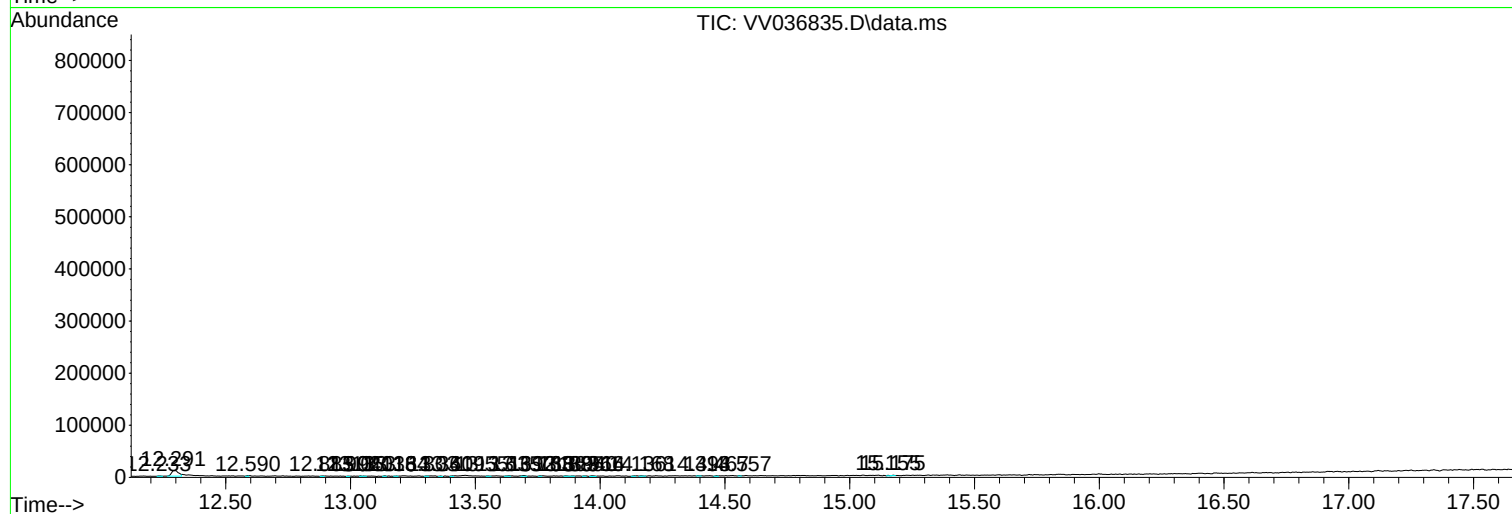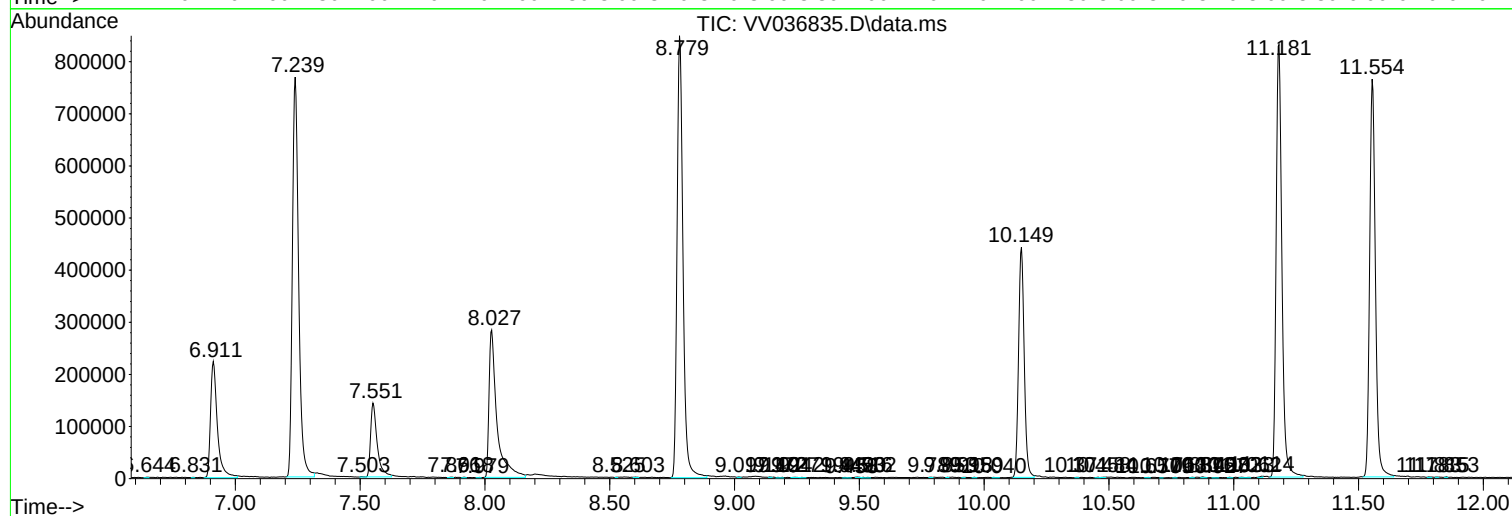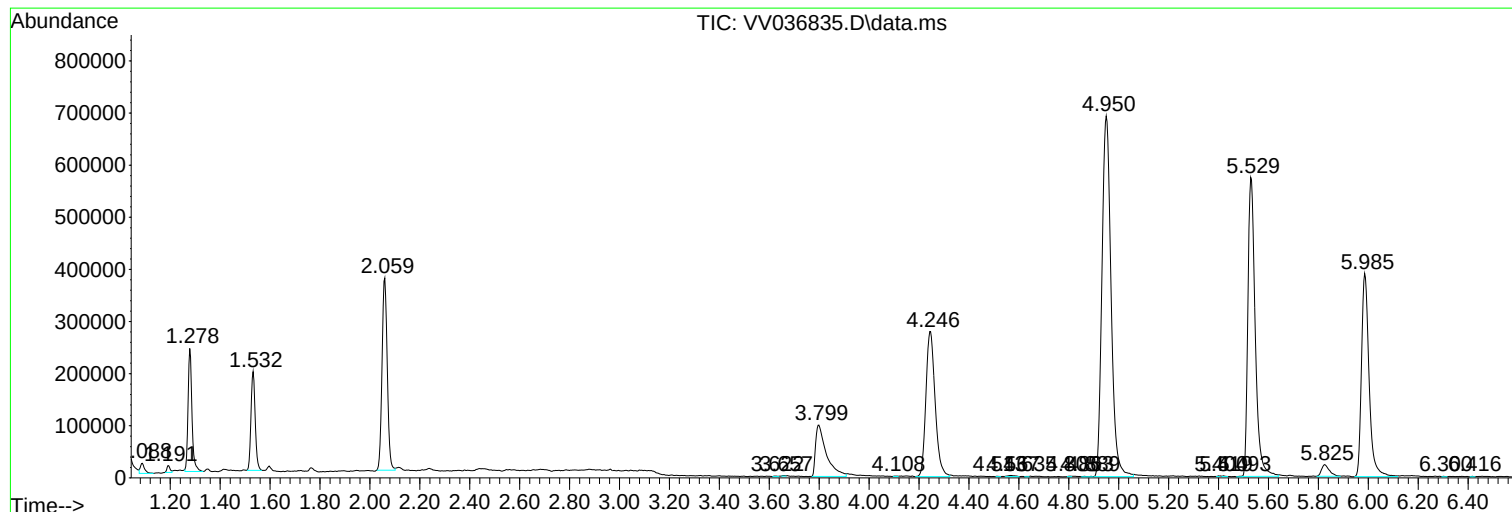

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036835.D
Acq On : 07 Aug 2024 13:15
Operator : SY/MD
Sample : P3498-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036835.D
Acq On : 07 Aug 2024 13:15
Operator : SY/MD
Sample : P3498-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc