

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036837.D
 Acq On : 07 Aug 2024 14:49
 Operator : SY/MD
 Sample : VIBLK326
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	152431	160964	10.45%	1.454%
2	1.532	146	153	166	rVB	158543	187621	12.18%	1.695%
3	2.056	307	316	331	rBV	260151	378769	24.60%	3.421%
4	3.449	747	749	752	rVB4	1184	548	0.04%	0.005%
5	3.715	830	832	834	rVB2	982	434	0.03%	0.004%
6	3.789	847	855	897	rBV	103475	316896	20.58%	2.862%
7	4.239	979	995	1026	rBV	246759	627870	40.77%	5.671%
8	4.500	1072	1076	1084	rVB8	1097	1443	0.09%	0.013%
9	4.539	1084	1088	1091	rBV4	1022	1127	0.07%	0.010%
10	4.645	1118	1121	1125	rBV3	748	559	0.04%	0.005%
11	4.754	1152	1155	1158	rBV2	799	686	0.04%	0.006%
12	4.796	1165	1168	1172	rBV2	699	572	0.04%	0.005%
13	4.815	1172	1174	1178	rVB4	874	540	0.04%	0.005%
14	4.947	1196	1215	1249	rBV2	602330	1539998	100.00%	13.910%
15	5.297	1319	1324	1327	rBV5	756	808	0.05%	0.007%
16	5.458	1371	1374	1377	rVB3	752	453	0.03%	0.004%
17	5.529	1385	1396	1432	rBV	435694	897861	58.30%	8.110%
18	5.821	1476	1487	1508	rBV2	22525	51727	3.36%	0.467%
19	5.982	1524	1537	1565	rBV	351482	733572	47.63%	6.626%
20	6.140	1584	1586	1589	rVB2	1073	490	0.03%	0.004%
21	6.757	1776	1778	1784	rVB4	653	637	0.04%	0.006%
22	6.796	1784	1790	1795	rBV6	586	639	0.04%	0.006%
23	6.847	1802	1806	1810	rBV3	731	537	0.03%	0.005%
24	6.908	1814	1825	1850	rBV	190897	368110	23.90%	3.325%
25	7.085	1878	1880	1887	rVB6	813	604	0.04%	0.005%
26	7.236	1917	1927	1952	rBV	595346	1052770	68.36%	9.509%
27	7.551	2016	2025	2050	rBV	126841	235900	15.32%	2.131%
28	7.696	2068	2070	2074	rVB4	1321	916	0.06%	0.008%
29	7.947	2142	2148	2155	rBV6	779	940	0.06%	0.008%
30	7.982	2155	2159	2163	rBV5	639	544	0.04%	0.005%
31	8.024	2163	2172	2216	rBV2	275624	606031	39.35%	5.474%
32	8.638	2359	2363	2364	rBV2	791	453	0.03%	0.004%
33	8.648	2364	2366	2369	rVV3	877	574	0.04%	0.005%
34	8.715	2385	2387	2389	rBV2	739	445	0.03%	0.004%
35	8.780	2395	2407	2438	rBV	637210	1058037	68.70%	9.557%
36	9.050	2487	2491	2494	rBV5	839	634	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036837.D
 Acq On : 07 Aug 2024 14:49
 Operator : SY/MD
 Sample : VIBLK326
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.085	2498	2502	2508	rVB6	946	923	0.06%	0.008%
38	9.111	2508	2510	2515	rVB5	843	613	0.04%	0.006%
39	9.175	2527	2530	2533	rBV3	929	799	0.05%	0.007%
40	9.223	2542	2545	2547	rBV2	729	578	0.04%	0.005%
41	9.236	2547	2549	2553	rVB3	968	552	0.04%	0.005%
42	9.271	2553	2560	2561	rBV5	842	834	0.05%	0.008%
43	9.342	2578	2582	2588	rBV6	822	802	0.05%	0.007%
44	9.371	2588	2591	2595	rVB4	1066	715	0.05%	0.006%
45	9.394	2595	2598	2600	rBV3	997	643	0.04%	0.006%
46	9.580	2653	2656	2662	rBV5	777	748	0.05%	0.007%
47	9.619	2664	2668	2670	rBV3	592	431	0.03%	0.004%
48	9.660	2676	2681	2683	rBV6	618	579	0.04%	0.005%
49	9.773	2711	2716	2719	rBV4	600	494	0.03%	0.004%
50	10.053	2799	2803	2804	rBV3	795	556	0.04%	0.005%
51	10.062	2804	2806	2810	rVB3	952	701	0.05%	0.006%
52	10.146	2819	2832	2854	rBV	419559	677919	44.02%	6.123%
53	10.320	2885	2886	2890	rVB2	912	552	0.04%	0.005%
54	10.458	2923	2929	2931	rBV4	439	441	0.03%	0.004%
55	10.587	2965	2969	2971	rBV2	698	483	0.03%	0.004%
56	10.638	2982	2985	2987	rBV2	788	571	0.04%	0.005%
57	10.709	3004	3007	3008	rBV3	704	423	0.03%	0.004%
58	10.812	3035	3039	3042	rBV7	738	629	0.04%	0.006%
59	10.857	3051	3053	3055	rBV3	881	568	0.04%	0.005%
60	10.937	3072	3078	3082	rBV4	920	1037	0.07%	0.009%
61	11.127	3132	3137	3140	rBV6	1403	1380	0.09%	0.012%
62	11.181	3143	3154	3183	rBV	618540	989338	64.24%	8.936%
63	11.477	3242	3246	3247	rBV3	986	696	0.05%	0.006%
64	11.554	3258	3270	3297	rBV	605076	997532	64.77%	9.010%
65	11.728	3319	3324	3331	rVB6	3987	4737	0.31%	0.043%
66	11.783	3337	3341	3346	rVB7	1103	1138	0.07%	0.010%
67	11.805	3346	3348	3350	rBV2	641	434	0.03%	0.004%
68	11.931	3380	3387	3388	rBV5	835	956	0.06%	0.009%
69	11.959	3389	3396	3402	rVB4	3401	5289	0.34%	0.048%
70	12.056	3421	3426	3430	rBV7	1744	1661	0.11%	0.015%
71	12.091	3430	3437	3438	rBV5	1761	1585	0.10%	0.014%
72	12.168	3457	3461	3464	rBV4	1151	1134	0.07%	0.010%
73	12.249	3483	3486	3488	rBV3	905	501	0.03%	0.005%
74	12.355	3513	3519	3527	rVV6	4311	6342	0.41%	0.057%
75	12.403	3527	3534	3545	rVV4	6041	8970	0.58%	0.081%
76	12.487	3555	3560	3562	rBV3	4380	4161	0.27%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036837.D
 Acq On : 07 Aug 2024 14:49
 Operator : SY/MD
 Sample : VIBLK326
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.551	3577	3580	3588	rVB4	4048	4503	0.29%	0.041%
78	12.606	3591	3597	3604	rVB7	2058	2946	0.19%	0.027%
79	12.664	3609	3615	3628	rVB5	9654	15129	0.98%	0.137%
80	12.738	3628	3638	3646	rBV4	4360	8211	0.53%	0.074%
81	12.789	3649	3654	3657	rVV5	3154	3465	0.23%	0.031%
82	12.821	3658	3664	3680	rVB5	9650	19086	1.24%	0.172%
83	12.940	3694	3701	3708	rBV3	6693	9777	0.63%	0.088%
84	13.094	3746	3749	3751	rBV3	1097	736	0.05%	0.007%
85	13.207	3774	3784	3790	rBV10	5893	9643	0.63%	0.087%
86	13.274	3803	3805	3810	rVB5	1038	819	0.05%	0.007%
87	13.303	3810	3814	3815	rBV3	558	502	0.03%	0.005%
88	13.445	3851	3858	3867	rBV2	10269	18028	1.17%	0.163%
89	13.541	3882	3888	3891	rBV7	1510	1806	0.12%	0.016%
90	13.557	3891	3893	3894	rBV2	1055	467	0.03%	0.004%
91	13.625	3911	3914	3915	rBV3	721	519	0.03%	0.005%
92	13.837	3973	3980	3987	rBV3	7130	10369	0.67%	0.094%
93	14.024	4035	4038	4039	rBV3	974	610	0.04%	0.006%
94	14.088	4051	4058	4059	rBV4	855	917	0.06%	0.008%
95	14.313	4125	4128	4130	rBV3	1381	946	0.06%	0.009%
96	14.506	4185	4188	4189	rBV2	998	504	0.03%	0.005%
97	14.577	4208	4210	4211	rBV2	1205	554	0.04%	0.005%
98	14.638	4227	4229	4232	rVB4	930	500	0.03%	0.005%
99	14.782	4267	4274	4283	rVB4	8270	10935	0.71%	0.099%
100	14.824	4285	4287	4292	rBV5	996	812	0.05%	0.007%




Sum of corrected areas: 11070938

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036837.D
Acq On : 07 Aug 2024 14:49
Operator : SY/MD
Sample : VIBLK326
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

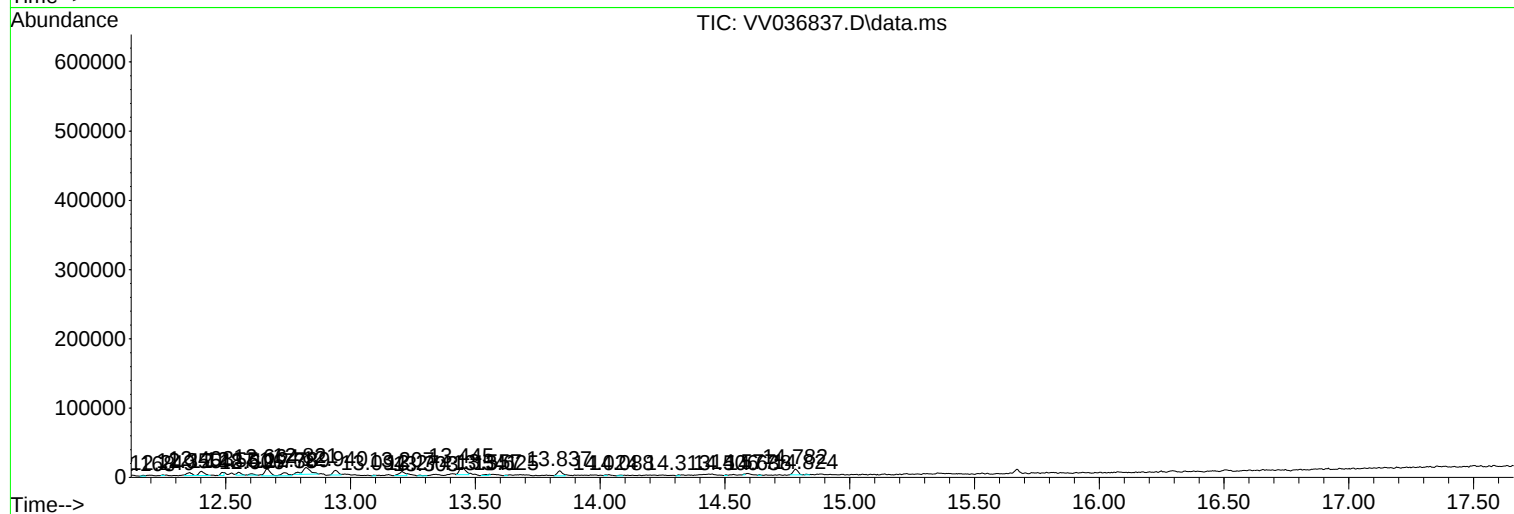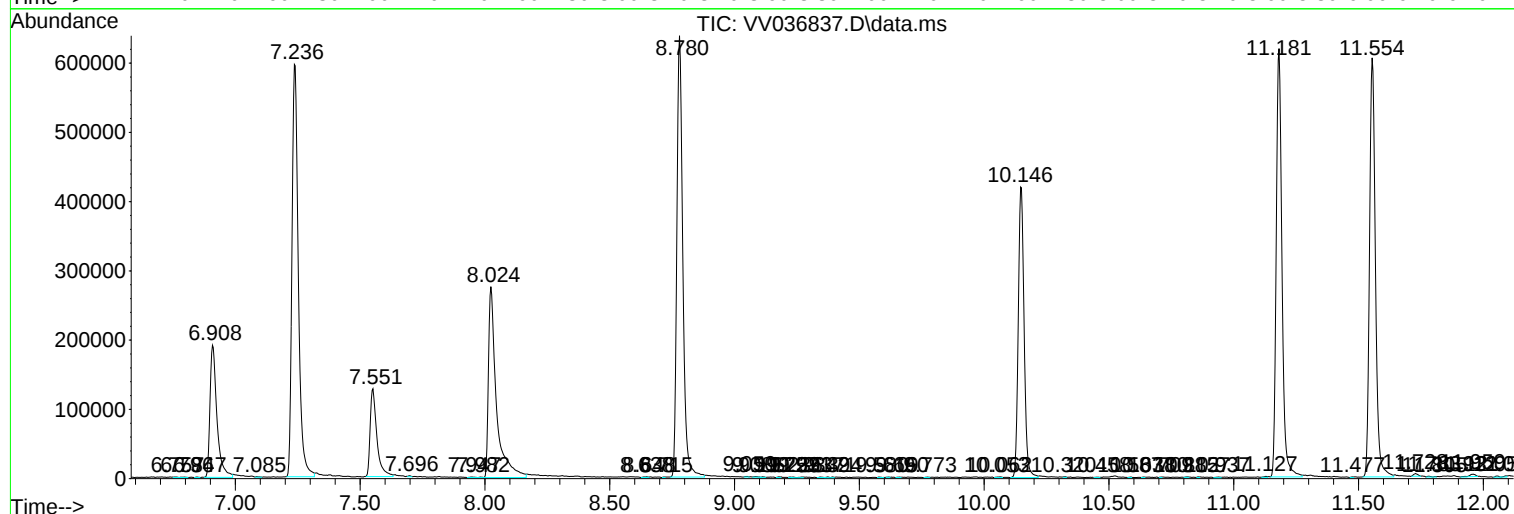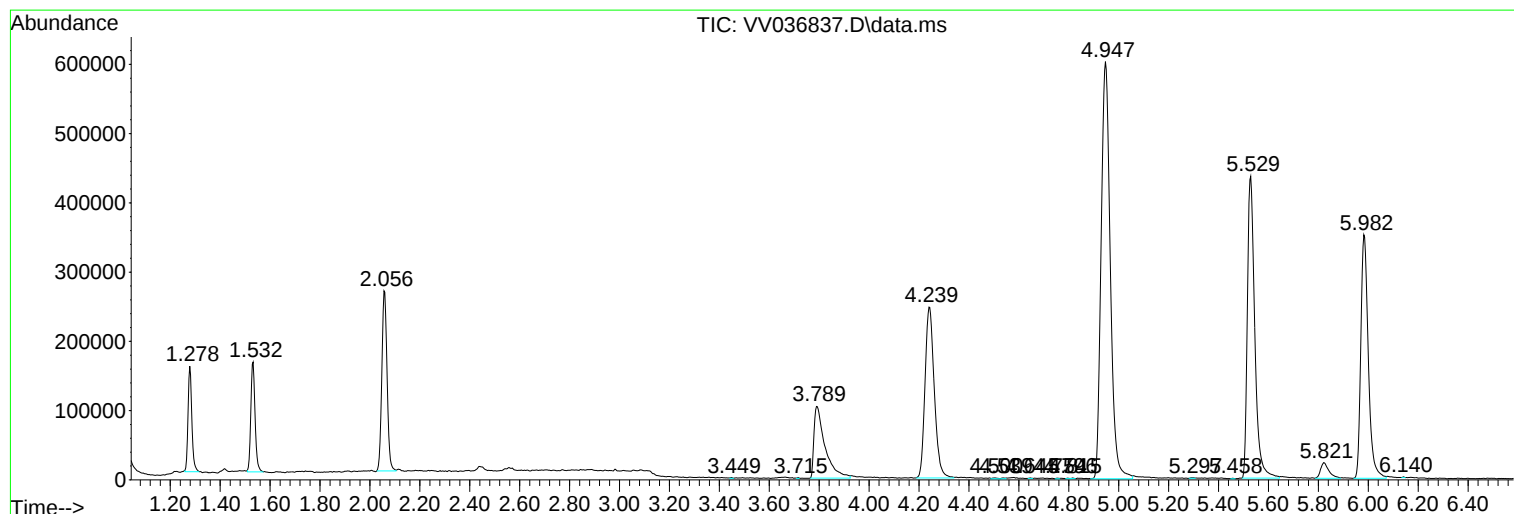

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036837.D
Acq On : 07 Aug 2024 14:49
Operator : SY/MD
Sample : VIBLK326
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036837.D
Acq On : 07 Aug 2024 14:49
Operator : SY/MD
Sample : VIBLK326
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------