

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036838.D
 Acq On : 07 Aug 2024 15:32
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036838.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	235570	250534	13.98%	1.850%
2	1.532	145	153	167	rVB	200254	241539	13.48%	1.784%
3	2.056	307	316	331	rVB	391538	557417	31.11%	4.116%
4	3.606	794	798	800	rBV5	743	620	0.03%	0.005%
5	3.677	817	820	823	rBV4	949	779	0.04%	0.006%
6	3.793	847	856	894	rBV	99577	289829	16.17%	2.140%
7	3.998	917	920	922	rBV4	1013	632	0.04%	0.005%
8	4.085	944	947	950	rBV4	828	705	0.04%	0.005%
9	4.240	979	995	1025	rBV	280559	719122	40.13%	5.310%
10	4.622	1111	1114	1115	rBV3	1014	571	0.03%	0.004%
11	4.735	1148	1149	1157	rVB4	741	571	0.03%	0.004%
12	4.770	1157	1160	1163	rBV2	746	482	0.03%	0.004%
13	4.809	1166	1172	1175	rBV5	690	738	0.04%	0.005%
14	4.947	1197	1215	1250	rBV2	705558	1791883	100.00%	13.231%
15	5.407	1356	1358	1362	rVB4	915	639	0.04%	0.005%
16	5.436	1362	1367	1369	rBV3	744	672	0.04%	0.005%
17	5.478	1375	1380	1382	rBV4	1368	1064	0.06%	0.008%
18	5.526	1384	1395	1432	rVV	579987	1178573	65.77%	8.703%
19	5.822	1476	1487	1506	rBV3	24761	58421	3.26%	0.431%
20	5.982	1522	1537	1567	rBV	402216	833348	46.51%	6.154%
21	6.259	1620	1623	1627	rVB6	945	596	0.03%	0.004%
22	6.314	1637	1640	1643	rBV4	927	616	0.03%	0.005%
23	6.477	1688	1691	1693	rBV4	1174	659	0.04%	0.005%
24	6.513	1699	1702	1703	rBV2	901	422	0.02%	0.003%
25	6.587	1720	1725	1726	rBV3	578	466	0.03%	0.003%
26	6.635	1734	1740	1743	rBV3	1045	1040	0.06%	0.008%
27	6.654	1743	1746	1749	rVB3	795	516	0.03%	0.004%
28	6.680	1749	1754	1757	rBV5	1000	856	0.05%	0.006%
29	6.908	1815	1825	1855	rBV	228671	436215	24.34%	3.221%
30	7.146	1897	1899	1901	rVB3	833	431	0.02%	0.003%
31	7.166	1901	1905	1908	rBV5	909	885	0.05%	0.007%
32	7.236	1916	1927	1954	rBV	775136	1382818	77.17%	10.211%
33	7.548	2015	2024	2055	rBV	147568	276272	15.42%	2.040%
34	7.899	2128	2133	2137	rBV5	1059	1121	0.06%	0.008%
35	8.024	2163	2172	2212	rBV2	266634	584771	32.63%	4.318%
36	8.307	2256	2260	2262	rBV5	1015	703	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036838.D
 Acq On : 07 Aug 2024 15:32
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.516	2322	2325	2329	rBV4	657	625	0.03%	0.005%
38	8.693	2378	2380	2383	rVB4	755	420	0.02%	0.003%
39	8.780	2394	2407	2438	rBV	856661	1431415	79.88%	10.570%
40	9.191	2533	2535	2541	rVB4	937	681	0.04%	0.005%
41	9.284	2559	2564	2569	rBV4	918	903	0.05%	0.007%
42	9.310	2569	2572	2575	rBV4	526	402	0.02%	0.003%
43	9.391	2595	2597	2600	rVB3	822	442	0.02%	0.003%
44	9.413	2600	2604	2607	rBV3	619	557	0.03%	0.004%
45	9.471	2619	2622	2625	rBV3	561	493	0.03%	0.004%
46	9.529	2638	2640	2643	rBV3	729	485	0.03%	0.004%
47	9.583	2655	2657	2663	rVB5	963	688	0.04%	0.005%
48	9.635	2670	2673	2678	rVB6	449	458	0.03%	0.003%
49	9.670	2678	2684	2687	rBV6	748	865	0.05%	0.006%
50	9.722	2690	2700	2701	rBV7	770	1052	0.06%	0.008%
51	9.818	2727	2730	2735	rBV6	901	942	0.05%	0.007%
52	9.899	2751	2755	2758	rBV5	677	567	0.03%	0.004%
53	10.001	2783	2787	2789	rBV4	545	510	0.03%	0.004%
54	10.069	2803	2808	2809	rBV3	601	462	0.03%	0.003%
55	10.146	2821	2832	2854	rBV	437941	690342	38.53%	5.098%
56	10.362	2897	2899	2902	rVB3	785	513	0.03%	0.004%
57	10.391	2906	2908	2911	rVB2	869	433	0.02%	0.003%
58	10.442	2918	2924	2928	rBV7	966	1258	0.07%	0.009%
59	10.516	2942	2947	2949	rBV3	949	667	0.04%	0.005%
60	10.715	3004	3009	3014	rVB5	801	822	0.05%	0.006%
61	10.744	3014	3018	3020	rBV4	734	600	0.03%	0.004%
62	10.770	3022	3026	3029	rVB3	702	634	0.04%	0.005%
63	10.792	3029	3033	3036	rBV6	983	844	0.05%	0.006%
64	10.944	3076	3080	3081	rBV2	801	524	0.03%	0.004%
65	11.014	3100	3102	3106	rVV3	542	415	0.02%	0.003%
66	11.053	3109	3114	3117	rBV4	896	945	0.05%	0.007%
67	11.127	3134	3137	3140	rBV4	981	825	0.05%	0.006%
68	11.178	3142	3153	3182	rBV	906359	1437098	80.20%	10.612%
69	11.445	3233	3236	3239	rVB5	835	622	0.03%	0.005%
70	11.554	3258	3270	3301	rBV	833530	1314376	73.35%	9.706%
71	11.715	3318	3320	3322	rBV3	1073	635	0.04%	0.005%
72	11.950	3390	3393	3396	rBV5	830	513	0.03%	0.004%
73	12.095	3433	3438	3441	rBV4	655	517	0.03%	0.004%
74	12.156	3454	3457	3461	rVB3	580	411	0.02%	0.003%
75	12.252	3484	3487	3491	rVV3	612	519	0.03%	0.004%
76	12.397	3529	3532	3534	rBV4	916	661	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036838.D
 Acq On : 07 Aug 2024 15:32
 Operator : SY/MD
 Sample : P3437-19
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.493	3554	3562	3567	rBV6	1254	1903	0.11%	0.014%
78	12.519	3567	3570	3573	rVB4	885	667	0.04%	0.005%
79	12.538	3573	3576	3578	rBV2	656	497	0.03%	0.004%
80	12.599	3591	3595	3598	rBV4	1270	1182	0.07%	0.009%
81	12.667	3613	3616	3623	rBV5	1637	2255	0.13%	0.017%
82	12.828	3661	3666	3675	rVB7	2517	3637	0.20%	0.027%
83	12.940	3696	3701	3702	rBV3	1678	1335	0.07%	0.010%
84	13.037	3727	3731	3736	rBV5	958	892	0.05%	0.007%
85	13.114	3750	3755	3760	rBV7	899	985	0.05%	0.007%
86	13.207	3779	3784	3788	rBV7	1752	1604	0.09%	0.012%
87	13.252	3795	3798	3804	rVB5	751	572	0.03%	0.004%
88	13.300	3810	3813	3818	rBV3	933	780	0.04%	0.006%
89	13.323	3818	3820	3823	rVV4	605	450	0.03%	0.003%
90	13.397	3839	3843	3845	rBV4	542	526	0.03%	0.004%
91	13.455	3855	3861	3874	rVB6	2947	5000	0.28%	0.037%
92	13.751	3950	3953	3957	rVB4	527	420	0.02%	0.003%
93	13.841	3975	3981	3987	rVB7	2128	2685	0.15%	0.020%
94	13.898	3996	3999	4002	rVB4	706	507	0.03%	0.004%
95	14.069	4050	4052	4056	rVB4	837	522	0.03%	0.004%
96	14.098	4058	4061	4066	rVB4	713	519	0.03%	0.004%
97	14.323	4126	4131	4133	rVV2	875	778	0.04%	0.006%
98	14.448	4165	4170	4172	rBV5	975	899	0.05%	0.007%
99	14.660	4233	4236	4238	rBV4	897	620	0.03%	0.005%
100	14.873	4300	4302	4304	rBV2	973	668	0.04%	0.005%




Sum of corrected areas: 13542570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036838.D
Acq On : 07 Aug 2024 15:32
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

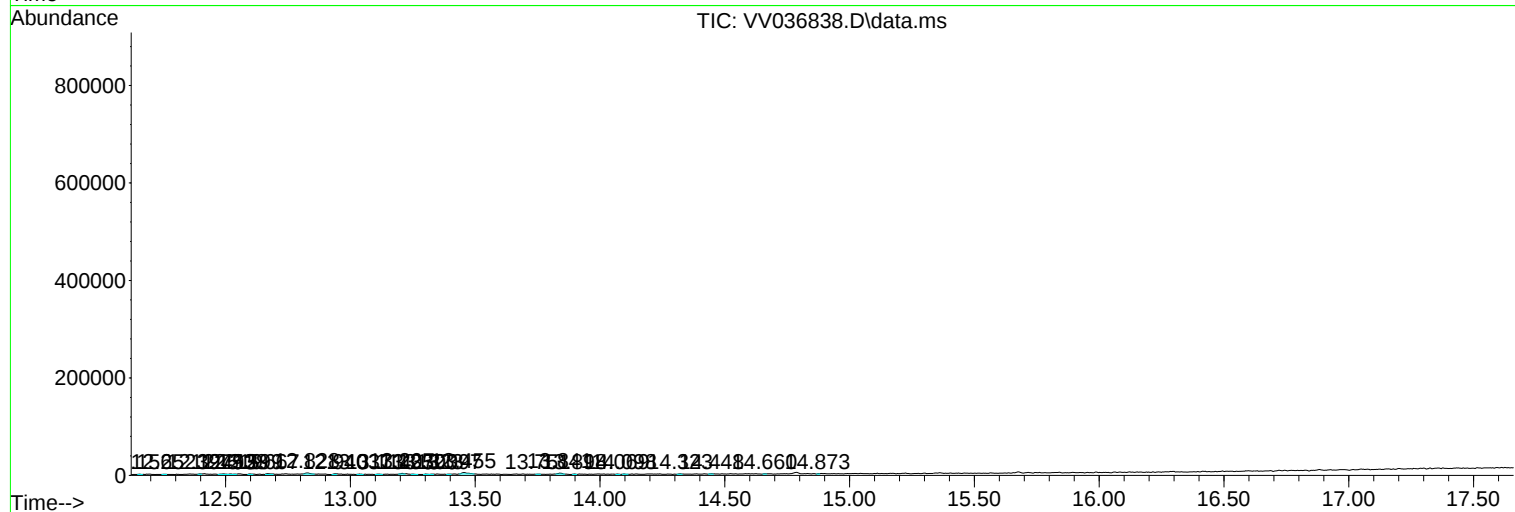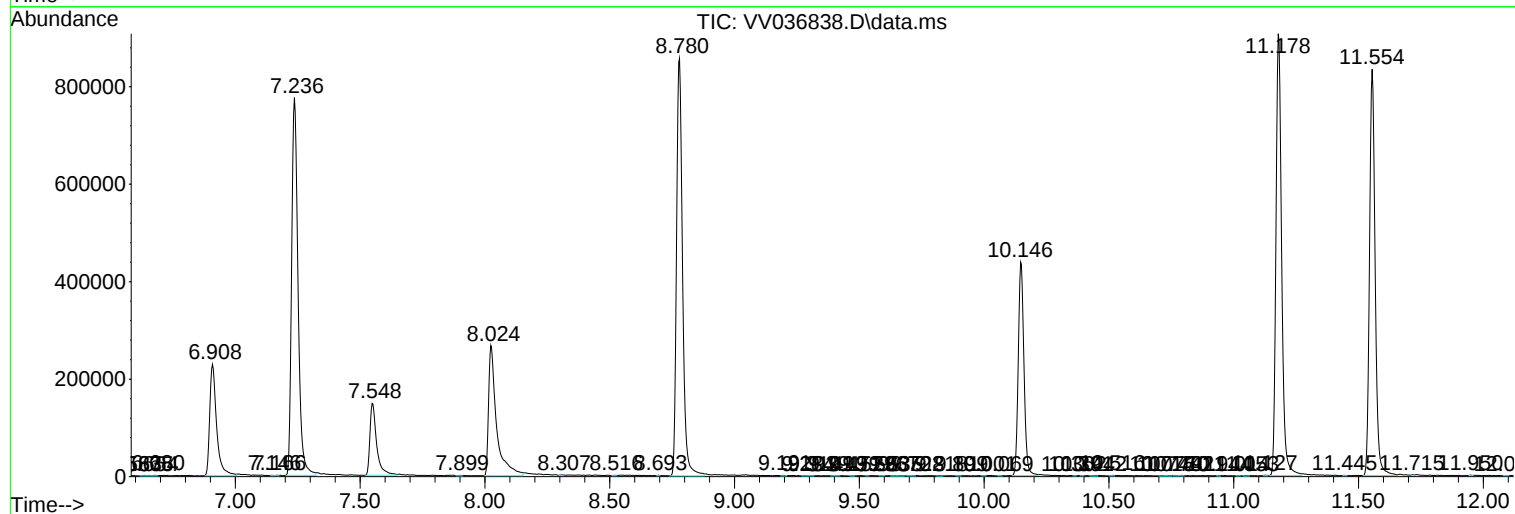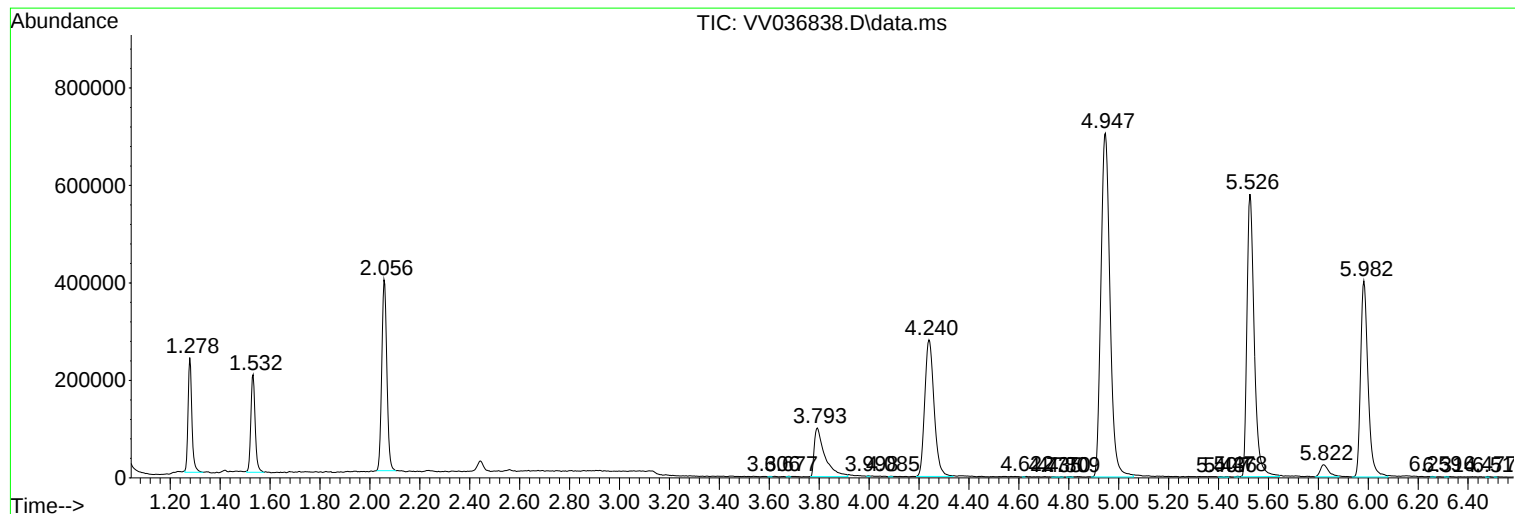

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036838.D
Acq On : 07 Aug 2024 15:32
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036838.D
Acq On : 07 Aug 2024 15:32
Operator : SY/MD
Sample : P3437-19
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc