

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036839.D
 Acq On : 07 Aug 2024 15:54
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036839.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	223845	240372	13.75%	1.944%
2	1.532	145	153	169	rVB	201344	235766	13.49%	1.906%
3	2.060	307	317	329	rBV	374292	534638	30.58%	4.323%
4	3.400	732	734	739	rBV5	834	467	0.03%	0.004%
5	3.709	825	830	831	rBV4	644	453	0.03%	0.004%
6	3.796	849	857	893	rBV	100632	281113	16.08%	2.273%
7	4.246	980	997	1032	rBV3	294232	869710	49.75%	7.033%
8	4.526	1080	1084	1089	rBV6	547	624	0.04%	0.005%
9	4.667	1124	1128	1129	rBV4	885	544	0.03%	0.004%
10	4.738	1147	1150	1156	rBV5	773	1012	0.06%	0.008%
11	4.818	1171	1175	1179	rVB4	744	660	0.04%	0.005%
12	4.950	1201	1216	1251	rBV2	693615	1748235	100.00%	14.137%
13	5.323	1328	1332	1334	rBV5	1306	828	0.05%	0.007%
14	5.381	1347	1350	1353	rVB4	717	606	0.03%	0.005%
15	5.494	1382	1385	1386	rBV3	920	444	0.03%	0.004%
16	5.532	1386	1397	1429	rVV	397539	821332	46.98%	6.642%
17	5.821	1476	1487	1507	rBV2	35811	80983	4.63%	0.655%
18	5.940	1520	1524	1525	rBV4	893	515	0.03%	0.004%
19	5.985	1525	1538	1569	rVV	392216	811453	46.42%	6.562%
20	6.387	1659	1663	1667	rBV4	712	561	0.03%	0.005%
21	6.439	1667	1679	1696	rBV2	16121	37467	2.14%	0.303%
22	6.654	1742	1746	1747	rBV4	903	621	0.04%	0.005%
23	6.715	1760	1765	1767	rBV4	594	621	0.04%	0.005%
24	6.821	1796	1798	1805	rVB6	837	701	0.04%	0.006%
25	6.911	1815	1826	1854	rBV	226888	428385	24.50%	3.464%
26	7.239	1916	1928	1954	rBV	763742	1360867	77.84%	11.004%
27	7.551	2016	2025	2052	rBV	145787	271143	15.51%	2.193%
28	7.789	2096	2099	2101	rBV2	1436	854	0.05%	0.007%
29	7.870	2121	2124	2127	rBV4	536	506	0.03%	0.004%
30	7.911	2135	2137	2141	rVB5	1364	893	0.05%	0.007%
31	7.934	2141	2144	2146	rBV3	817	614	0.04%	0.005%
32	8.027	2164	2173	2214	rBV2	266914	603761	34.54%	4.882%
33	8.522	2323	2327	2331	rBV3	548	520	0.03%	0.004%
34	8.545	2331	2334	2336	rBV3	895	628	0.04%	0.005%
35	8.670	2366	2373	2375	rBV7	556	603	0.03%	0.005%
36	8.780	2396	2407	2434	rBV	601760	1006593	57.58%	8.140%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036839.D
 Acq On : 07 Aug 2024 15:54
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.140	2516	2519	2524	rVB6	747	596	0.03%	0.005%
38	9.226	2543	2546	2549	rVB2	678	448	0.03%	0.004%
39	9.262	2555	2557	2560	rBV3	619	446	0.03%	0.004%
40	9.278	2560	2562	2566	rVB3	786	502	0.03%	0.004%
41	9.300	2566	2569	2572	rVB3	1041	753	0.04%	0.006%
42	9.320	2572	2575	2578	rBV4	878	564	0.03%	0.005%
43	9.419	2602	2606	2608	rBV3	723	496	0.03%	0.004%
44	9.471	2618	2622	2624	rBV2	788	526	0.03%	0.004%
45	9.490	2624	2628	2632	rBV5	1539	1488	0.09%	0.012%
46	9.522	2633	2638	2641	rBV6	1302	1065	0.06%	0.009%
47	9.574	2650	2654	2658	rVV5	612	483	0.03%	0.004%
48	9.657	2678	2680	2683	rVB4	902	535	0.03%	0.004%
49	9.673	2683	2685	2687	rBV3	794	452	0.03%	0.004%
50	9.796	2719	2723	2727	rBV5	621	518	0.03%	0.004%
51	9.837	2727	2736	2739	rBV6	1033	1320	0.08%	0.011%
52	9.927	2762	2764	2769	rBV3	575	578	0.03%	0.005%
53	10.030	2791	2796	2799	rBV3	696	597	0.03%	0.005%
54	10.091	2810	2815	2819	rBV6	749	842	0.05%	0.007%
55	10.149	2819	2833	2857	rBV	414886	672539	38.47%	5.438%
56	10.300	2877	2880	2882	rBV3	1008	461	0.03%	0.004%
57	10.599	2969	2973	2976	rBV4	592	447	0.03%	0.004%
58	10.667	2992	2994	2998	rVB3	780	622	0.04%	0.005%
59	10.699	2998	3004	3006	rBV4	1274	1193	0.07%	0.010%
60	11.085	3122	3124	3129	rVB3	936	578	0.03%	0.005%
61	11.111	3129	3132	3134	rBV3	1082	742	0.04%	0.006%
62	11.127	3134	3137	3141	rVB5	1218	1063	0.06%	0.009%
63	11.181	3143	3154	3181	rBV	624275	1009170	57.73%	8.160%
64	11.464	3240	3242	3246	rVB2	992	495	0.03%	0.004%
65	11.554	3258	3270	3298	rBV	805749	1293741	74.00%	10.462%
66	11.722	3319	3322	3324	rBV4	922	691	0.04%	0.006%
67	11.815	3347	3351	3353	rBV4	641	488	0.03%	0.004%
68	12.069	3423	3430	3432	rBV5	724	654	0.04%	0.005%
69	12.210	3471	3474	3478	rBV3	587	463	0.03%	0.004%
70	12.310	3499	3505	3506	rBV4	1124	806	0.05%	0.007%
71	12.400	3527	3533	3537	rBV7	1440	1899	0.11%	0.015%
72	12.525	3569	3572	3576	rBV4	570	441	0.03%	0.004%
73	12.673	3613	3618	3621	rVB6	1445	1262	0.07%	0.010%
74	12.693	3621	3624	3627	rBV3	482	443	0.03%	0.004%
75	12.731	3634	3636	3640	rVB4	1069	588	0.03%	0.005%
76	12.866	3676	3678	3682	rVB3	1101	588	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
 Data File : VV036839.D
 Acq On : 07 Aug 2024 15:54
 Operator : SY/MD
 Sample : P3498-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08M1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.940	3696	3701	3703	rBV5	768	711	0.04%	0.006%
78	12.988	3713	3716	3719	rVB5	791	500	0.03%	0.004%
79	13.030	3722	3729	3733	rBV7	1189	1412	0.08%	0.011%
80	13.056	3735	3737	3742	rVB5	686	446	0.03%	0.004%
81	13.130	3757	3760	3765	rBV5	690	491	0.03%	0.004%
82	13.162	3765	3770	3773	rBV5	634	478	0.03%	0.004%
83	13.278	3804	3806	3812	rVB4	669	635	0.04%	0.005%
84	13.368	3830	3834	3836	rBV4	500	445	0.03%	0.004%
85	13.448	3852	3859	3862	rBV4	2512	2703	0.15%	0.022%
86	13.619	3906	3912	3913	rBV4	776	678	0.04%	0.005%
87	13.660	3921	3925	3926	rBV3	828	558	0.03%	0.005%
88	13.805	3968	3970	3973	rVB3	718	474	0.03%	0.004%
89	13.840	3973	3981	3985	rBV8	1779	2310	0.13%	0.019%
90	13.979	4019	4024	4029	rBV5	1022	1300	0.07%	0.011%
91	14.088	4056	4058	4061	rBV4	564	448	0.03%	0.004%
92	14.120	4066	4068	4071	rBV2	856	508	0.03%	0.004%
93	14.143	4071	4075	4078	rBV3	945	553	0.03%	0.004%
94	14.619	4219	4223	4225	rBV3	736	551	0.03%	0.004%
95	14.773	4266	4271	4272	rBV4	1327	1065	0.06%	0.009%
96	14.818	4282	4285	4287	rBV4	855	457	0.03%	0.004%
97	14.831	4287	4289	4294	rVB6	939	625	0.04%	0.005%
98	15.123	4377	4380	4382	rBV4	894	714	0.04%	0.006%
99	15.287	4429	4431	4433	rBV3	949	581	0.03%	0.005%
100	15.631	4536	4538	4544	rBV5	1252	1273	0.07%	0.010%


Sum of corrected areas: 12366592

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036839.D
Acq On : 07 Aug 2024 15:54
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

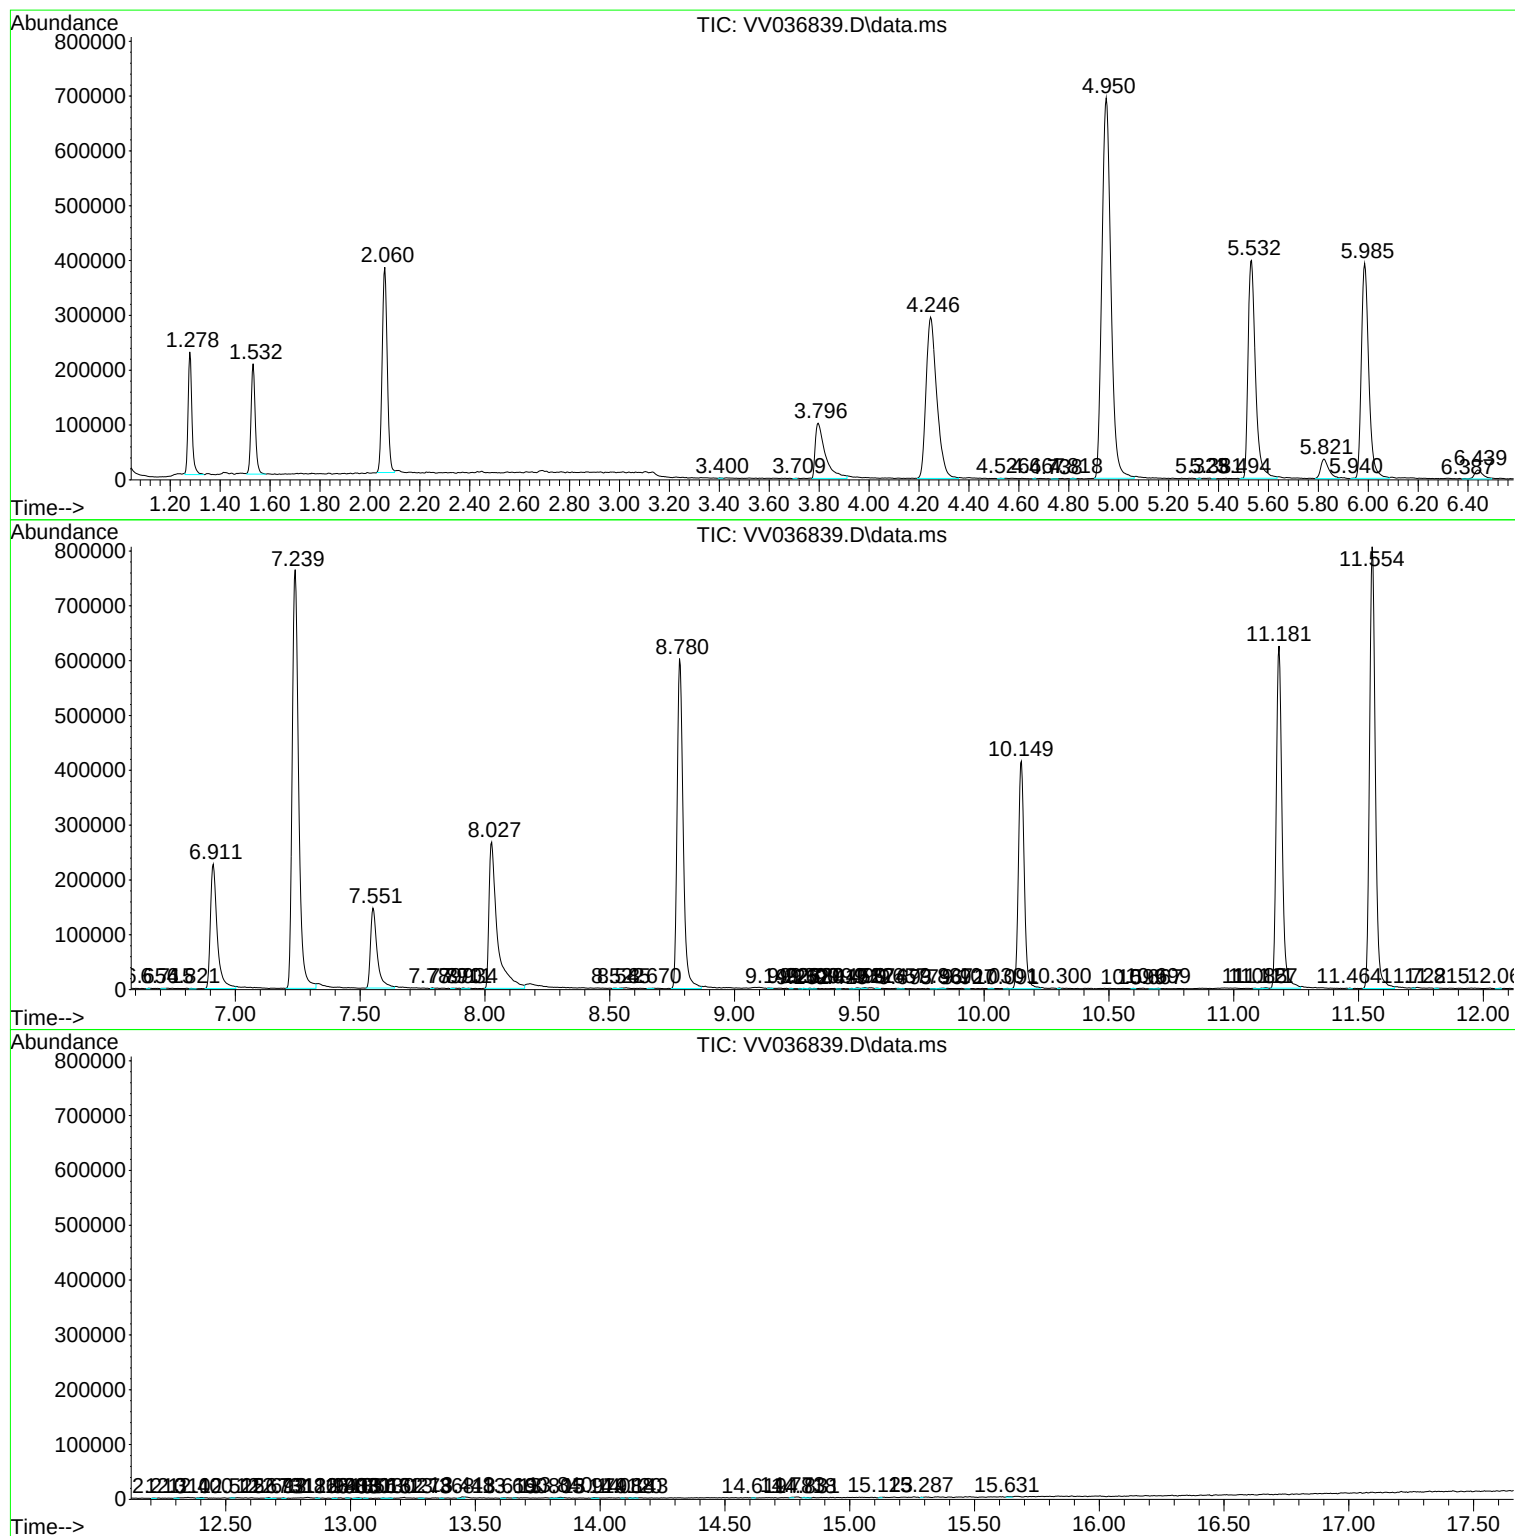

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036839.D
Acq On : 07 Aug 2024 15:54
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036839.D
Acq On : 07 Aug 2024 15:54
Operator : SY/MD
Sample : P3498-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08M1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc