
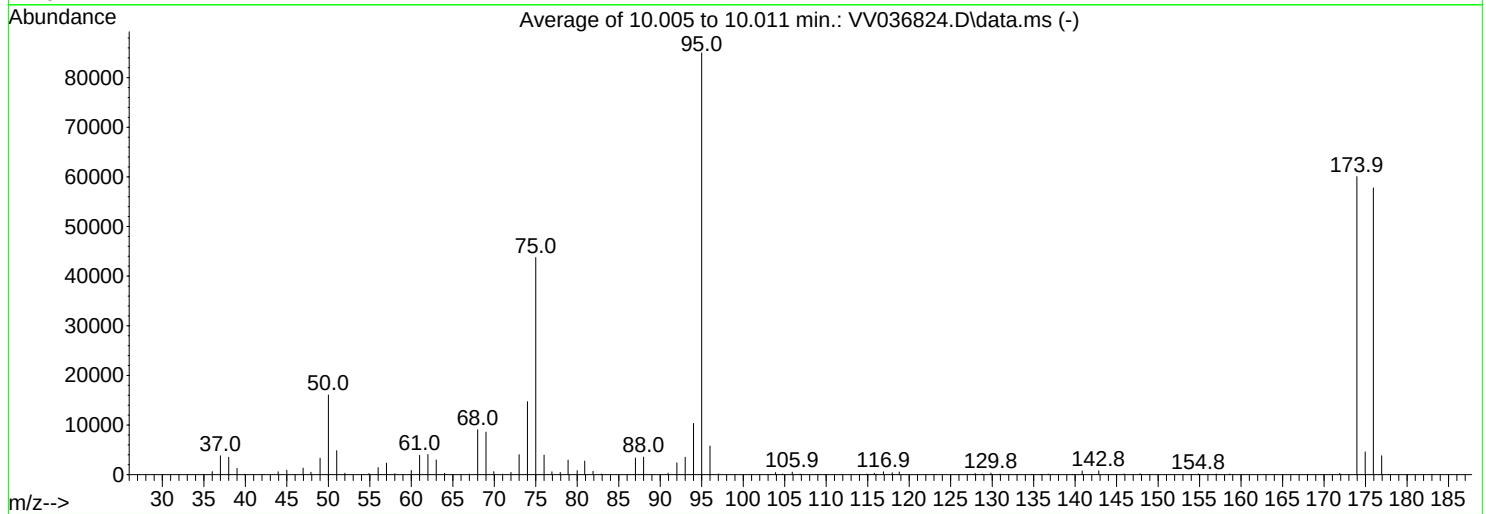


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080724\
Data File : VV036824.D
Acq On : 07 Aug 2024 08:18
Operator : SY/MD
Sample : BFB356
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB356

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Fri Aug 09 02:41:02 2024

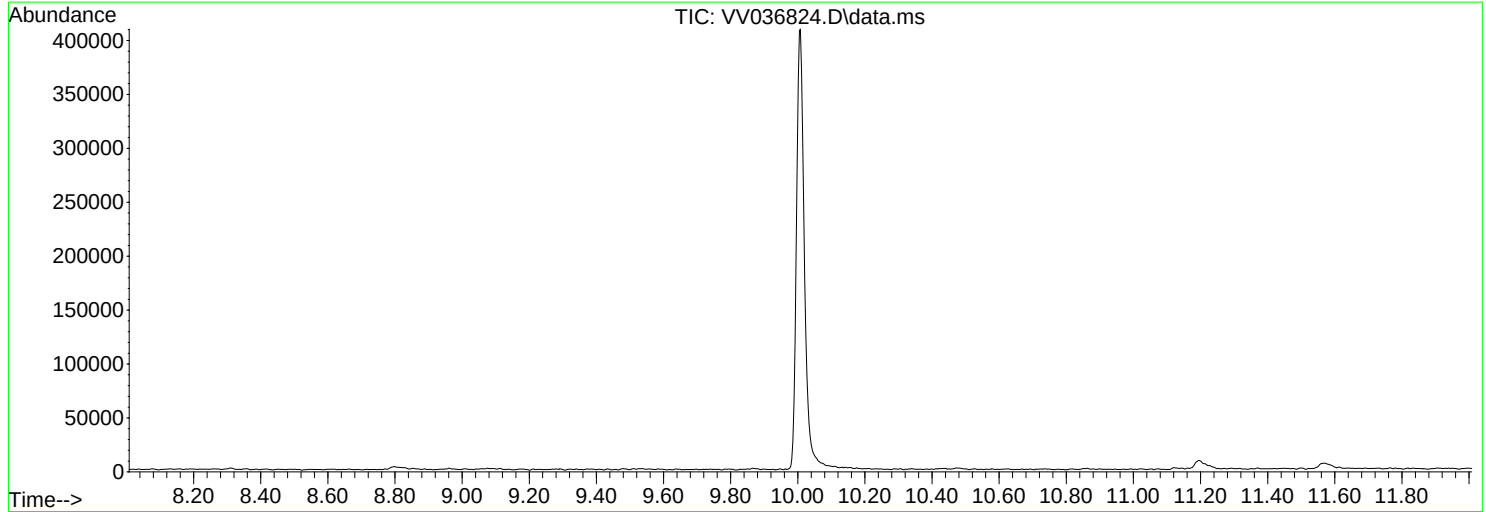

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	16060	PASS
75	95	30	80	51.5	43771	PASS
95	95	100	100	100.0	85003	PASS
96	95	5	9	6.8	5763	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.7	60056	PASS
175	174	5	9	7.6	4580	PASS
176	174	95	105	96.2	57768	PASS
177	176	5	10	6.6	3813	PASS

m/z	Abundance
36.00	133.0
39.00	275.0
39.90	257.0
41.00	182.0
41.90	105.0
43.10	187.0
43.90	875.0
54.90	155.0
67.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	748.0
37.00	4019.0
38.00	3851.0
39.00	1659.0
39.90	355.0
40.90	177.0
43.10	200.0
44.00	1467.0
45.00	987.0
47.00	1401.0
47.90	535.0
49.00	3584.0
50.00	16880.0
51.00	5142.0
52.00	279.0
54.90	394.0
56.00	1520.0
57.00	2311.0
58.00	164.0
60.00	876.0
61.00	4039.0
62.00	4268.0
63.00	3104.0
64.00	301.0
64.80	102.0
67.10	283.0
68.00	9362.0
69.00	8950.0
69.90	687.0
71.00	118.0
72.00	453.0
73.00	4238.0
74.00	15035.0
75.00	45720.0
76.00	4245.0
76.90	546.0
78.00	495.0
78.90	2935.0
80.00	821.0
80.90	2710.0
81.90	679.0
82.90	133.0
87.00	3385.0
88.00	3673.0
90.90	353.0
92.00	2496.0
93.00	3613.0
94.00	10879.0
95.00	87544.0
96.00	5897.0
97.00	177.0
103.90	468.0
104.70	147.0
105.90	501.0
106.90	137.0
111.80	110.0
113.00	115.0
114.90	123.0
115.80	246.0
116.90	583.0
118.00	447.0
118.80	524.0
127.90	268.0
128.80	165.0
129.90	317.0
131.00	129.0
134.90	117.0
136.80	144.0
140.80	767.0
142.80	792.0
145.90	175.0
147.80	203.0
148.70	103.0
154.90	194.0
157.00	206.0
158.60	114.0
161.00	113.0
171.90	313.0
173.90	61008.0
175.00	4700.0
176.00	58064.0
176.90	3794.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	739.0
37.00	3939.0
38.00	3672.0
39.00	1568.0
39.90	373.0
40.90	166.0
43.10	173.0
44.00	1472.0
45.00	929.0
47.00	1353.0
47.90	533.0
49.00	3373.0
50.00	16560.0
51.00	4977.0
52.00	311.0
55.00	397.0
56.00	1442.0
57.00	2378.0
58.00	199.0
60.00	869.0
61.00	4002.0
62.00	4177.0
63.00	3000.0
64.00	321.0
64.80	114.0
67.00	261.0
68.00	9422.0
69.00	8823.0
69.90	630.0
71.00	132.0
72.00	467.0
73.00	4159.0
74.00	15203.0
75.00	45160.0
76.00	4042.0
77.00	619.0
78.00	474.0
78.90	3029.0
80.00	876.0
80.90	2849.0
81.90	706.0
82.90	139.0
87.00	3412.0
88.00	3679.0
91.00	335.0
92.00	2428.0
93.00	3577.0
94.00	10766.0
95.00	87712.0
96.00	6035.0
97.00	155.0
103.90	452.0
104.70	141.0
105.90	568.0
106.80	150.0
109.80	110.0
111.80	114.0
114.90	154.0
115.80	295.0
116.10	258.0
116.90	611.0
118.00	386.0
118.80	604.0
127.90	270.0
128.80	144.0
129.90	328.0
131.00	130.0
135.80	114.0
136.80	126.0
139.70	124.0
140.90	759.0
141.80	105.0
142.90	780.0
145.90	175.0
147.80	193.0
154.80	174.0
157.00	175.0
158.70	156.0
161.00	108.0
171.90	276.0
173.90	62232.0
175.00	4716.0
175.90	59648.0
176.90	3952.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	711.0
37.00	3492.0
38.00	3055.0
39.00	1353.0
39.90	341.0
41.00	160.0
41.90	107.0
43.10	171.0
44.00	1424.0
45.00	773.0
46.90	1213.0
47.90	427.0
49.00	3009.0
50.00	14741.0
51.00	4440.0
52.00	282.0
55.00	386.0
56.00	1296.0
57.00	2249.0
58.00	201.0
60.00	757.0
61.00	3659.0
62.00	3705.0
63.00	2778.0
64.00	296.0
67.00	230.0
68.00	8443.0
69.00	8012.0
70.00	538.0
71.00	150.0
72.00	432.0
73.00	3655.0
74.00	13871.0
75.00	40432.0
76.00	3558.0
77.00	584.0
77.90	416.0
78.90	2800.0
80.00	757.0
80.90	2688.0
81.90	649.0
82.90	130.0
87.00	3282.0
88.00	3275.0
91.00	310.0
92.00	2250.0
93.00	3314.0
94.00	9357.0
95.00	79752.0
96.00	5358.0
97.10	133.0
103.90	346.0
104.80	109.0
105.90	452.0
106.80	151.0
109.90	115.0
114.90	157.0
115.80	321.0
116.90	592.0
117.90	289.0
118.80	560.0
128.00	272.0
128.80	110.0
129.80	303.0
130.90	118.0
134.70	104.0
136.70	102.0
139.70	116.0
140.90	727.0
142.90	762.0
145.90	142.0
147.80	167.0
154.00	104.0
154.90	146.0
157.10	126.0
158.70	123.0
171.90	184.0
174.00	56928.0
174.90	4324.0
175.90	55592.0
177.00	3693.0
177.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356