

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027245.D
 Acq On : 08 Aug 2022 13:55
 Operator : SY/MD
 Sample : VIBLK272
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rBV	159767	172268	9.71%	1.271%
2	1.558	155	161	173	rVB	142393	165429	9.32%	1.221%
3	2.098	321	329	342	rVB	282885	394184	22.21%	2.909%
4	2.327	398	400	403	rBV2	689	405	0.02%	0.003%
5	2.449	436	438	440	rBV2	428	171	0.01%	0.001%
6	2.751	531	532	535	rBV2	506	270	0.02%	0.002%
7	2.806	547	549	551	rVB2	466	183	0.01%	0.001%
8	2.863	564	567	570	rVB2	318	191	0.01%	0.001%
9	2.876	570	571	573	rBV	509	194	0.01%	0.001%
10	2.918	581	584	585	rBV2	430	163	0.01%	0.001%
11	2.966	596	599	602	rBV	324	193	0.01%	0.001%
12	2.989	602	606	608	rVB3	349	265	0.01%	0.002%
13	3.005	609	611	612	rBV	303	145	0.01%	0.001%
14	3.066	626	630	632	rBV	225	149	0.01%	0.001%
15	3.079	632	634	636	rVV	268	120	0.01%	0.001%
16	3.201	670	672	675	rVV2	289	119	0.01%	0.001%
17	3.253	685	688	691	rVB	301	133	0.01%	0.001%
18	3.275	692	695	697	rVB3	386	221	0.01%	0.002%
19	3.307	701	705	707	rBV2	271	219	0.01%	0.002%
20	3.336	709	714	719	rBV5	546	615	0.03%	0.005%
21	3.355	719	720	722	rVB	391	122	0.01%	0.001%
22	3.388	726	730	732	rBV4	492	338	0.02%	0.002%
23	3.400	732	734	736	rBV2	213	120	0.01%	0.001%
24	3.449	747	749	751	rVB2	351	120	0.01%	0.001%
25	3.709	825	830	832	rBV2	465	268	0.02%	0.002%
26	3.735	836	838	841	rVB	284	130	0.01%	0.001%
27	3.761	842	846	848	rVB2	485	300	0.02%	0.002%
28	3.777	848	851	854	rBV	442	251	0.01%	0.002%
29	3.799	855	858	860	rVB	328	128	0.01%	0.001%
30	3.818	862	864	865	rBV2	247	113	0.01%	0.001%
31	3.863	868	878	913	rBV	163462	475132	26.78%	3.506%
32	4.339	1010	1026	1050	rBV	257929	667890	37.64%	4.928%
33	4.580	1099	1101	1104	rVB4	724	254	0.01%	0.002%
34	4.632	1114	1117	1120	rVB3	708	454	0.03%	0.003%
35	4.651	1120	1123	1125	rBV2	523	331	0.02%	0.002%
36	4.741	1148	1151	1155	rVB4	770	515	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027245.D
 Acq On : 08 Aug 2022 13:55
 Operator : SY/MD
 Sample : VIBLK272
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	4.767	1155	1159	1161	rBV3	556	441	0.02%	0.003%
38	4.780	1161	1163	1166	rVV2	468	265	0.01%	0.002%
39	4.812	1172	1173	1175	rBV	377	130	0.01%	0.001%
40	4.867	1184	1190	1192	rBV5	499	518	0.03%	0.004%
41	4.892	1197	1198	1200	rBV	444	158	0.01%	0.001%
42	4.924	1206	1208	1209	rBV	316	141	0.01%	0.001%
43	4.953	1213	1217	1221	rBV4	620	528	0.03%	0.004%
44	5.037	1224	1243	1284	rBV3	656384	1774445	100.00%	13.094%
45	5.391	1351	1353	1359	rBV4	575	614	0.03%	0.005%
46	5.426	1363	1364	1369	rBV2	402	183	0.01%	0.001%
47	5.458	1372	1374	1376	rBV2	373	230	0.01%	0.002%
48	5.471	1376	1378	1380	rVB3	715	317	0.02%	0.002%
49	5.484	1380	1382	1383	rBV2	688	240	0.01%	0.002%
50	5.609	1408	1421	1455	rBV	500157	1065331	60.04%	7.861%
51	5.905	1501	1513	1526	rBV8	9439	21260	1.20%	0.157%
52	6.063	1547	1562	1597	rBV	396619	841350	47.41%	6.208%
53	6.349	1648	1651	1654	rBV	384	258	0.01%	0.002%
54	6.407	1666	1669	1670	rBV	434	238	0.01%	0.002%
55	6.439	1676	1679	1683	rVB3	347	262	0.01%	0.002%
56	6.465	1683	1687	1692	rBV4	625	589	0.03%	0.004%
57	6.510	1697	1701	1705	rVV2	528	506	0.03%	0.004%
58	6.535	1707	1709	1713	rVB2	530	243	0.01%	0.002%
59	6.603	1728	1730	1732	rBV2	290	144	0.01%	0.001%
60	6.658	1745	1747	1750	rBV2	379	255	0.01%	0.002%
61	6.699	1758	1760	1762	rVB	437	144	0.01%	0.001%
62	6.744	1772	1774	1777	rVB3	437	220	0.01%	0.002%
63	6.780	1783	1785	1787	rBV	428	192	0.01%	0.001%
64	6.831	1799	1801	1803	rVV	340	196	0.01%	0.001%
65	6.857	1806	1809	1814	rVB2	350	227	0.01%	0.002%
66	6.879	1814	1816	1817	rBV2	530	135	0.01%	0.001%
67	6.889	1817	1819	1820	rBV2	337	115	0.01%	0.001%
68	6.902	1821	1823	1825	rBV2	335	154	0.01%	0.001%
69	6.915	1825	1827	1830	rBV3	757	420	0.02%	0.003%
70	6.979	1835	1847	1876	rBV	202272	390033	21.98%	2.878%
71	7.310	1938	1950	1974	rBV	724621	1295053	72.98%	9.556%
72	7.616	2035	2045	2071	rBV	146966	269115	15.17%	1.986%
73	8.021	2169	2171	2172	rBV	439	154	0.01%	0.001%
74	8.082	2180	2190	2227	rBV	536828	1011477	57.00%	7.464%
75	8.535	2329	2331	2333	rBV3	407	235	0.01%	0.002%
76	8.706	2382	2384	2386	rBV	471	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027245.D
 Acq On : 08 Aug 2022 13:55
 Operator : SY/MD
 Sample : VIBLK272
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	8.747	2391	2397	2400	rBV5	890	903	0.05%	0.007%
78	8.847	2417	2428	2464	rBV	833221	1377037	77.60%	10.161%
79	9.111	2507	2510	2514	rVB4	1644	1164	0.07%	0.009%
80	9.140	2514	2519	2531	rBV9	2306	4585	0.26%	0.034%
81	9.262	2554	2557	2559	rBV3	457	268	0.02%	0.002%
82	9.278	2559	2562	2563	rBV2	542	242	0.01%	0.002%
83	9.323	2571	2576	2578	rBV2	513	469	0.03%	0.003%
84	9.461	2617	2619	2620	rBV2	446	181	0.01%	0.001%
85	9.551	2640	2647	2652	rBV5	1371	1738	0.10%	0.013%
86	9.625	2667	2670	2673	rBV3	489	390	0.02%	0.003%
87	9.757	2708	2711	2713	rBV3	552	315	0.02%	0.002%
88	9.825	2731	2732	2734	rBV	467	164	0.01%	0.001%
89	9.911	2756	2759	2760	rBV2	446	251	0.01%	0.002%
90	9.960	2771	2774	2778	rVB	540	349	0.02%	0.003%
91	9.998	2784	2786	2789	rBV2	753	599	0.03%	0.004%
92	10.014	2789	2791	2798	rVB5	915	730	0.04%	0.005%
93	10.214	2840	2853	2875	rBV	605971	956043	53.88%	7.055%
94	10.374	2901	2903	2905	rBV3	910	411	0.02%	0.003%
95	10.484	2935	2937	2940	rBV3	892	465	0.03%	0.003%
96	10.638	2983	2985	2988	rBV2	461	318	0.02%	0.002%
97	10.657	2988	2991	2994	rBV4	944	835	0.05%	0.006%
98	11.030	3099	3107	3111	rBV5	2775	4248	0.24%	0.031%
99	11.246	3164	3174	3195	rBV	882053	1352330	76.21%	9.979%
100	11.622	3280	3291	3310	rBV	818276	1288720	72.63%	9.510%




Sum of corrected areas: 13551613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
Data File : VV027245.D
Acq On : 08 Aug 2022 13:55
Operator : SY/MD
Sample : VIBLK272
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

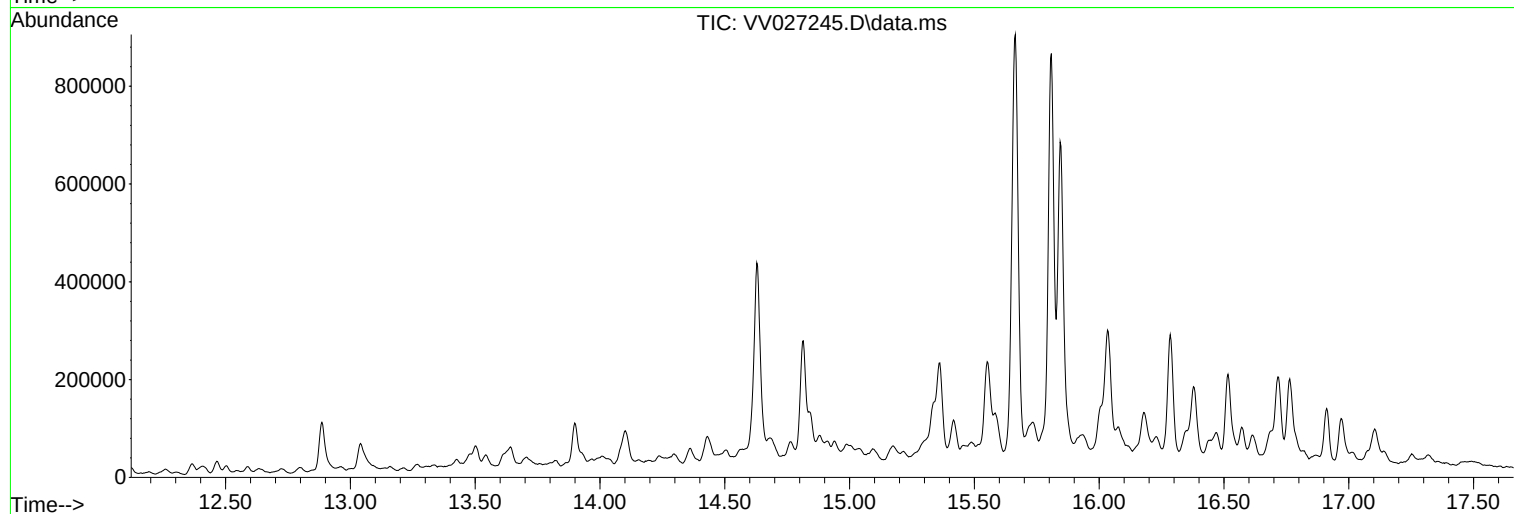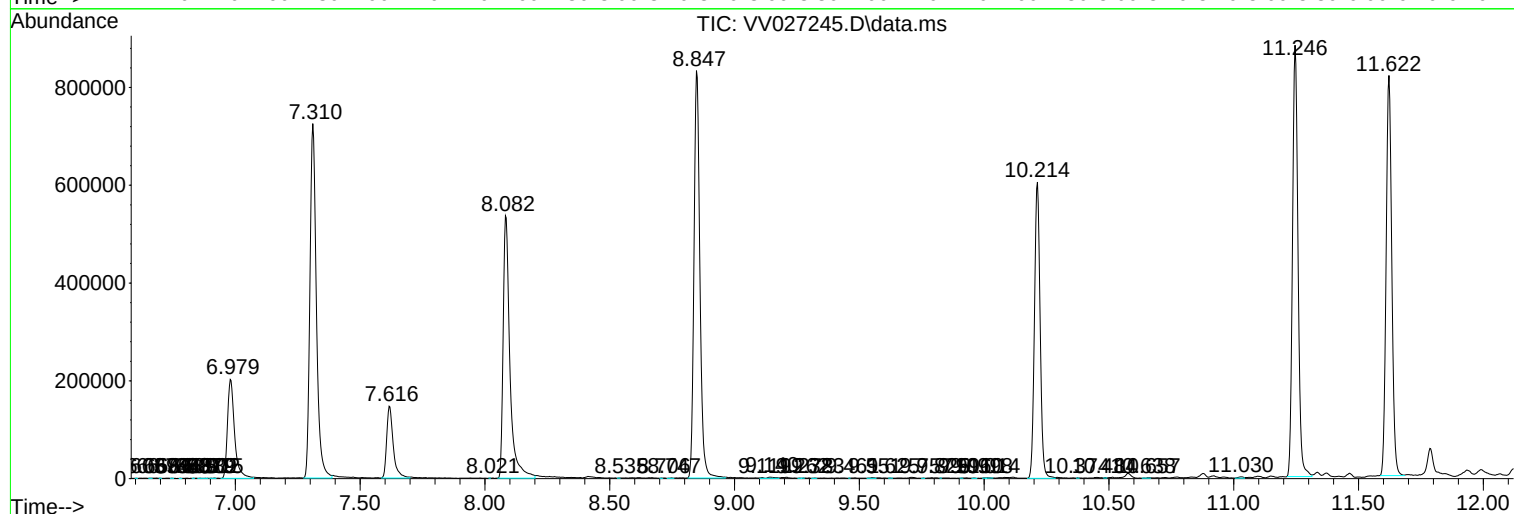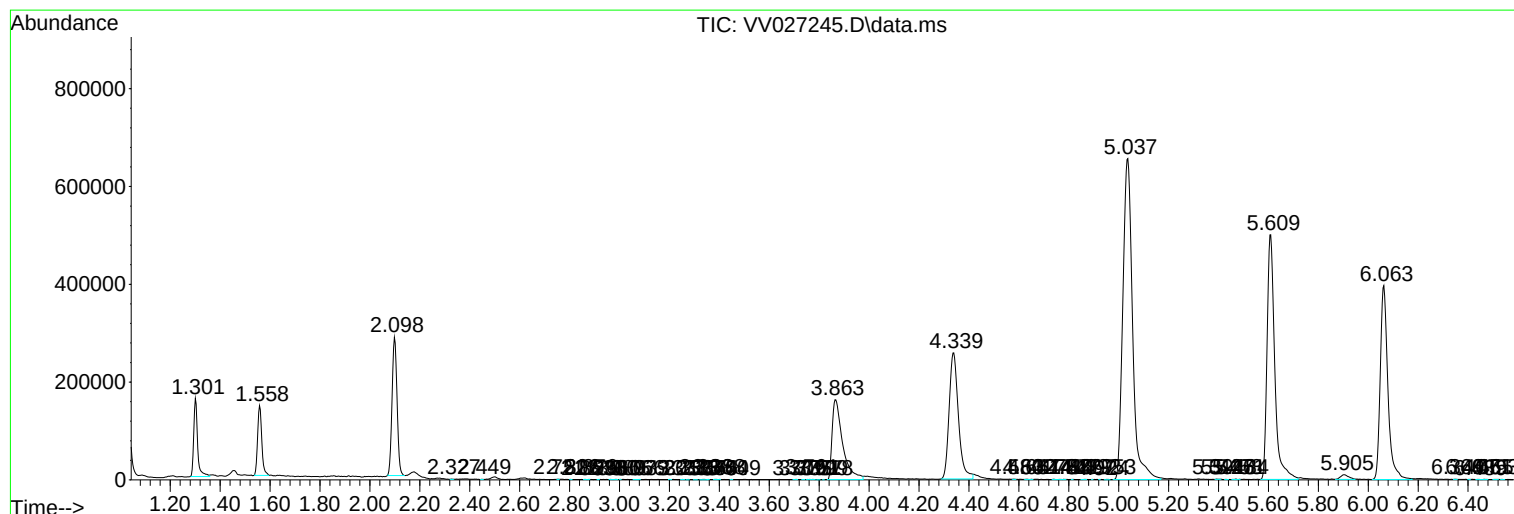

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
Data File : VV027245.D
Acq On : 08 Aug 2022 13:55
Operator : SY/MD
Sample : VIBLK272
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
Data File : VV027245.D
Acq On : 08 Aug 2022 13:55
Operator : SY/MD
Sample : VIBLK272
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------