

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027246.D
 Acq On : 08 Aug 2022 15:21
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rBV	212173	228657	12.19%	1.591%
2	1.558	154	161	177	rVB	173199	205369	10.95%	1.429%
3	2.098	320	329	344	rVB	366978	516541	27.55%	3.594%
4	2.458	440	441	444	rBV	643	331	0.02%	0.002%
5	2.613	479	489	501	rVB2	5281	10502	0.56%	0.073%
6	2.699	512	516	518	rBV2	548	476	0.03%	0.003%
7	2.728	523	525	528	rVV3	330	175	0.01%	0.001%
8	2.757	528	534	538	rVB6	929	1033	0.06%	0.007%
9	2.863	562	567	569	rBV3	459	284	0.02%	0.002%
10	2.902	576	579	584	rVB3	534	360	0.02%	0.003%
11	3.056	625	627	630	rVB4	818	341	0.02%	0.002%
12	3.082	633	635	640	rVB4	505	385	0.02%	0.003%
13	3.191	664	669	671	rBV4	808	717	0.04%	0.005%
14	3.301	699	703	705	rBV	571	394	0.02%	0.003%
15	3.391	728	731	735	rVB3	642	397	0.02%	0.003%
16	3.410	735	737	740	rBV3	561	371	0.02%	0.003%
17	3.461	750	753	755	rBV2	302	157	0.01%	0.001%
18	3.484	758	760	762	rBV2	353	174	0.01%	0.001%
19	3.561	779	784	788	rBV3	255	234	0.01%	0.002%
20	3.606	794	798	799	rVV2	417	346	0.02%	0.002%
21	3.690	815	824	826	rBV3	483	510	0.03%	0.004%
22	3.712	829	831	833	rBV	363	210	0.01%	0.001%
23	3.735	836	838	842	rVV2	371	293	0.02%	0.002%
24	3.754	842	844	847	rVB3	469	190	0.01%	0.001%
25	3.780	847	852	854	rBV2	503	341	0.02%	0.002%
26	3.822	862	865	868	rBV4	388	306	0.02%	0.002%
27	3.863	868	878	912	rBV2	173769	513244	27.37%	3.571%
28	4.336	1010	1025	1047	rBV	282203	706979	37.70%	4.919%
29	4.548	1089	1091	1092	rBV	493	211	0.01%	0.001%
30	4.561	1092	1095	1096	rVV2	809	413	0.02%	0.003%
31	4.728	1145	1147	1149	rBV	542	244	0.01%	0.002%
32	4.757	1154	1156	1159	rBV2	657	485	0.03%	0.003%
33	4.821	1173	1176	1178	rBV	582	260	0.01%	0.002%
34	4.834	1178	1180	1182	rVV2	556	261	0.01%	0.002%
35	4.850	1182	1185	1190	rVB3	619	521	0.03%	0.004%
36	4.937	1209	1212	1214	rVB3	748	345	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027246.D
 Acq On : 08 Aug 2022 15:21
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	4.973	1221	1223	1225	rBV	421	172	0.01%	0.001%
38	5.034	1225	1242	1285	rBV2	705486	1875239	100.00%	13.048%
39	5.384	1348	1351	1353	rBV3	756	532	0.03%	0.004%
40	5.458	1370	1374	1377	rBV4	605	466	0.02%	0.003%
41	5.519	1390	1393	1401	rVB8	1128	1253	0.07%	0.009%
42	5.551	1401	1403	1407	rBV2	662	476	0.03%	0.003%
43	5.606	1408	1420	1452	rBV	537796	1135554	60.56%	7.901%
44	5.802	1479	1481	1484	rVB	963	397	0.02%	0.003%
45	6.059	1547	1561	1595	rBV	417035	875674	46.70%	6.093%
46	6.387	1661	1663	1666	rVB3	688	437	0.02%	0.003%
47	6.468	1683	1688	1689	rBV2	642	365	0.02%	0.003%
48	6.542	1707	1711	1715	rBV3	594	410	0.02%	0.003%
49	6.625	1735	1737	1739	rBV3	513	210	0.01%	0.001%
50	6.645	1739	1743	1745	rBV3	550	307	0.02%	0.002%
51	6.677	1752	1753	1759	rVB3	769	522	0.03%	0.004%
52	6.706	1759	1762	1765	rBV3	920	584	0.03%	0.004%
53	6.725	1765	1768	1772	rBV2	461	462	0.02%	0.003%
54	6.760	1776	1779	1780	rBV	469	174	0.01%	0.001%
55	6.767	1780	1781	1784	rBV	340	169	0.01%	0.001%
56	6.831	1799	1801	1805	rVB2	431	281	0.01%	0.002%
57	6.870	1810	1813	1815	rBV3	734	471	0.03%	0.003%
58	6.918	1825	1828	1830	rBV2	341	197	0.01%	0.001%
59	6.931	1830	1832	1833	rBV2	407	190	0.01%	0.001%
60	6.979	1836	1847	1873	rBV	215151	412620	22.00%	2.871%
61	7.310	1937	1950	1979	rBV	798552	1440284	76.81%	10.022%
62	7.616	2035	2045	2071	rBV	154642	279348	14.90%	1.944%
63	7.982	2153	2159	2164	rBV4	892	1011	0.05%	0.007%
64	8.043	2176	2178	2180	rBV	562	207	0.01%	0.001%
65	8.082	2180	2190	2229	rBV	524721	986464	52.60%	6.864%
66	8.522	2323	2327	2331	rBV4	1001	800	0.04%	0.006%
67	8.542	2331	2333	2335	rBV3	492	237	0.01%	0.002%
68	8.567	2340	2341	2344	rBV3	530	298	0.02%	0.002%
69	8.677	2373	2375	2377	rBV2	480	295	0.02%	0.002%
70	8.728	2388	2391	2393	rBV4	364	220	0.01%	0.002%
71	8.773	2402	2405	2408	rBV2	622	400	0.02%	0.003%
72	8.847	2416	2428	2459	rBV	846817	1412365	75.32%	9.827%
73	9.140	2515	2519	2520	rBV3	698	548	0.03%	0.004%
74	9.252	2552	2554	2556	rBV3	453	215	0.01%	0.001%
75	9.275	2559	2561	2563	rBV2	512	273	0.01%	0.002%
76	9.307	2568	2571	2572	rBV3	442	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027246.D
 Acq On : 08 Aug 2022 15:21
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	9.445	2611	2614	2615	rBV3	545	353	0.02%	0.002%
78	9.455	2615	2617	2620	rVV3	372	262	0.01%	0.002%
79	9.500	2629	2631	2634	rVB	489	221	0.01%	0.002%
80	9.538	2641	2643	2646	rBV3	726	596	0.03%	0.004%
81	9.693	2687	2691	2696	rVV2	330	291	0.02%	0.002%
82	9.831	2729	2734	2739	rBV4	470	514	0.03%	0.004%
83	9.908	2754	2758	2761	rBV3	736	635	0.03%	0.004%
84	10.001	2783	2787	2789	rVB2	656	463	0.02%	0.003%
85	10.014	2789	2791	2793	rBV	485	257	0.01%	0.002%
86	10.053	2799	2803	2805	rBV3	556	325	0.02%	0.002%
87	10.075	2808	2810	2813	rBV2	336	228	0.01%	0.002%
88	10.120	2822	2824	2827	rBV3	423	233	0.01%	0.002%
89	10.214	2841	2853	2879	rBV	593900	943256	50.30%	6.563%
90	10.413	2913	2915	2916	rBV2	624	201	0.01%	0.001%
91	10.516	2945	2947	2949	rBV	404	244	0.01%	0.002%
92	10.577	2961	2966	2973	rBV6	1787	2334	0.12%	0.016%
93	10.635	2982	2984	2987	rBV2	630	328	0.02%	0.002%
94	10.728	3011	3013	3015	rBV2	606	246	0.01%	0.002%
95	11.246	3163	3174	3196	rBV	907561	1375970	73.38%	9.574%
96	11.461	3236	3241	3245	rBV6	1447	1518	0.08%	0.011%
97	11.622	3279	3291	3314	rBV	848488	1355153	72.27%	9.429%
98	12.291	3497	3499	3500	rBV2	1217	486	0.03%	0.003%
99	12.885	3678	3684	3699	rVB3	18994	28175	1.50%	0.196%
100	13.898	3993	3999	4014	rVB	22948	37052	1.98%	0.258%




Sum of corrected areas: 14371771

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027246.D
 Acq On : 08 Aug 2022 15:21
 Operator : SY/MD
 Sample : VIBLK273
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
 TIC Integration Parameters: LSCINT.P

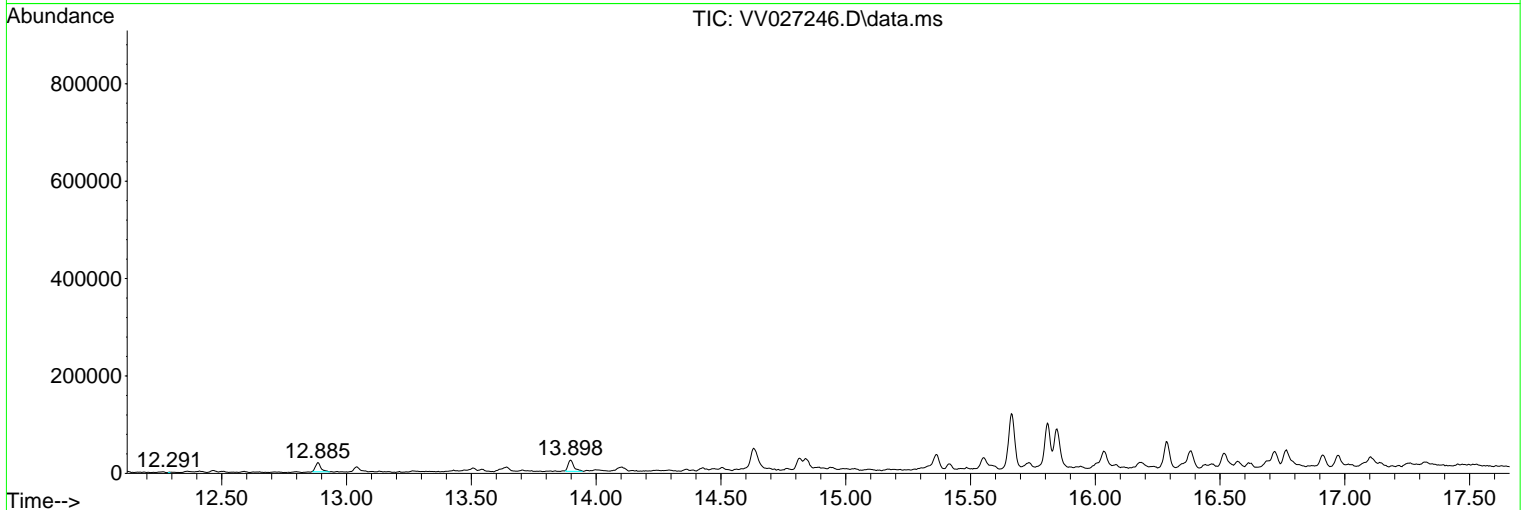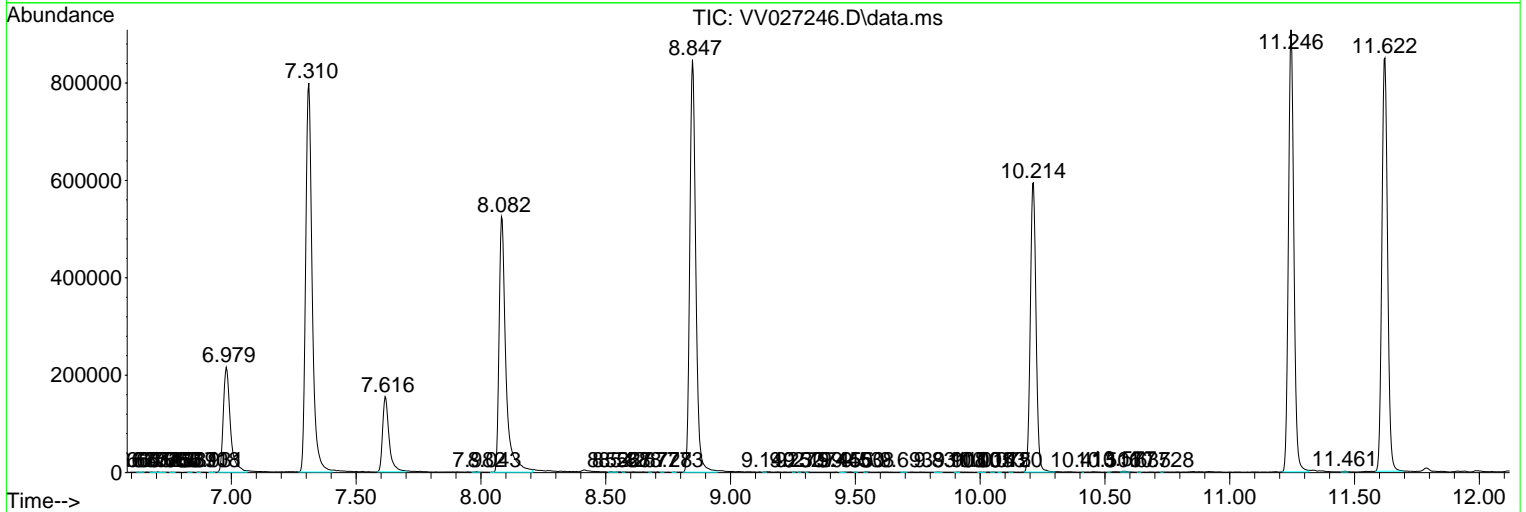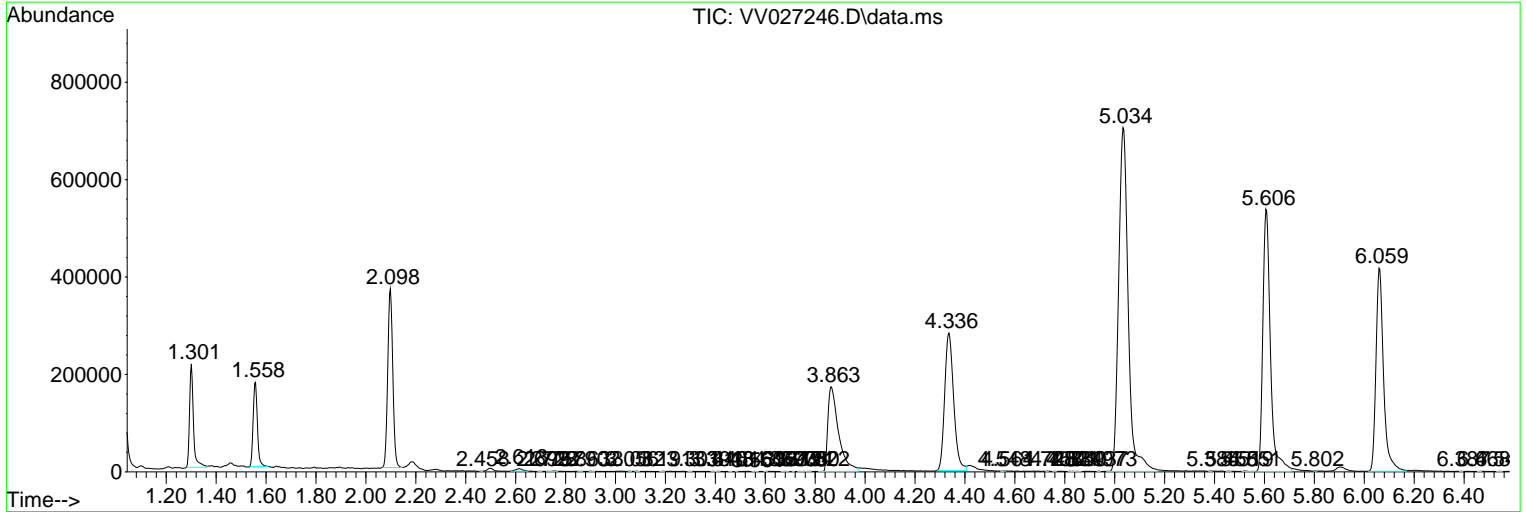

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
Data File : VV027246.D
Acq On : 08 Aug 2022 15:21
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
Data File : VV027246.D
Acq On : 08 Aug 2022 15:21
Operator : SY/MD
Sample : VIBLK273
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK273

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
