
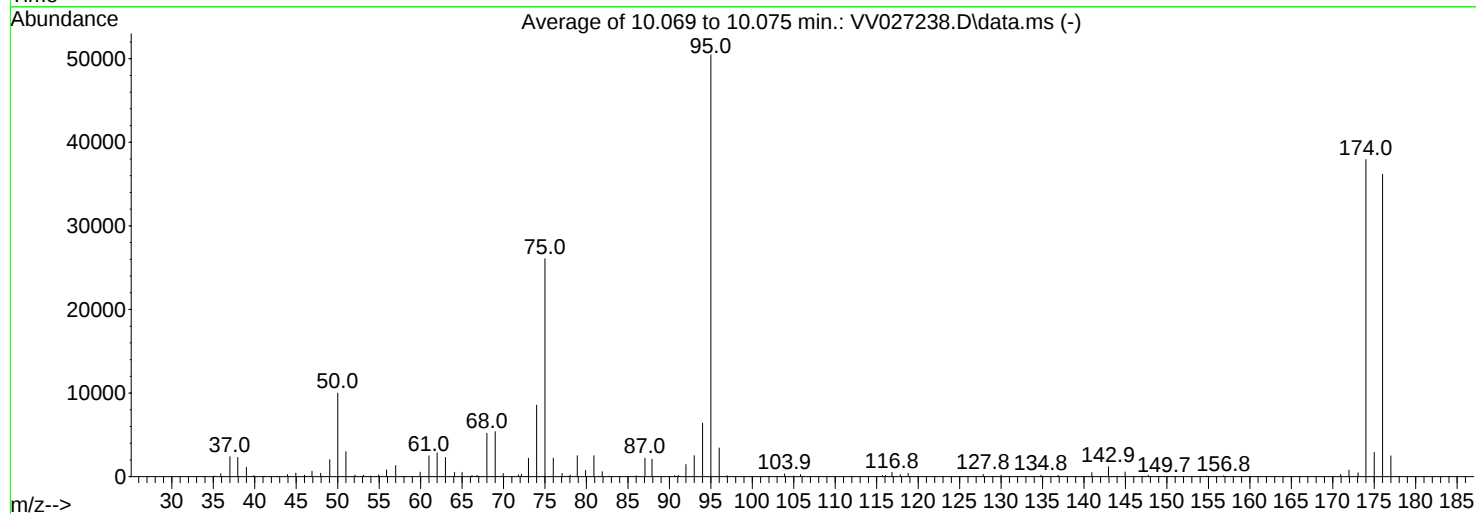


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080822\
 Data File : VV027238.D
 Acq On : 08 Aug 2022 08:43
 Operator : SY/MD
 Sample : BFB307
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB307

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 09 02:29:12 2022

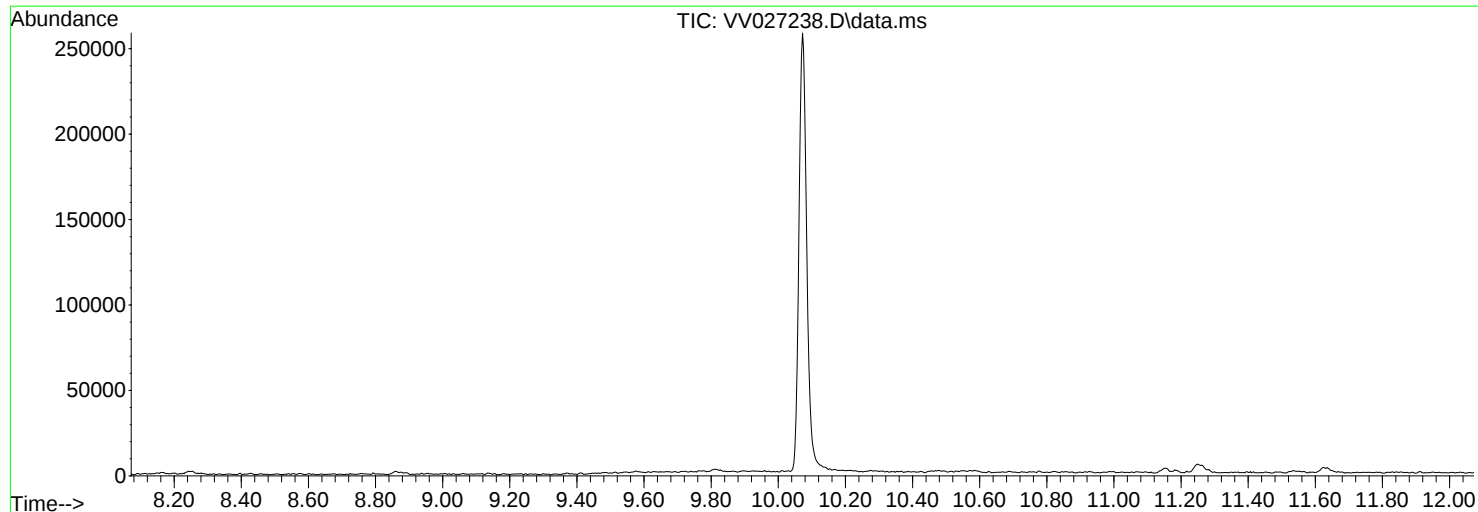

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9990	PASS
75	95	30	80	51.6	26064	PASS
95	95	100	100	100.0	50464	PASS
96	95	5	9	6.8	3435	PASS
173	174	0.00	2	1.2	466	PASS
174	95	50	120	75.2	37947	PASS
175	174	5	9	7.7	2908	PASS
176	174	95	105	95.3	36160	PASS
177	176	5	10	6.9	2488	PASS

m/z	Abundance
35.90	1109.0
37.30	151.0
37.90	490.0
39.90	266.0
43.90	554.0
127.30	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
35.90	1465.0
37.00	2396.0
38.00	2722.0
39.00	1113.0
39.90	397.0
42.60	105.0
44.00	773.0
45.10	421.0
46.00	232.0
46.90	646.0
48.00	434.0
49.10	2018.0
50.00	10118.0
51.00	2919.0
52.20	200.0
53.10	212.0
55.00	249.0
55.90	777.0
57.00	1324.0
57.80	105.0
58.30	115.0
60.00	492.0
61.00	2485.0
62.00	2993.0
63.00	2268.0
64.10	472.0
65.00	516.0
66.20	126.0
66.80	132.0
68.00	5254.0
69.00	5259.0
69.90	339.0
72.10	275.0
73.00	2284.0
74.00	8399.0
75.00	25760.0
76.00	2304.0
77.10	336.0
78.10	222.0
78.90	2415.0
79.90	714.0
80.90	2418.0
81.90	545.0
82.70	124.0
87.10	2258.0
87.90	1996.0
91.10	208.0
92.00	1410.0
93.00	2517.0
94.00	6128.0
95.00	49768.0
96.00	3380.0
96.90	117.0
103.90	330.0
104.90	130.0
105.80	236.0
115.70	204.0
116.80	484.0
117.80	259.0
118.80	453.0
127.80	278.0
129.90	216.0
134.80	158.0
136.90	197.0
141.00	453.0
143.00	1076.0
145.00	620.0
147.80	197.0
154.80	118.0
158.90	103.0
170.90	252.0
171.90	734.0
173.00	659.0
174.00	35936.0
175.00	2675.0
176.00	34408.0
177.00	2443.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	1505.0
37.00	2494.0
38.00	2863.0
39.00	1150.0
40.00	409.0
44.00	823.0
44.90	403.0
46.00	184.0
46.90	677.0
47.90	414.0
49.10	2116.0
50.00	10327.0
51.00	3074.0
52.10	191.0
53.10	181.0
54.00	117.0
55.00	225.0
55.90	806.0
57.00	1335.0
59.90	551.0
61.00	2576.0
62.00	2931.0
63.00	2383.0
64.10	514.0
65.00	519.0
66.20	129.0
66.80	152.0
68.00	5372.0
69.00	5557.0
69.90	411.0
71.80	284.0
72.10	249.0
73.00	2220.0
74.00	8847.0
75.00	27016.0
76.00	2260.0
77.10	413.0
78.10	197.0
78.90	2601.0
79.90	781.0
80.90	2590.0
81.90	642.0
86.00	131.0
87.10	2219.0
87.90	2162.0
90.60	181.0
91.10	191.0
92.00	1509.0
93.00	2604.0
94.00	6627.0
95.00	52024.0
96.00	3605.0
96.90	125.0
103.90	346.0
105.00	131.0
105.80	248.0
115.70	201.0
116.00	188.0
116.80	525.0
117.80	263.0
118.80	431.0
127.80	278.0
130.00	186.0
134.80	190.0
136.90	151.0
140.90	478.0
142.90	1221.0
145.00	570.0
146.00	110.0
147.80	172.0
149.70	101.0
154.80	118.0
156.80	130.0
170.90	281.0
171.90	832.0
174.00	39184.0
175.00	3042.0
176.00	37304.0
177.00	2598.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
35.10	221.0
36.00	1446.0
37.00	2310.0
38.00	2777.0
39.00	1083.0
40.00	421.0
41.20	110.0
44.00	826.0
44.90	436.0
46.00	131.0
46.90	616.0
48.00	355.0
49.00	1976.0
50.00	9526.0
51.00	2982.0
52.00	174.0
53.10	138.0
53.90	143.0
54.90	184.0
55.90	843.0
57.00	1304.0
59.90	555.0
61.00	2378.0
62.00	2644.0
63.00	2221.0
64.10	511.0
65.00	546.0
66.20	122.0
66.80	157.0
68.00	4898.0
69.00	5341.0
70.00	422.0
71.80	348.0
72.20	262.0
73.00	2098.0
74.00	8423.0
75.00	25416.0
76.00	2115.0
77.00	424.0
77.80	170.0
78.00	170.0
78.90	2534.0
79.90	744.0
80.90	2522.0
81.90	616.0
83.10	119.0
86.10	148.0
87.00	2134.0
87.90	2125.0
90.70	199.0
92.00	1464.0
93.00	2387.0
94.00	6505.0
95.00	49600.0
96.00	3320.0
97.00	111.0
103.90	301.0
105.80	241.0
111.80	125.0
116.10	248.0
116.90	542.0
117.90	247.0
118.80	354.0
127.90	255.0
130.10	152.0
134.80	187.0
136.90	107.0
140.90	523.0
142.90	1252.0
144.90	471.0
147.70	133.0
155.00	142.0
156.90	156.0
171.00	258.0
172.00	789.0
173.10	739.0
174.00	38720.0
175.00	3006.0
176.00	36768.0
177.00	2422.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307