

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036853.D
 Acq On : 08 Aug 2024 15:41
 Operator : SY/MD
 Sample : P3480-17
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 09 02:43:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 09 02:41:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	448543	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	417871	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	202248	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	104829	29.261	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	58.520%#		
7) Chloroethane-d5	1.532	69	97377	34.467	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	68.940%#		
11) 1,1-Dichloroethene-d2	2.060	65	47906	31.261	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	62.520%		
21) 2-Butanone-d5	3.796	46	161891	85.288	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	85.290%		
24) Chloroform-d	4.243	84	251664	39.145	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	78.280%		
26) 1,2-Dichloroethane-d4	4.937	65	166855	40.366	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	80.740%		
32) Benzene-d6	4.953	84	477734	37.852	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.700%		
36) 1,2-Dichloropropane-d6	5.985	67	167090	41.036	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	82.080%		
41) Toluene-d8	7.239	98	408984	35.325	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	70.660%#		
43) trans-1,3-Dichloroprop...	7.551	79	72479	34.203	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.400%		
47) 2-Hexanone-d5	8.024	63	88437	75.538	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	75.540%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	204910	43.829	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.660%		
66) 1,2-Dichlorobenzene-d4	11.554	152	172781	41.924	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.840%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	4873	0.859	ug/L #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036853.D
Acq On : 08 Aug 2024 15:41
Operator : SY/MD
Sample : P3480-17
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 09 02:43:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 02:41:02 2024
Response via : Initial Calibration

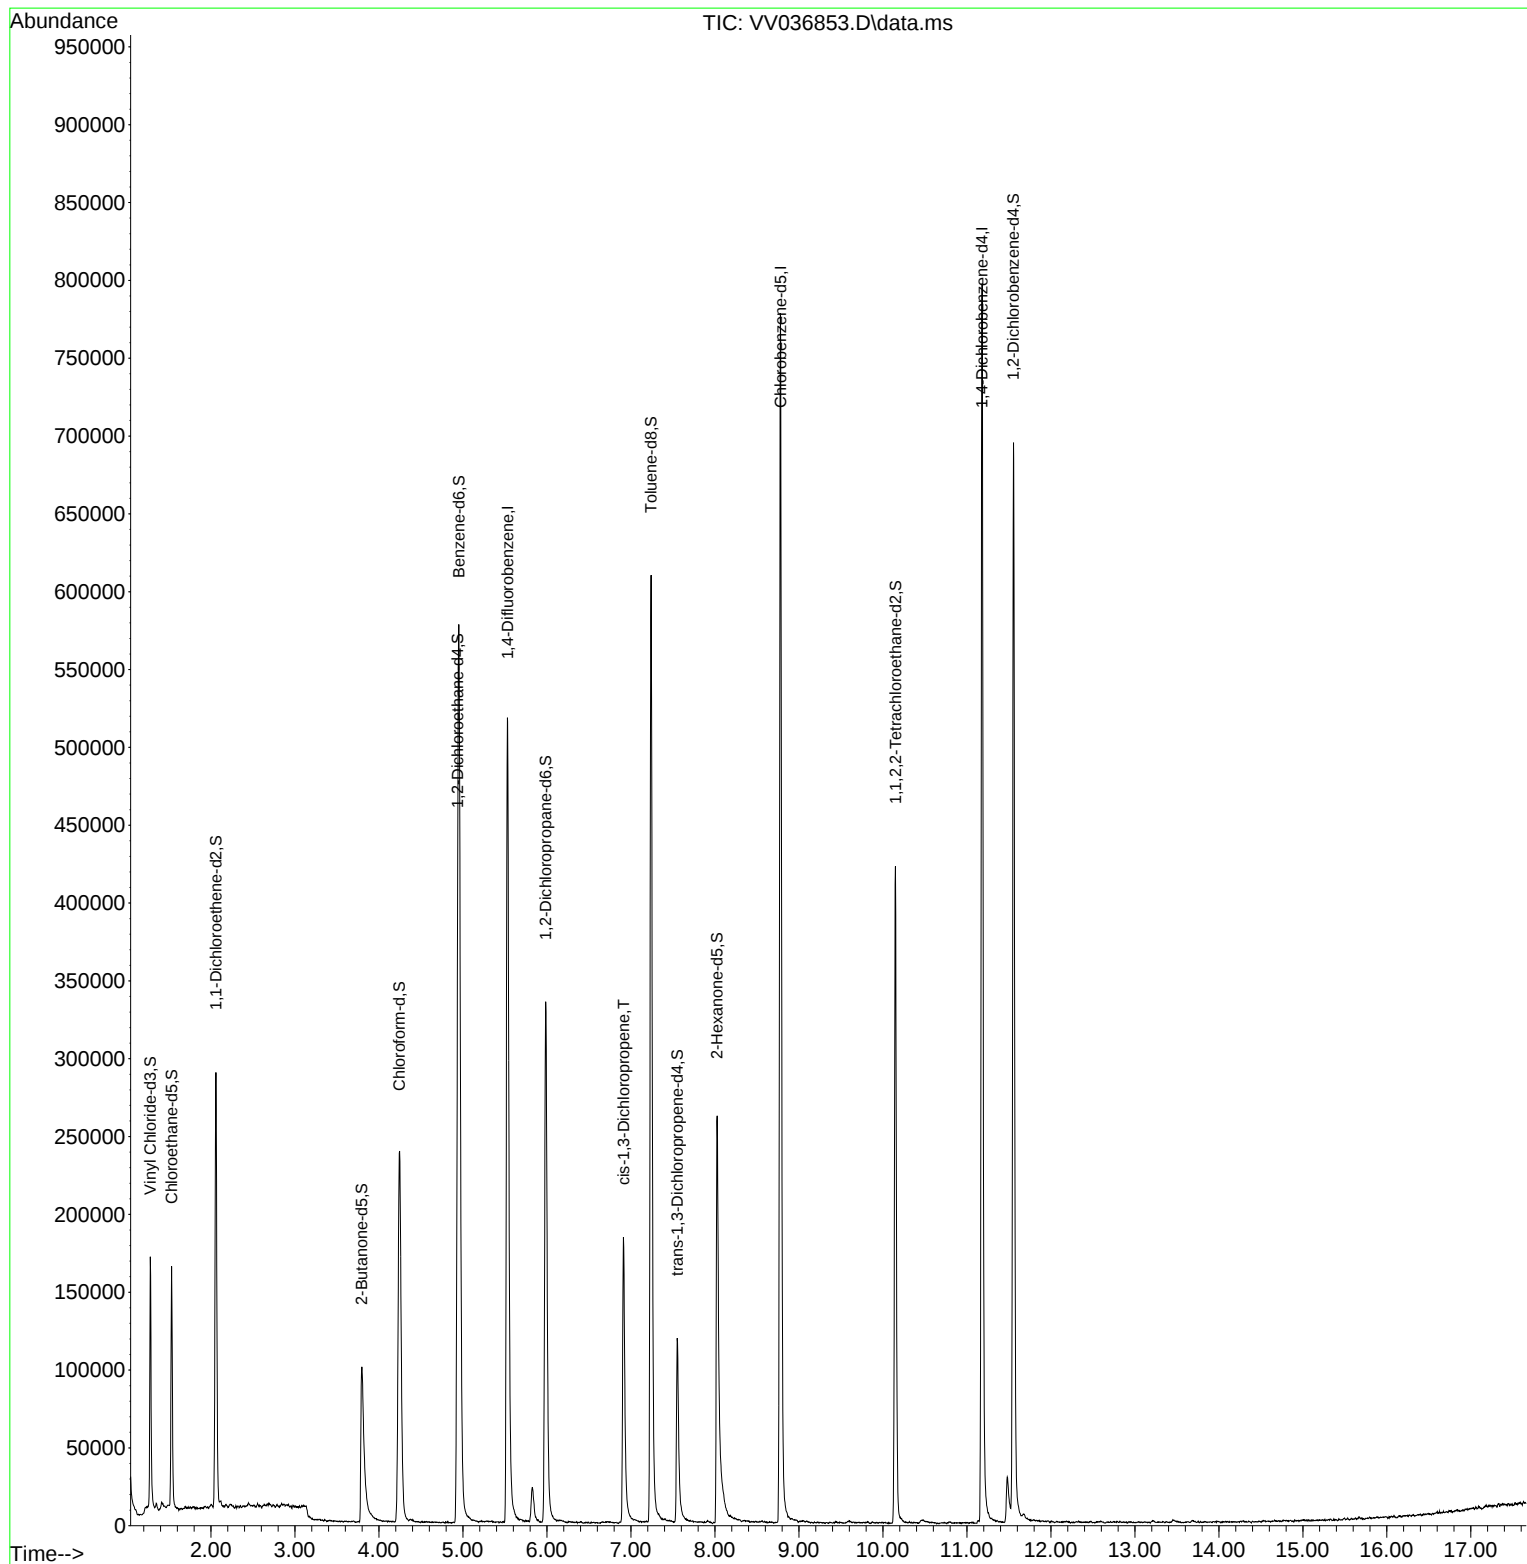

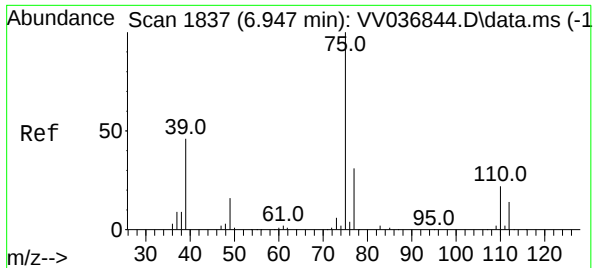

#39
cis-1,3-Dichloropropene
Concen: 0.859 ug/L
RT: 6.915 min Scan# 11
Delta R.T. -0.032 min
Lab File: VV036853.D
Acq: 08 Aug 2024 15:41

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 4873
Ion Ratio Lower Upper
75 100
77 44.6 22.2 41.2#

