

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036854.D
 Acq On : 08 Aug 2024 16:03
 Operator : SY/MD
 Sample : P3480-18
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 09 02:44:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 09 02:41:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	459625	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	428275	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	208648	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	105099	28.629	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	57.260%#
7) Chloroethane-d5	1.532	69	96429	33.309	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	66.620%#
11) 1,1-Dichloroethene-d2	2.060	65	47023	29.945	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.900%#
21) 2-Butanone-d5	3.796	46	159320	81.910	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.910%
24) Chloroform-d	4.243	84	249115	37.814	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.620%
26) 1,2-Dichloroethane-d4	4.937	65	168509	39.783	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.560%
32) Benzene-d6	4.953	84	476536	36.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.680%
36) 1,2-Dichloropropane-d6	5.985	67	168761	40.439	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.880%
41) Toluene-d8	7.239	98	409942	34.548	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	69.100%#
43) trans-1,3-Dichloroprop...	7.551	79	75205	34.627	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.260%
47) 2-Hexanone-d5	8.027	63	89957	74.970	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.970%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	207003	43.201	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.400%
66) 1,2-Dichlorobenzene-d4	11.554	152	175108	41.185	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.380%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.911	75	5362	0.923	ug/L	# 53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036854.D
Acq On : 08 Aug 2024 16:03
Operator : SY/MD
Sample : P3480-18
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 09 02:44:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 02:41:02 2024
Response via : Initial Calibration

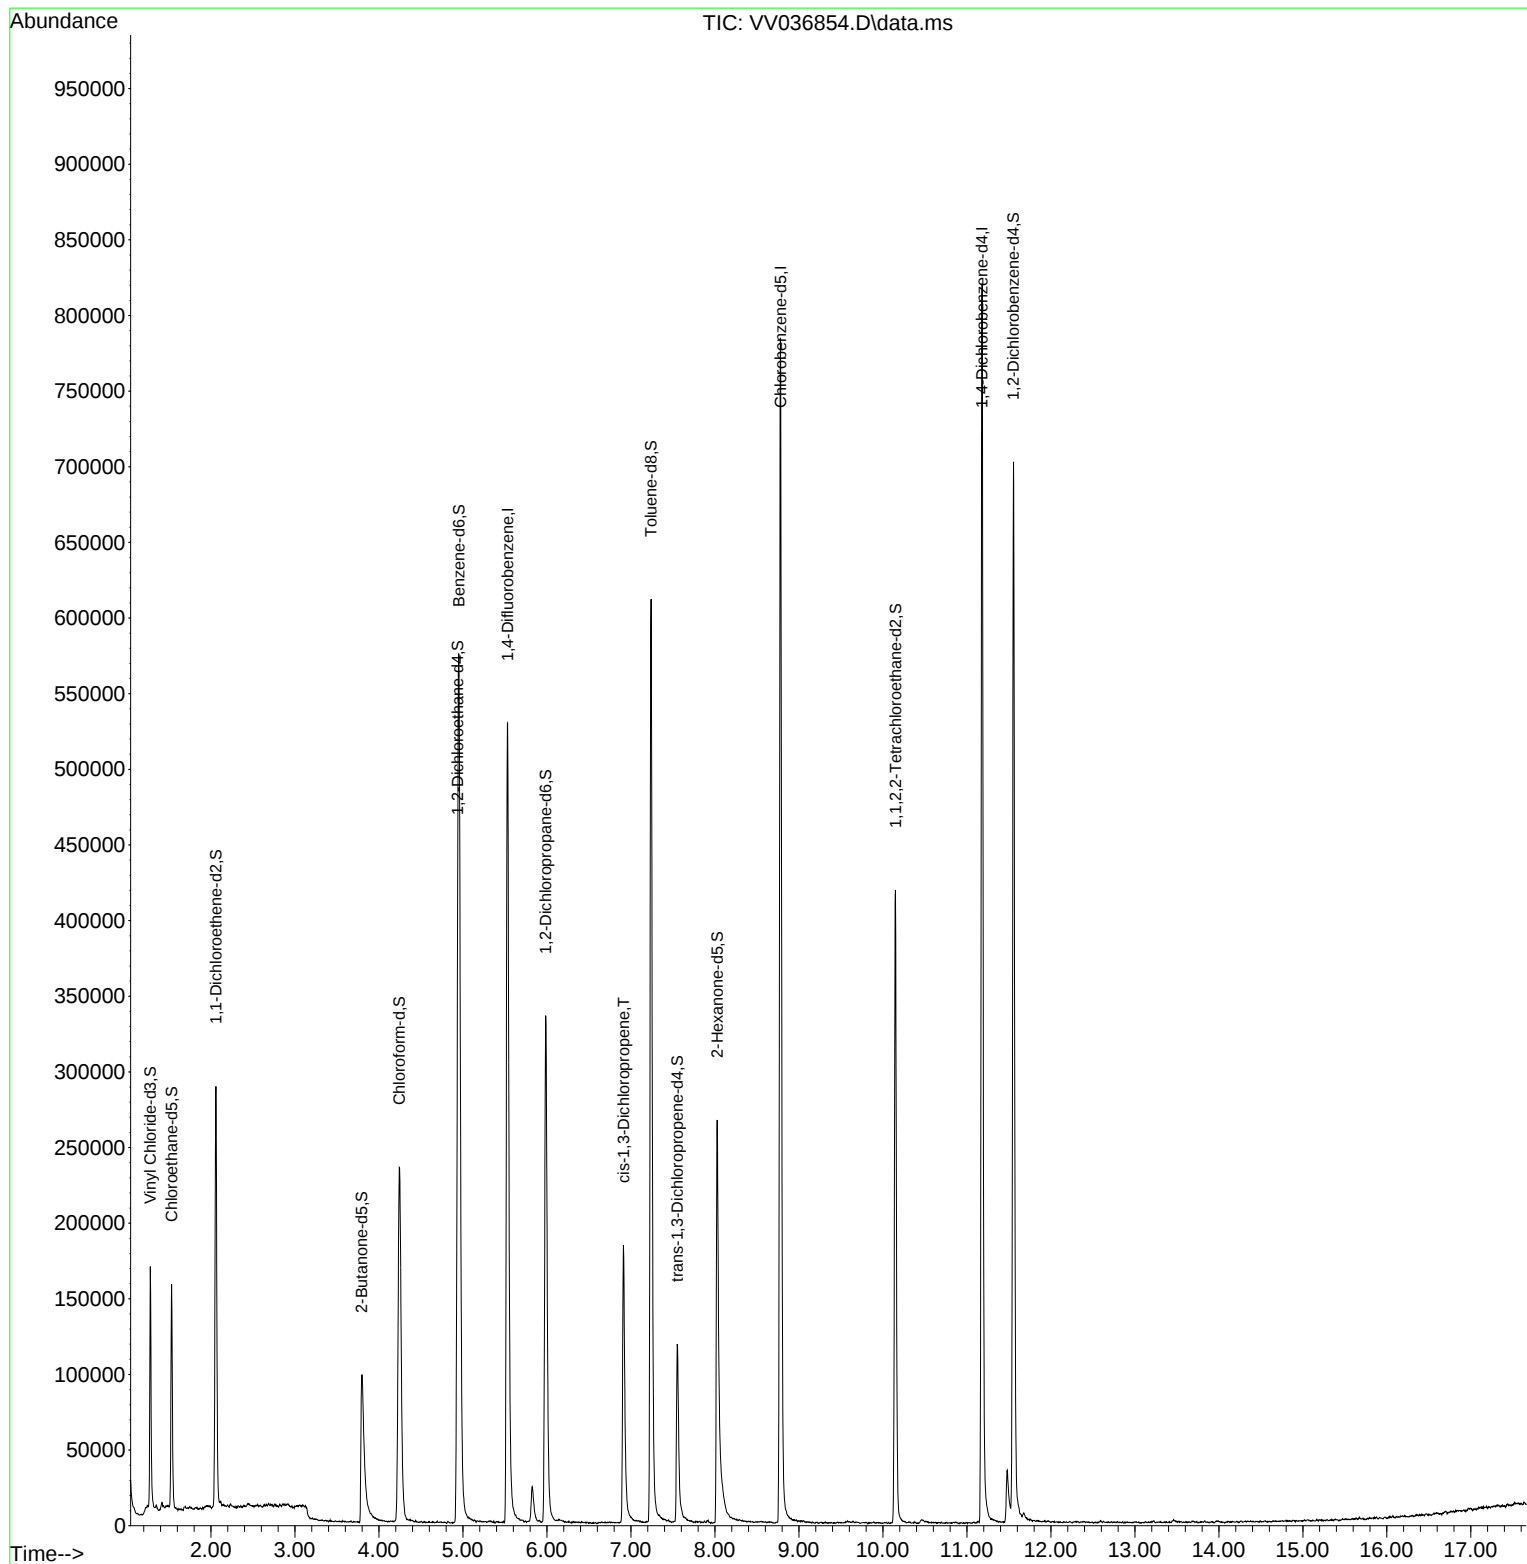

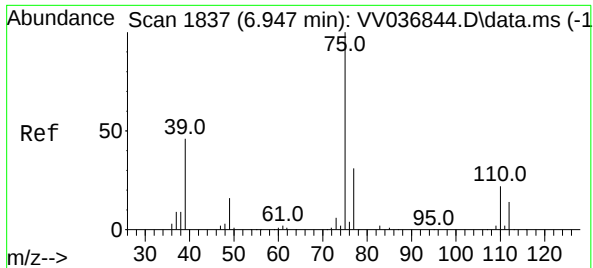

#39
 cis-1,3-Dichloropropene
 Concen: 0.923 ug/L
 RT: 6.911 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV036854.D
 Acq: 08 Aug 2024 16:03

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 5362
 Ion Ratio Lower Upper
 75 100
 77 57.8 22.2 41.2#

