

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036859.D
 Acq On : 08 Aug 2024 17:52
 Operator : SY/MD
 Sample : P3480-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Quant Time: Aug 09 02:45:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 09 02:41:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	441317	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	413587	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	199089	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	97247	27.589	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	55.180%#
7) Chloroethane-d5	1.532	69	92784	33.379	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	66.760%#
11) 1,1-Dichloroethene-d2	2.060	65	45966	30.486	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.980%
21) 2-Butanone-d5	3.796	46	159392	85.347	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.350%
24) Chloroform-d	4.246	84	238170	37.652	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.300%
26) 1,2-Dichloroethane-d4	4.940	65	161015	39.591	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.180%
32) Benzene-d6	4.953	84	458077	36.670	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.340%
36) 1,2-Dichloropropane-d6	5.985	67	162135	40.231	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	80.460%
41) Toluene-d8	7.239	98	389626	34.002	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	68.000%#
43) trans-1,3-Dichloroprop...	7.554	79	69066	32.930	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.860%
47) 2-Hexanone-d5	8.027	63	78054	67.360	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.360%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	180724	39.056	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.120%
66) 1,2-Dichlorobenzene-d4	11.554	152	168446	41.521	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.040%
Target Compounds						
13) Acetone	2.114	43	23719	15.180	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036859.D
Acq On : 08 Aug 2024 17:52
Operator : SY/MD
Sample : P3480-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6

Quant Time: Aug 09 02:45:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 09 02:41:02 2024
Response via : Initial Calibration

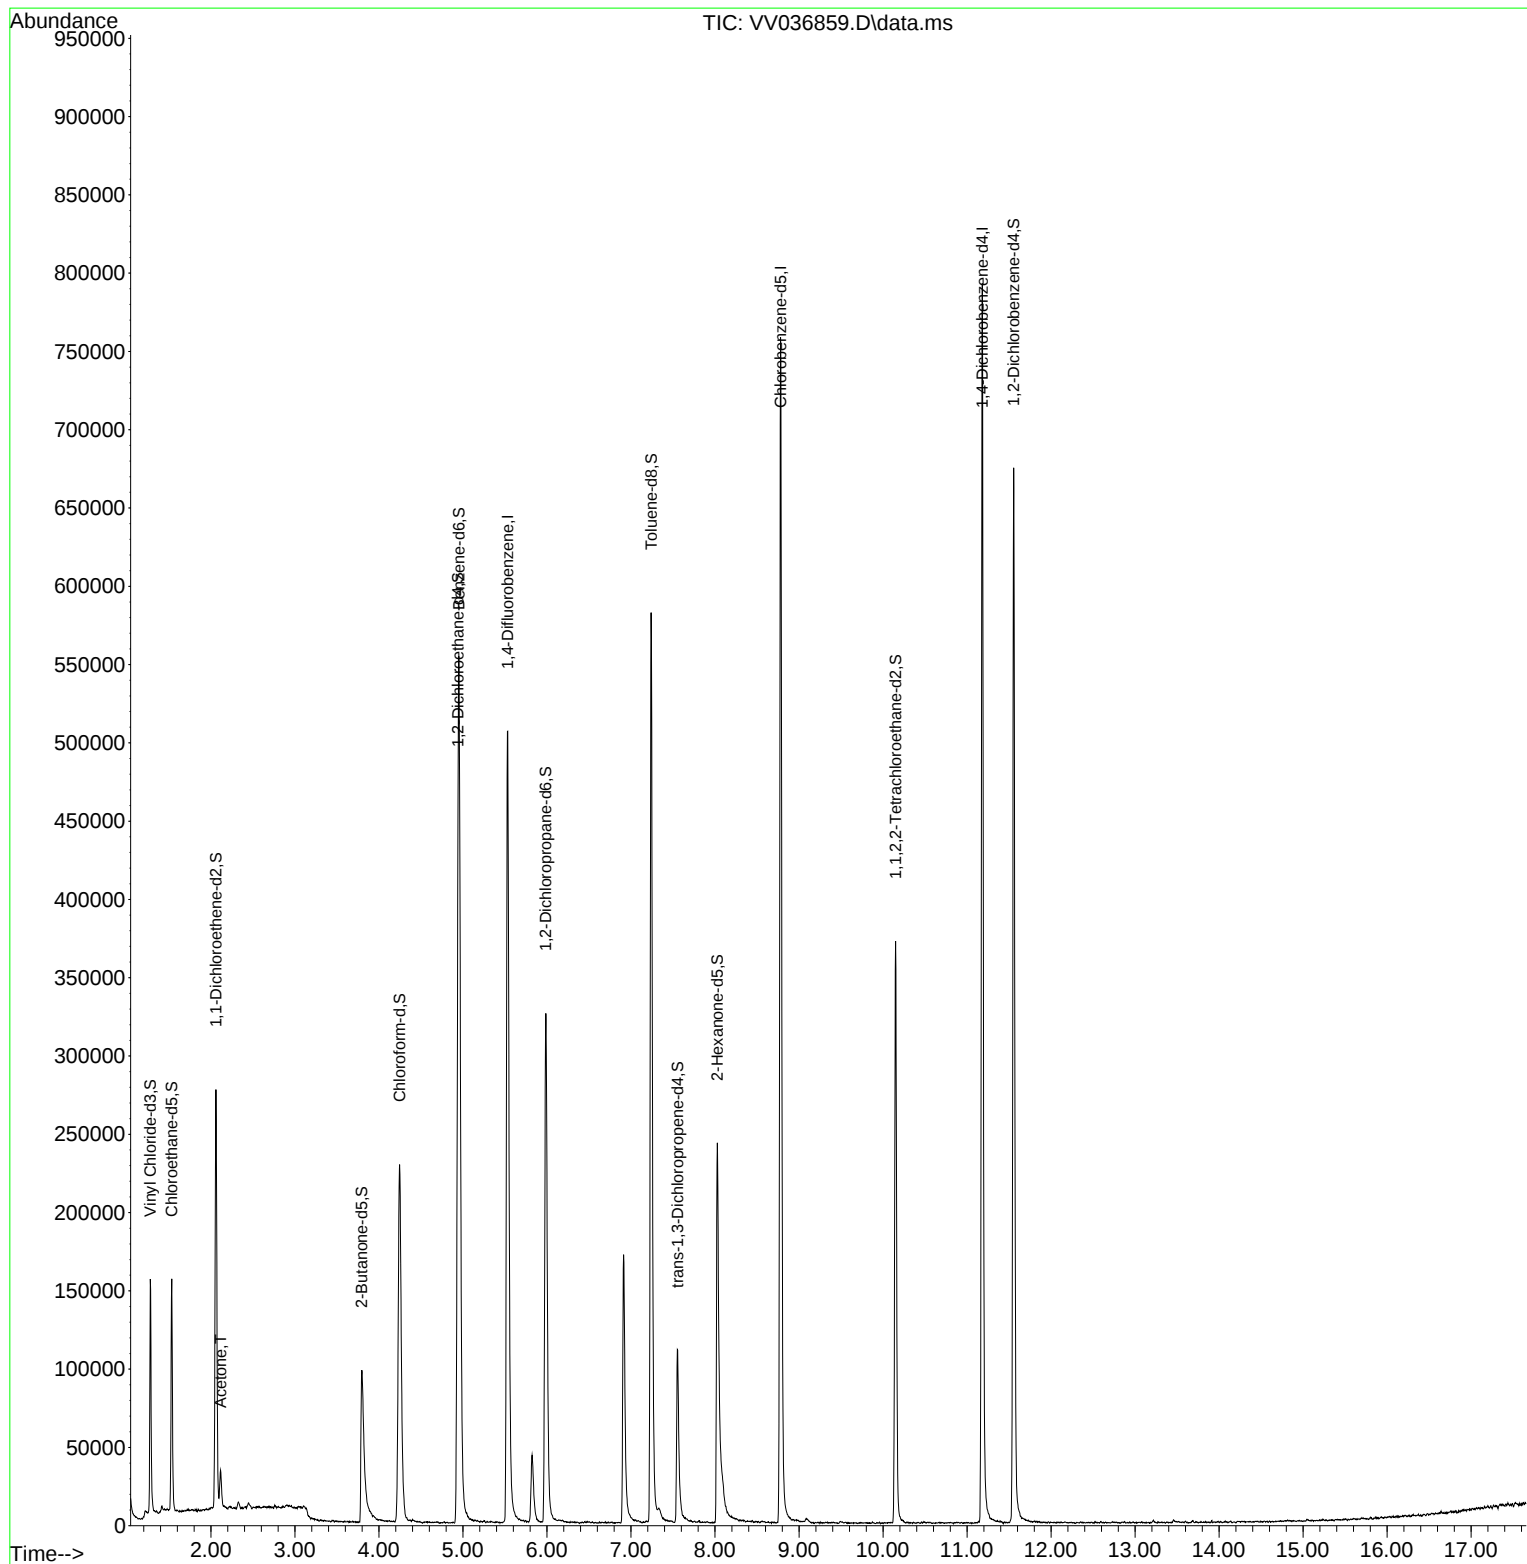

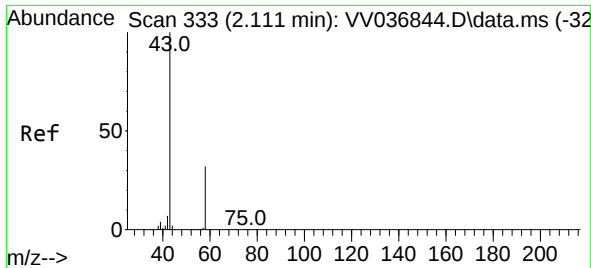

#13

Acetone

Concen: 15.180 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036859.D


Acq: 08 Aug 2024 17:52

Instrument :

MSVOA_V

ClientSampleId :

E0AA6

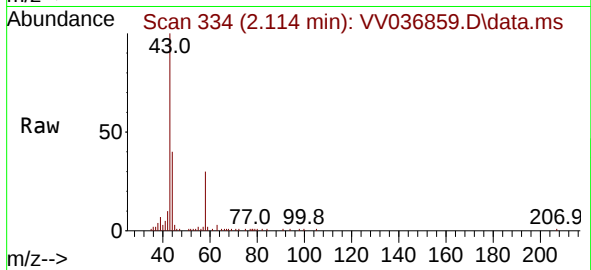

Tgt Ion: 43 Resp: 23719

Ion Ratio Lower Upper

43 100

58 31.7 0.0 63.4

