

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036857.D
 Acq On : 08 Aug 2024 17:08
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	147446	157187	11.09%	1.403%
2	1.532	147	153	165	rVB	137959	161811	11.41%	1.444%
3	2.060	309	317	328	rBV	259321	358322	25.28%	3.199%
4	3.799	849	858	884	rBV2	88329	261988	18.48%	2.339%
5	4.246	983	997	1025	rVB	226679	575109	40.57%	5.134%
6	4.677	1128	1131	1133	rBV3	1137	415	0.03%	0.004%
7	4.706	1138	1140	1143	rBV2	656	525	0.04%	0.005%
8	4.950	1201	1216	1251	rBV2	554639	1417681	100.00%	12.655%
9	5.375	1344	1348	1354	rBV5	891	1007	0.07%	0.009%
10	5.529	1385	1396	1431	rBV	509500	1052209	74.22%	9.393%
11	5.821	1477	1487	1506	rBV3	43652	98999	6.98%	0.884%
12	5.985	1527	1538	1567	rBV	321972	666236	46.99%	5.947%
13	6.349	1649	1651	1655	rVB4	883	428	0.03%	0.004%
14	6.387	1661	1663	1666	rVB2	519	283	0.02%	0.003%
15	6.603	1725	1730	1734	rBV6	806	974	0.07%	0.009%
16	6.632	1736	1739	1741	rBV3	271	183	0.01%	0.002%
17	6.654	1743	1746	1752	rVB4	921	916	0.06%	0.008%
18	6.725	1765	1768	1769	rBV3	657	392	0.03%	0.003%
19	6.911	1816	1826	1851	rBV	172383	337636	23.82%	3.014%
20	7.239	1917	1928	1949	rBV	595827	1047536	73.89%	9.351%
21	7.551	2017	2025	2062	rBV	112151	215705	15.22%	1.926%
22	7.850	2116	2118	2119	rBV2	504	192	0.01%	0.002%
23	7.911	2133	2137	2140	rBV5	943	754	0.05%	0.007%
24	7.979	2154	2158	2160	rBV3	680	586	0.04%	0.005%
25	8.027	2165	2173	2222	rVV2	243155	578353	40.80%	5.163%
26	8.731	2389	2392	2394	rBV4	639	469	0.03%	0.004%
27	8.780	2396	2407	2443	rVV	784907	1286938	90.78%	11.488%
28	9.191	2533	2535	2537	rBV2	564	405	0.03%	0.004%
29	9.239	2546	2550	2552	rBV3	387	297	0.02%	0.003%
30	9.259	2552	2556	2558	rVB4	559	426	0.03%	0.004%
31	9.300	2568	2569	2574	rVB2	756	441	0.03%	0.004%
32	9.403	2599	2601	2603	rBV2	551	317	0.02%	0.003%
33	9.487	2624	2627	2629	rBV2	1110	716	0.05%	0.006%
34	9.535	2640	2642	2644	rBV3	494	289	0.02%	0.003%
35	9.548	2644	2646	2650	rVB3	1039	504	0.04%	0.004%
36	9.571	2650	2653	2655	rBV3	399	269	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036857.D
 Acq On : 08 Aug 2024 17:08
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.616	2660	2667	2669	rBV5	661	858	0.06%	0.008%
38	9.644	2674	2676	2678	rVB2	520	210	0.01%	0.002%
39	9.677	2685	2686	2687	rBV2	200	55	0.00%	0.000%
40	9.686	2687	2689	2691	rVV2	442	199	0.01%	0.002%
41	9.696	2691	2692	2694	rVV	347	157	0.01%	0.001%
42	9.709	2694	2696	2700	rVB2	558	377	0.03%	0.003%
43	9.735	2700	2704	2706	rBV3	752	407	0.03%	0.004%
44	9.747	2706	2708	2709	rBV	256	110	0.01%	0.001%
45	9.808	2721	2727	2730	rBV4	735	800	0.06%	0.007%
46	9.847	2737	2739	2740	rBV2	526	203	0.01%	0.002%
47	9.879	2748	2749	2753	rVB4	863	444	0.03%	0.004%
48	9.898	2753	2755	2756	rBV2	740	272	0.02%	0.002%
49	9.934	2763	2766	2767	rBV2	277	178	0.01%	0.002%
50	9.944	2767	2769	2773	rVV2	593	393	0.03%	0.004%
51	9.963	2773	2775	2777	rVV3	476	236	0.02%	0.002%
52	9.976	2777	2779	2781	rVB	540	198	0.01%	0.002%
53	9.998	2783	2786	2790	rVB3	527	337	0.02%	0.003%
54	10.021	2790	2793	2797	rVB3	1048	745	0.05%	0.007%
55	10.046	2797	2801	2805	rBV5	1179	978	0.07%	0.009%
56	10.149	2820	2833	2852	rBV	368794	585843	41.32%	5.230%
57	10.387	2905	2907	2909	rBV2	483	160	0.01%	0.001%
58	10.452	2924	2927	2931	rBV4	771	551	0.04%	0.005%
59	10.535	2948	2953	2954	rBV2	598	431	0.03%	0.004%
60	10.596	2967	2972	2977	rBV5	1002	1060	0.07%	0.009%
61	10.657	2987	2991	2994	rBV4	887	717	0.05%	0.006%
62	10.699	2999	3004	3008	rBV4	1012	836	0.06%	0.007%
63	10.731	3008	3014	3018	rBV3	769	656	0.05%	0.006%
64	10.751	3018	3020	3024	rBV4	582	383	0.03%	0.003%
65	10.834	3045	3046	3049	rVB	597	278	0.02%	0.002%
66	10.857	3049	3053	3057	rBV5	1007	1118	0.08%	0.010%
67	10.953	3080	3083	3085	rBV2	520	317	0.02%	0.003%
68	10.985	3089	3093	3094	rBV3	530	385	0.03%	0.003%
69	10.998	3094	3097	3099	rVB3	372	218	0.02%	0.002%
70	11.021	3102	3104	3108	rVB2	665	413	0.03%	0.004%
71	11.046	3108	3112	3115	rBV3	625	499	0.04%	0.004%
72	11.117	3132	3134	3135	rBV	363	154	0.01%	0.001%
73	11.133	3135	3139	3143	rBV4	1385	1275	0.09%	0.011%
74	11.181	3143	3154	3188	rVV	805378	1269758	89.57%	11.335%
75	11.509	3243	3256	3258	rBV9	3459	5749	0.41%	0.051%
76	11.554	3260	3270	3298	rVV	686749	1088904	76.81%	9.720%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036857.D
 Acq On : 08 Aug 2024 17:08
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.098	3437	3439	3442	rBV2	325	196	0.01%	0.002%
78	12.136	3448	3451	3454	rBV2	905	680	0.05%	0.006%
79	12.152	3454	3456	3459	rBV4	655	465	0.03%	0.004%
80	12.201	3468	3471	3473	rBV3	724	403	0.03%	0.004%
81	12.326	3508	3510	3513	rBV3	1002	506	0.04%	0.005%
82	12.374	3523	3525	3528	rVB4	531	246	0.02%	0.002%
83	12.394	3528	3531	3534	rBV3	516	379	0.03%	0.003%
84	12.522	3569	3571	3572	rBV2	529	195	0.01%	0.002%
85	12.570	3584	3586	3587	rBV	547	178	0.01%	0.002%
86	12.612	3597	3599	3603	rVB3	662	310	0.02%	0.003%
87	12.689	3621	3623	3626	rVB2	532	227	0.02%	0.002%
88	12.786	3650	3653	3655	rBV2	808	476	0.03%	0.004%
89	12.947	3701	3703	3704	rBV2	274	90	0.01%	0.001%
90	12.959	3704	3707	3715	rVB5	1099	1248	0.09%	0.011%
91	12.992	3715	3717	3718	rBV	921	424	0.03%	0.004%
92	13.066	3737	3740	3741	rBV3	583	270	0.02%	0.002%
93	13.146	3763	3765	3768	rBV3	647	290	0.02%	0.003%
94	13.168	3770	3772	3774	rBV2	697	307	0.02%	0.003%
95	13.210	3782	3785	3787	rBV4	822	565	0.04%	0.005%
96	13.313	3812	3817	3820	rBV5	886	937	0.07%	0.008%
97	13.429	3850	3853	3854	rBV5	699	337	0.02%	0.003%
98	14.326	4129	4132	4133	rBV3	595	369	0.03%	0.003%



Sum of corrected areas: 11202458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036857.D
Acq On : 08 Aug 2024 17:08
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

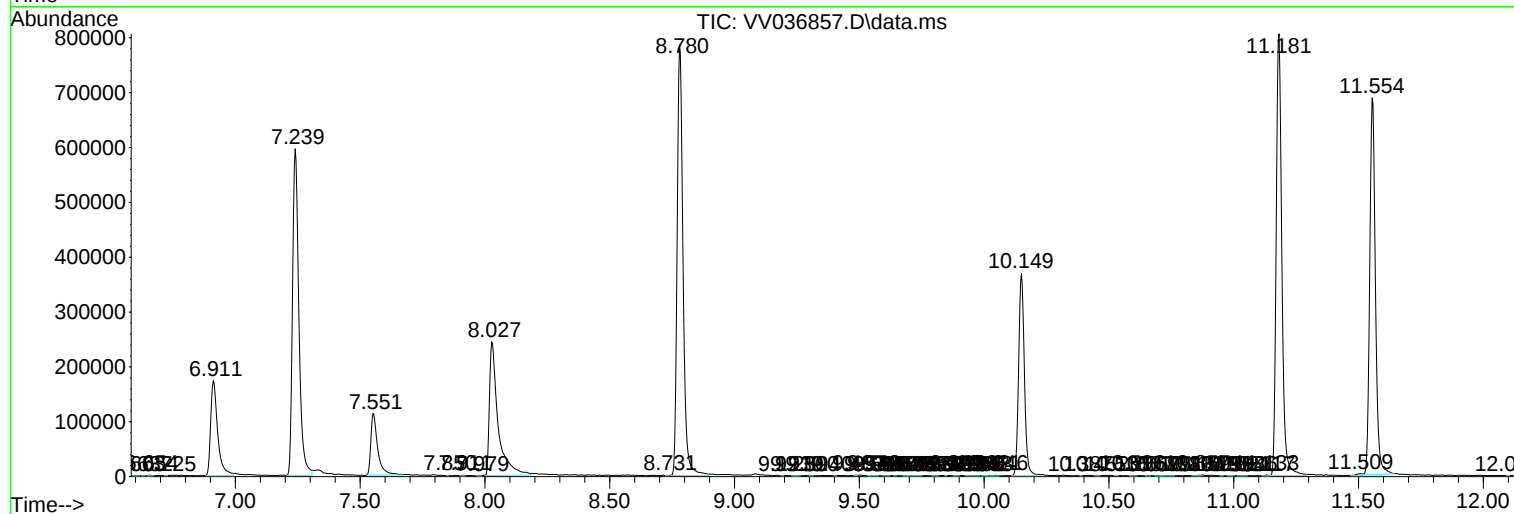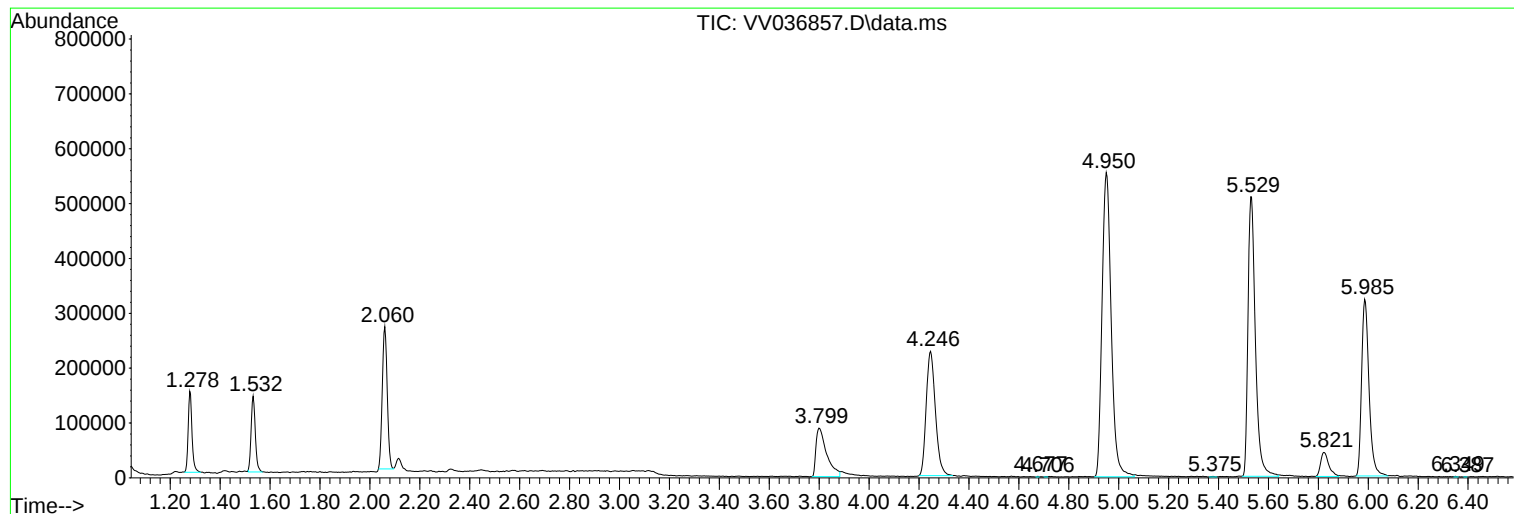

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036857.D
Acq On : 08 Aug 2024 17:08
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036857.D
Acq On : 08 Aug 2024 17:08
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc