

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036858.D
 Acq On : 08 Aug 2024 17:30
 Operator : SY/MD
 Sample : P3480-22
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036858.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	151361	160659	11.40%	1.442%
2	1.532	147	153	166	rVB	143869	169305	12.02%	1.520%
3	2.059	308	317	329	rBV	264054	379738	26.95%	3.409%
4	3.632	802	806	811	rBV2	931	1003	0.07%	0.009%
5	3.796	849	857	893	rBV	93270	266982	18.95%	2.397%
6	4.246	981	997	1028	rBV	227590	589272	41.83%	5.290%
7	4.542	1087	1089	1091	rBV2	735	432	0.03%	0.004%
8	4.638	1115	1119	1127	rBV5	854	1145	0.08%	0.010%
9	4.809	1165	1172	1176	rVB6	890	1302	0.09%	0.012%
10	4.828	1176	1178	1181	rBV	923	553	0.04%	0.005%
11	4.841	1181	1182	1184	rVV2	469	134	0.01%	0.001%
12	4.886	1194	1196	1198	rBV2	751	451	0.03%	0.004%
13	4.950	1201	1216	1254	rVV2	549774	1408864	100.00%	12.649%
14	5.532	1386	1397	1425	rBV	506980	1035292	73.48%	9.295%
15	5.821	1477	1487	1508	rBV2	45096	98265	6.97%	0.882%
16	5.985	1526	1538	1570	rBV	324114	674733	47.89%	6.058%
17	6.304	1634	1637	1638	rBV3	724	355	0.03%	0.003%
18	6.481	1690	1692	1696	rBV5	912	690	0.05%	0.006%
19	6.519	1702	1704	1708	rBV3	661	497	0.04%	0.004%
20	6.590	1722	1726	1730	rBV3	602	622	0.04%	0.006%
21	6.609	1730	1732	1736	rVB2	711	443	0.03%	0.004%
22	6.635	1736	1740	1742	rBV3	493	310	0.02%	0.003%
23	6.673	1751	1752	1756	rBV3	475	290	0.02%	0.003%
24	6.715	1763	1765	1767	rBV	511	243	0.02%	0.002%
25	6.757	1776	1778	1780	rBV3	575	309	0.02%	0.003%
26	6.857	1800	1809	1812	rBV4	891	1265	0.09%	0.011%
27	6.873	1812	1814	1816	rBV2	646	323	0.02%	0.003%
28	6.911	1816	1826	1850	rBV	173773	332922	23.63%	2.989%
29	7.239	1917	1928	1948	rBV	588974	1034464	73.43%	9.287%
30	7.551	2017	2025	2050	rBV	111121	211380	15.00%	1.898%
31	7.902	2132	2134	2135	rBV2	839	289	0.02%	0.003%
32	7.979	2151	2158	2164	rBV7	706	927	0.07%	0.008%
33	8.027	2164	2173	2215	rBV2	244152	572253	40.62%	5.138%
34	8.718	2386	2388	2390	rBV2	588	322	0.02%	0.003%
35	8.779	2397	2407	2438	rBV	757839	1252522	88.90%	11.245%
36	9.207	2536	2540	2544	rVB4	1280	1248	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036858.D
 Acq On : 08 Aug 2024 17:30
 Operator : SY/MD
 Sample : P3480-22
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.233	2544	2548	2551	rBV4	712	549	0.04%	0.005%
38	9.249	2551	2553	2555	rBV3	691	416	0.03%	0.004%
39	9.339	2577	2581	2583	rBV4	462	344	0.02%	0.003%
40	9.358	2583	2587	2590	rBV4	678	675	0.05%	0.006%
41	9.397	2596	2599	2600	rBV	759	299	0.02%	0.003%
42	9.432	2606	2610	2612	rVB3	692	497	0.04%	0.004%
43	9.445	2612	2614	2615	rBV	331	130	0.01%	0.001%
44	9.558	2644	2649	2653	rVB6	923	844	0.06%	0.008%
45	9.587	2655	2658	2660	rBV3	812	507	0.04%	0.005%
46	9.638	2671	2674	2676	rBV2	615	376	0.03%	0.003%
47	9.667	2681	2683	2688	rVB5	804	522	0.04%	0.005%
48	9.744	2706	2707	2709	rBV	604	250	0.02%	0.002%
49	9.799	2723	2724	2726	rBV2	357	116	0.01%	0.001%
50	9.873	2745	2747	2756	rVB5	920	871	0.06%	0.008%
51	9.985	2779	2782	2785	rBV3	362	243	0.02%	0.002%
52	10.001	2785	2787	2790	rVB3	600	299	0.02%	0.003%
53	10.017	2790	2792	2793	rBV	401	155	0.01%	0.001%
54	10.027	2793	2795	2796	rBV2	341	119	0.01%	0.001%
55	10.075	2808	2810	2811	rVB	366	100	0.01%	0.001%
56	10.098	2814	2817	2819	rBV2	619	258	0.02%	0.002%
57	10.149	2822	2833	2852	rBV	362648	579509	41.13%	5.203%
58	10.361	2895	2899	2902	rVB4	713	551	0.04%	0.005%
59	10.384	2902	2906	2910	rBV5	899	933	0.07%	0.008%
60	10.474	2931	2934	2937	rBV3	927	694	0.05%	0.006%
61	10.513	2944	2946	2949	rVV3	696	371	0.03%	0.003%
62	10.529	2949	2951	2955	rVB4	682	375	0.03%	0.003%
63	10.545	2955	2956	2957	rBV	215	50	0.00%	0.000%
64	10.631	2981	2983	2984	rBV2	481	150	0.01%	0.001%
65	10.641	2984	2986	2991	rVV3	393	284	0.02%	0.003%
66	10.680	2997	2998	3000	rVB2	217	48	0.00%	0.000%
67	10.696	3000	3003	3004	rVB	390	131	0.01%	0.001%
68	10.709	3004	3007	3010	rBV3	452	302	0.02%	0.003%
69	10.738	3013	3016	3017	rBV2	549	266	0.02%	0.002%
70	10.773	3024	3027	3029	rBV2	458	214	0.02%	0.002%
71	10.792	3029	3033	3034	rVV3	603	341	0.02%	0.003%
72	10.840	3044	3048	3049	rBV2	762	350	0.02%	0.003%
73	10.908	3065	3069	3072	rVB4	526	417	0.03%	0.004%
74	10.924	3072	3074	3076	rBV2	485	158	0.01%	0.001%
75	10.982	3090	3092	3094	rBV3	343	174	0.01%	0.002%
76	11.043	3109	3111	3112	rBV	312	93	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036858.D
Acq On : 08 Aug 2024 17:30
Operator : SY/MD
Sample : P3480-22
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis

77	11.181	3143	3154	3190	rBV	775836	1234573	87.63%	11.084%
78	11.490	3241	3250	3259	rBV5	12085	25115	1.78%	0.225%
79	11.554	3261	3270	3300	rVB	665638	1075755	76.36%	9.658%
80	11.947	3390	3392	3395	rVB4	632	367	0.03%	0.003%
81	11.975	3395	3401	3403	rBV6	1338	1192	0.08%	0.011%
82	12.152	3453	3456	3460	rBV4	698	466	0.03%	0.004%
83	12.172	3460	3462	3466	rBV3	1074	615	0.04%	0.006%
84	12.220	3473	3477	3481	rBV4	673	755	0.05%	0.007%
85	12.258	3485	3489	3490	rBV2	725	393	0.03%	0.004%
86	12.287	3495	3498	3500	rBV2	666	471	0.03%	0.004%
87	12.316	3505	3507	3510	rBV3	411	209	0.01%	0.002%
88	12.493	3560	3562	3566	rBV2	834	571	0.04%	0.005%
89	12.596	3589	3594	3596	rBV5	998	1007	0.07%	0.009%
90	12.705	3625	3628	3632	rBV6	599	478	0.03%	0.004%
91	12.789	3651	3654	3659	rVB2	621	437	0.03%	0.004%
92	12.850	3671	3673	3676	rBV2	719	437	0.03%	0.004%
93	12.914	3691	3693	3695	rBV2	401	172	0.01%	0.002%
94	12.982	3710	3714	3719	rVB4	563	604	0.04%	0.005%
95	13.146	3764	3765	3768	rBV3	441	266	0.02%	0.002%
96	13.599	3901	3906	3909	rBV3	1054	1020	0.07%	0.009%
97	13.799	3966	3968	3971	rVB2	657	328	0.02%	0.003%
98	14.204	4091	4094	4095	rBV	1107	541	0.04%	0.005%




Sum of corrected areas: 11138557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036858.D
Acq On : 08 Aug 2024 17:30
Operator : SY/MD
Sample : P3480-22
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

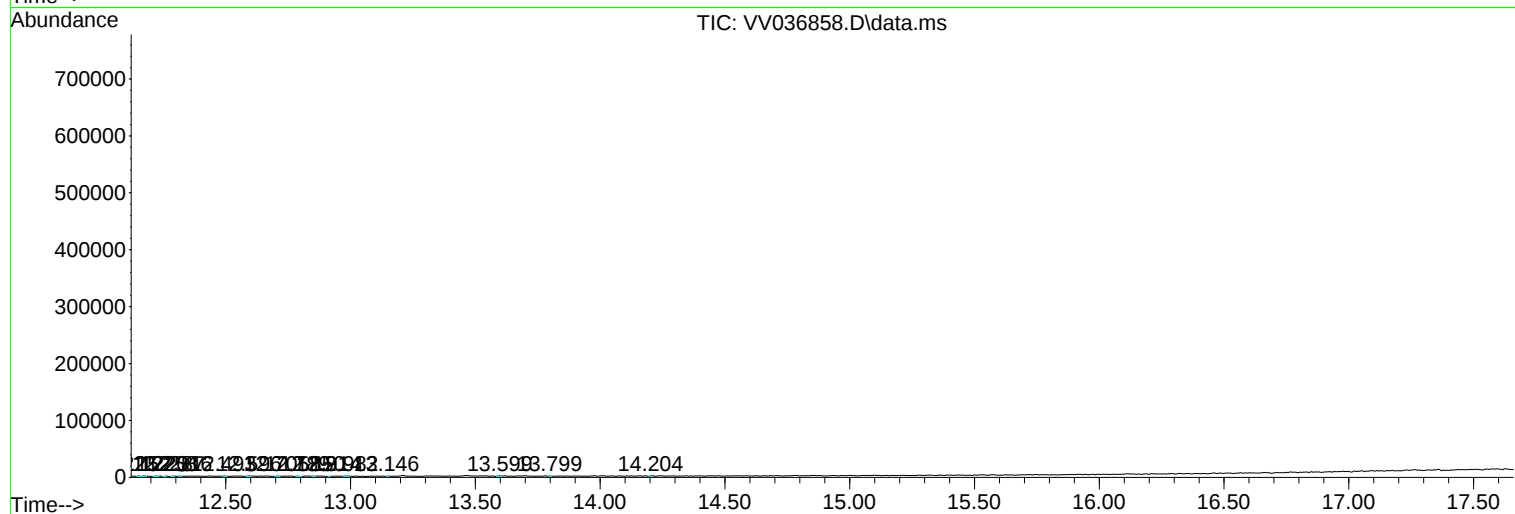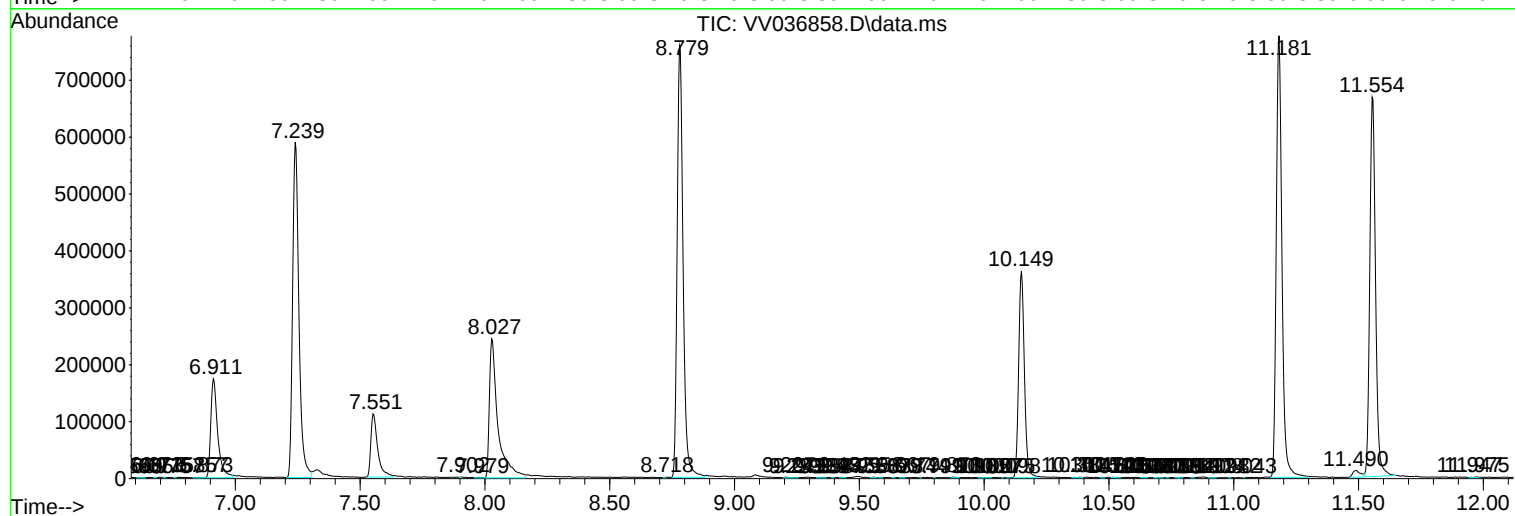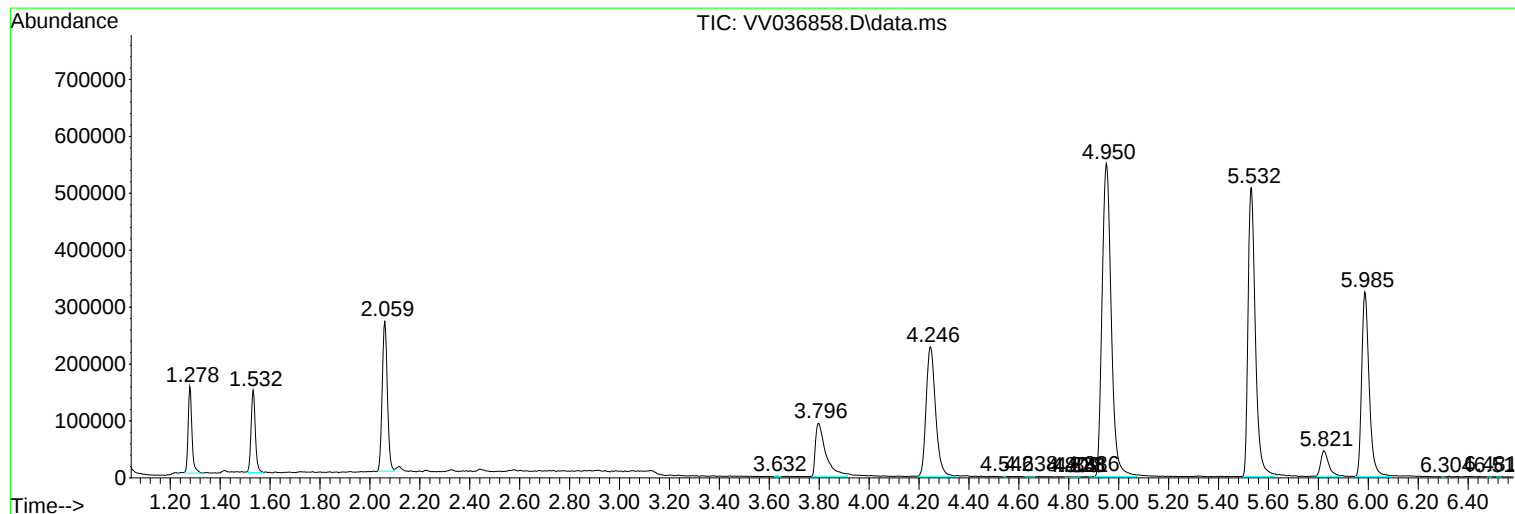

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036858.D
Acq On : 08 Aug 2024 17:30
Operator : SY/MD
Sample : P3480-22
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036858.D
Acq On : 08 Aug 2024 17:30
Operator : SY/MD
Sample : P3480-22
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc