

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036859.D
 Acq On : 08 Aug 2024 17:52
 Operator : SY/MD
 Sample : P3480-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036859.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	148149	156099	11.15%	1.409%
2	1.532	147	153	166	rVB	148051	170636	12.19%	1.540%
3	2.060	309	317	328	rBV	262186	364001	26.01%	3.285%
4	3.477	756	758	762	rBV4	1000	793	0.06%	0.007%
5	3.593	790	794	797	rBV3	938	731	0.05%	0.007%
6	3.648	809	811	813	rBV2	662	269	0.02%	0.002%
7	3.796	849	857	886	rBV	97055	265329	18.96%	2.394%
8	4.246	982	997	1021	rBV	227195	577654	41.28%	5.213%
9	4.532	1081	1086	1088	rBV3	867	734	0.05%	0.007%
10	4.838	1177	1181	1185	rBV4	278	232	0.02%	0.002%
11	4.857	1185	1187	1191	rBV4	392	341	0.02%	0.003%
12	4.950	1200	1216	1244	rBV2	553641	1399405	100.00%	12.628%
13	5.384	1349	1351	1353	rVB2	654	228	0.02%	0.002%
14	5.445	1368	1370	1373	rBV3	514	359	0.03%	0.003%
15	5.532	1386	1397	1428	rBV	503782	1035599	74.00%	9.345%
16	5.821	1478	1487	1505	rBV2	41508	88169	6.30%	0.796%
17	5.985	1526	1538	1572	rBV	324730	676488	48.34%	6.104%
18	6.358	1650	1654	1662	rVB7	994	1590	0.11%	0.014%
19	6.394	1662	1665	1667	rBV2	635	448	0.03%	0.004%
20	6.477	1689	1691	1694	rBV4	731	361	0.03%	0.003%
21	6.538	1708	1710	1715	rVB5	998	694	0.05%	0.006%
22	6.574	1715	1721	1722	rBV5	476	393	0.03%	0.004%
23	6.657	1744	1747	1751	rBV4	448	418	0.03%	0.004%
24	6.686	1754	1756	1758	rBV3	528	275	0.02%	0.002%
25	6.715	1762	1765	1767	rBV4	713	445	0.03%	0.004%
26	6.911	1815	1826	1854	rBV	171422	333131	23.81%	3.006%
27	7.239	1918	1928	1951	rBV	580113	1022578	73.07%	9.228%
28	7.551	2014	2025	2045	rBV	110439	207574	14.83%	1.873%
29	7.972	2154	2156	2159	rBV4	688	331	0.02%	0.003%
30	8.027	2164	2173	2209	rBV2	242456	552961	39.51%	4.990%
31	8.548	2331	2335	2337	rBV4	871	766	0.05%	0.007%
32	8.680	2374	2376	2379	rBV3	768	656	0.05%	0.006%
33	8.706	2382	2384	2388	rVB5	693	416	0.03%	0.004%
34	8.780	2397	2407	2437	rBV	756860	1265367	90.42%	11.418%
35	9.194	2531	2536	2539	rBV3	807	754	0.05%	0.007%
36	9.239	2548	2550	2553	rVB3	848	489	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036859.D
 Acq On : 08 Aug 2024 17:52
 Operator : SY/MD
 Sample : P3480-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.259	2553	2556	2558	rBV3	883	521	0.04%	0.005%
38	9.288	2561	2565	2567	rBV4	528	389	0.03%	0.004%
39	9.355	2584	2586	2589	rBV2	429	259	0.02%	0.002%
40	9.384	2593	2595	2598	rBV4	566	316	0.02%	0.003%
41	9.403	2598	2601	2602	rBV3	458	230	0.02%	0.002%
42	9.493	2621	2629	2633	rBV5	1385	1975	0.14%	0.018%
43	9.580	2654	2656	2658	rBV2	653	284	0.02%	0.003%
44	9.593	2658	2660	2664	rVB3	666	321	0.02%	0.003%
45	9.619	2664	2668	2672	rBV4	478	512	0.04%	0.005%
46	9.731	2701	2703	2704	rBV2	536	258	0.02%	0.002%
47	9.799	2722	2724	2728	rVB2	515	240	0.02%	0.002%
48	9.873	2744	2747	2752	rBV2	817	549	0.04%	0.005%
49	9.924	2760	2763	2767	rBV5	648	535	0.04%	0.005%
50	9.956	2771	2773	2776	rVB3	934	520	0.04%	0.005%
51	9.972	2776	2778	2780	rBV	345	209	0.01%	0.002%
52	10.008	2787	2789	2790	rBV	505	254	0.02%	0.002%
53	10.069	2803	2808	2813	rBV6	598	619	0.04%	0.006%
54	10.095	2813	2816	2818	rBV	621	418	0.03%	0.004%
55	10.149	2822	2833	2856	rBV	371393	588737	42.07%	5.313%
56	10.284	2872	2875	2877	rBV4	531	302	0.02%	0.003%
57	10.320	2883	2886	2888	rBV3	753	556	0.04%	0.005%
58	10.365	2895	2900	2903	rBV4	779	715	0.05%	0.006%
59	10.406	2909	2913	2915	rBV4	677	544	0.04%	0.005%
60	10.461	2924	2930	2932	rBV4	1028	772	0.06%	0.007%
61	10.484	2932	2937	2939	rBV5	1055	796	0.06%	0.007%
62	10.558	2957	2960	2966	rVB5	701	704	0.05%	0.006%
63	10.603	2969	2974	2976	rBV3	430	376	0.03%	0.003%
64	10.632	2981	2983	2986	rBV3	418	236	0.02%	0.002%
65	10.683	2997	2999	3001	rBV2	546	233	0.02%	0.002%
66	10.705	3004	3006	3013	rVB4	690	746	0.05%	0.007%
67	10.741	3013	3017	3020	rBV4	465	451	0.03%	0.004%
68	10.847	3047	3050	3052	rBV2	733	515	0.04%	0.005%
69	10.879	3057	3060	3063	rVV4	493	421	0.03%	0.004%
70	10.966	3085	3087	3090	rVB3	587	289	0.02%	0.003%
71	10.988	3091	3094	3097	rVB4	504	309	0.02%	0.003%
72	11.062	3115	3117	3123	rBV3	653	618	0.04%	0.006%
73	11.095	3123	3127	3129	rBV4	550	378	0.03%	0.003%
74	11.136	3136	3140	3142	rBV6	1048	748	0.05%	0.007%
75	11.181	3142	3154	3177	rBV	791303	1249075	89.26%	11.271%
76	11.442	3232	3235	3238	rBV3	1129	969	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
 Data File : VV036859.D
 Acq On : 08 Aug 2024 17:52
 Operator : SY/MD
 Sample : P3480-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	11.554	3255	3270	3295	rBV	673701	1084964	77.53%	9.791%
78	11.966	3394	3398	3404	rBV5	881	882	0.06%	0.008%
79	11.992	3404	3406	3409	rBV3	563	372	0.03%	0.003%
80	12.111	3441	3443	3445	rBV3	539	271	0.02%	0.002%
81	12.303	3501	3503	3508	rBV2	588	577	0.04%	0.005%
82	12.390	3528	3530	3535	rBV2	609	485	0.03%	0.004%
83	12.474	3553	3556	3558	rBV4	637	478	0.03%	0.004%
84	12.503	3563	3565	3568	rVB3	388	210	0.02%	0.002%
85	12.522	3568	3571	3572	rBV3	1100	561	0.04%	0.005%
86	12.593	3588	3593	3597	rBV6	1051	1089	0.08%	0.010%
87	12.651	3606	3611	3614	rBV4	763	698	0.05%	0.006%
88	12.834	3664	3668	3670	rBV	648	494	0.04%	0.004%
89	12.908	3689	3691	3695	rVB3	440	235	0.02%	0.002%
90	12.937	3697	3700	3703	rVB4	803	563	0.04%	0.005%
91	13.014	3722	3724	3726	rVB3	665	257	0.02%	0.002%
92	13.181	3774	3776	3779	rBV3	767	585	0.04%	0.005%
93	13.271	3801	3804	3809	rBV4	1099	1045	0.07%	0.009%
94	13.374	3832	3836	3838	rBV4	872	691	0.05%	0.006%
95	13.403	3843	3845	3847	rBV	556	323	0.02%	0.003%
96	13.438	3854	3856	3858	rBV	472	226	0.02%	0.002%
97	13.458	3858	3862	3866	rBV7	1761	1833	0.13%	0.017%
98	13.673	3927	3929	3931	rBV2	837	501	0.04%	0.005%
99	13.840	3979	3981	3985	rVB3	874	538	0.04%	0.005%
100	14.114	4063	4066	4067	rBV	599	302	0.02%	0.003%




Sum of corrected areas: 11081793

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036859.D
Acq On : 08 Aug 2024 17:52
Operator : SY/MD
Sample : P3480-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

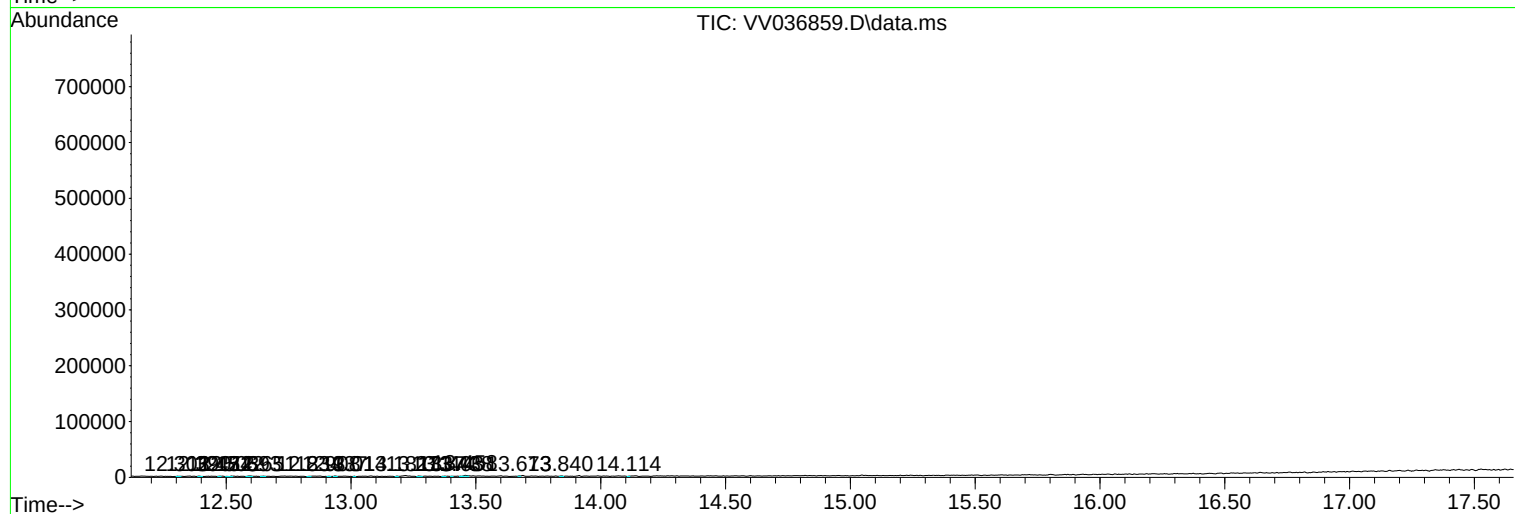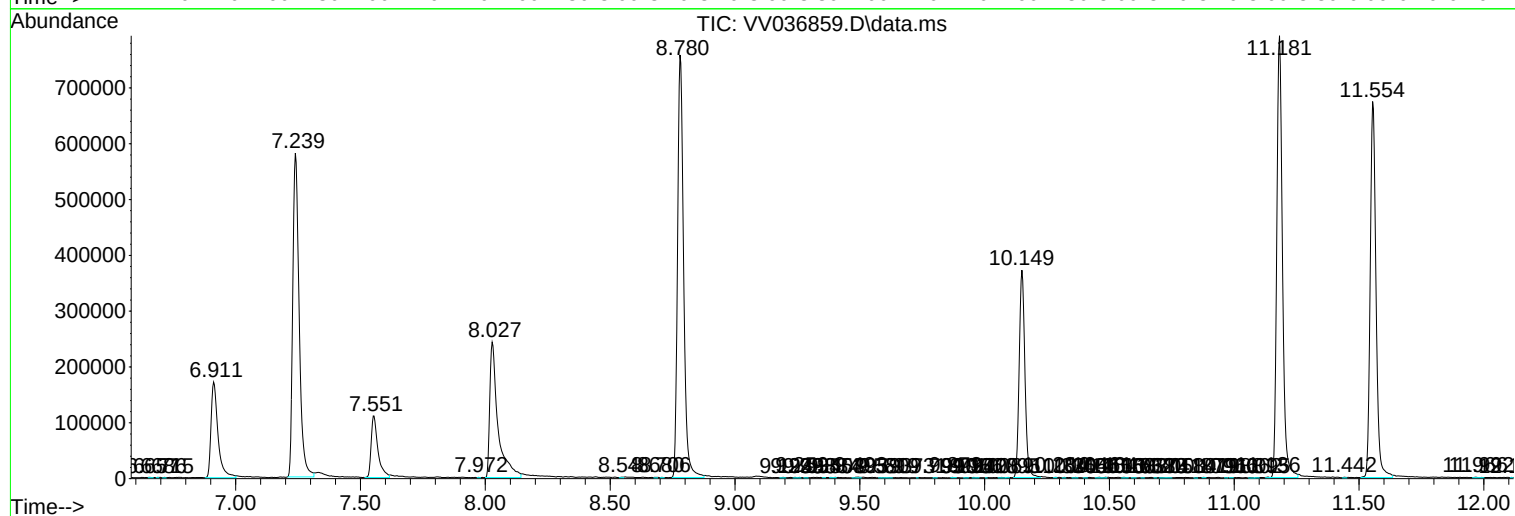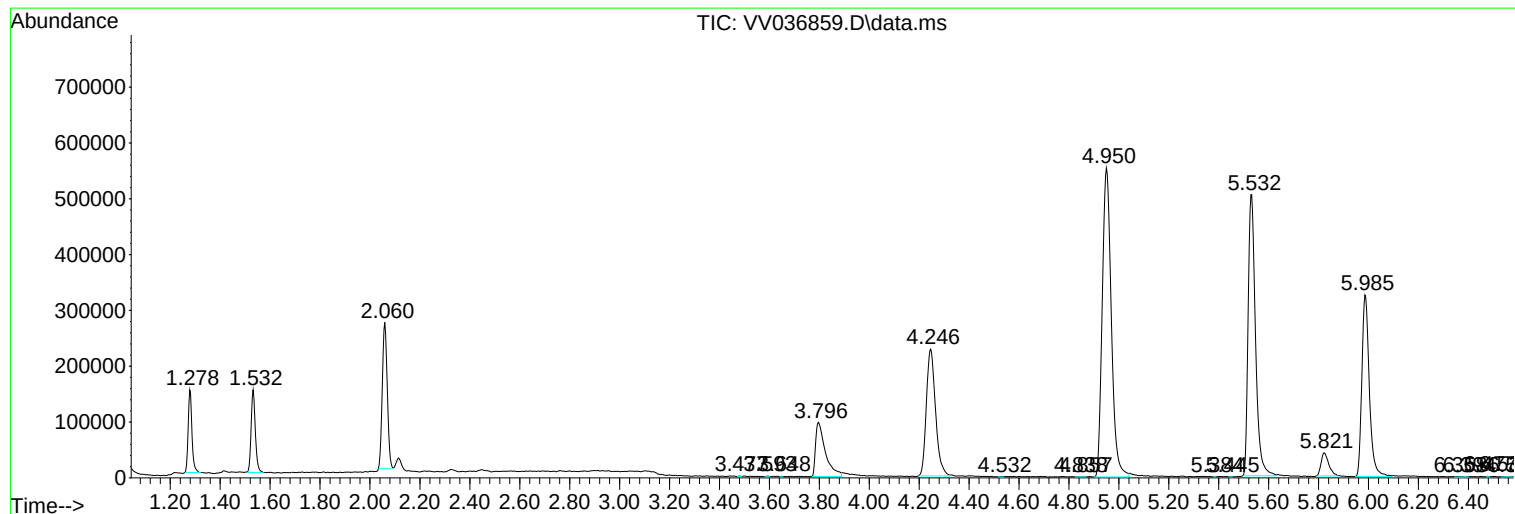

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036859.D
Acq On : 08 Aug 2024 17:52
Operator : SY/MD
Sample : P3480-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080824\
Data File : VV036859.D
Acq On : 08 Aug 2024 17:52
Operator : SY/MD
Sample : P3480-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
