

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036869.D
 Acq On : 09 Aug 2024 11:52
 Operator : SY/MD
 Sample : P3480-18RE
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB5RE

Quant Time: Aug 10 01:16:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.532	114	181586	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.783	117	171696	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.185	152	87456	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	182996	126.174	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	252.340%#	
7) Chloroethane-d5		1.532	69	142185	124.315	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	248.620%#	
11) 1,1-Dichloroethene-d2		2.059	65	76704	123.638	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	247.280%#	
21) 2-Butanone-d5		3.796	46	158141	205.794	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	205.790%#	
24) Chloroform-d		4.243	84	297280	114.219	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	228.440%#	
26) 1,2-Dichloroethane-d4		4.937	65	195369	116.748	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	233.500%#	
32) Benzene-d6		4.953	84	627858	121.072	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	242.140%#	
36) 1,2-Dichloropropane-d6		5.985	67	200992	120.136	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	240.280%#	
41) Toluene-d8		7.239	98	556257	116.934	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	233.860%#	
43) trans-1,3-Dichloroprop...		7.551	79	89027	102.248	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	204.500%#	
47) 2-Hexanone-d5		8.027	63	91109	189.398	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	189.400%#	
56) 1,1,2,2-Tetrachloroeth...		10.149	84	212156	110.441	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	220.880%#	
66) 1,2-Dichlorobenzene-d4		11.557	152	200501	112.507	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	225.020%#	
Target Compounds							
13) Acetone		2.114	43	5698	8.862	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036869.D
Acq On : 09 Aug 2024 11:52
Operator : SY/MD
Sample : P3480-18RE
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB5RE

Quant Time: Aug 10 01:16:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

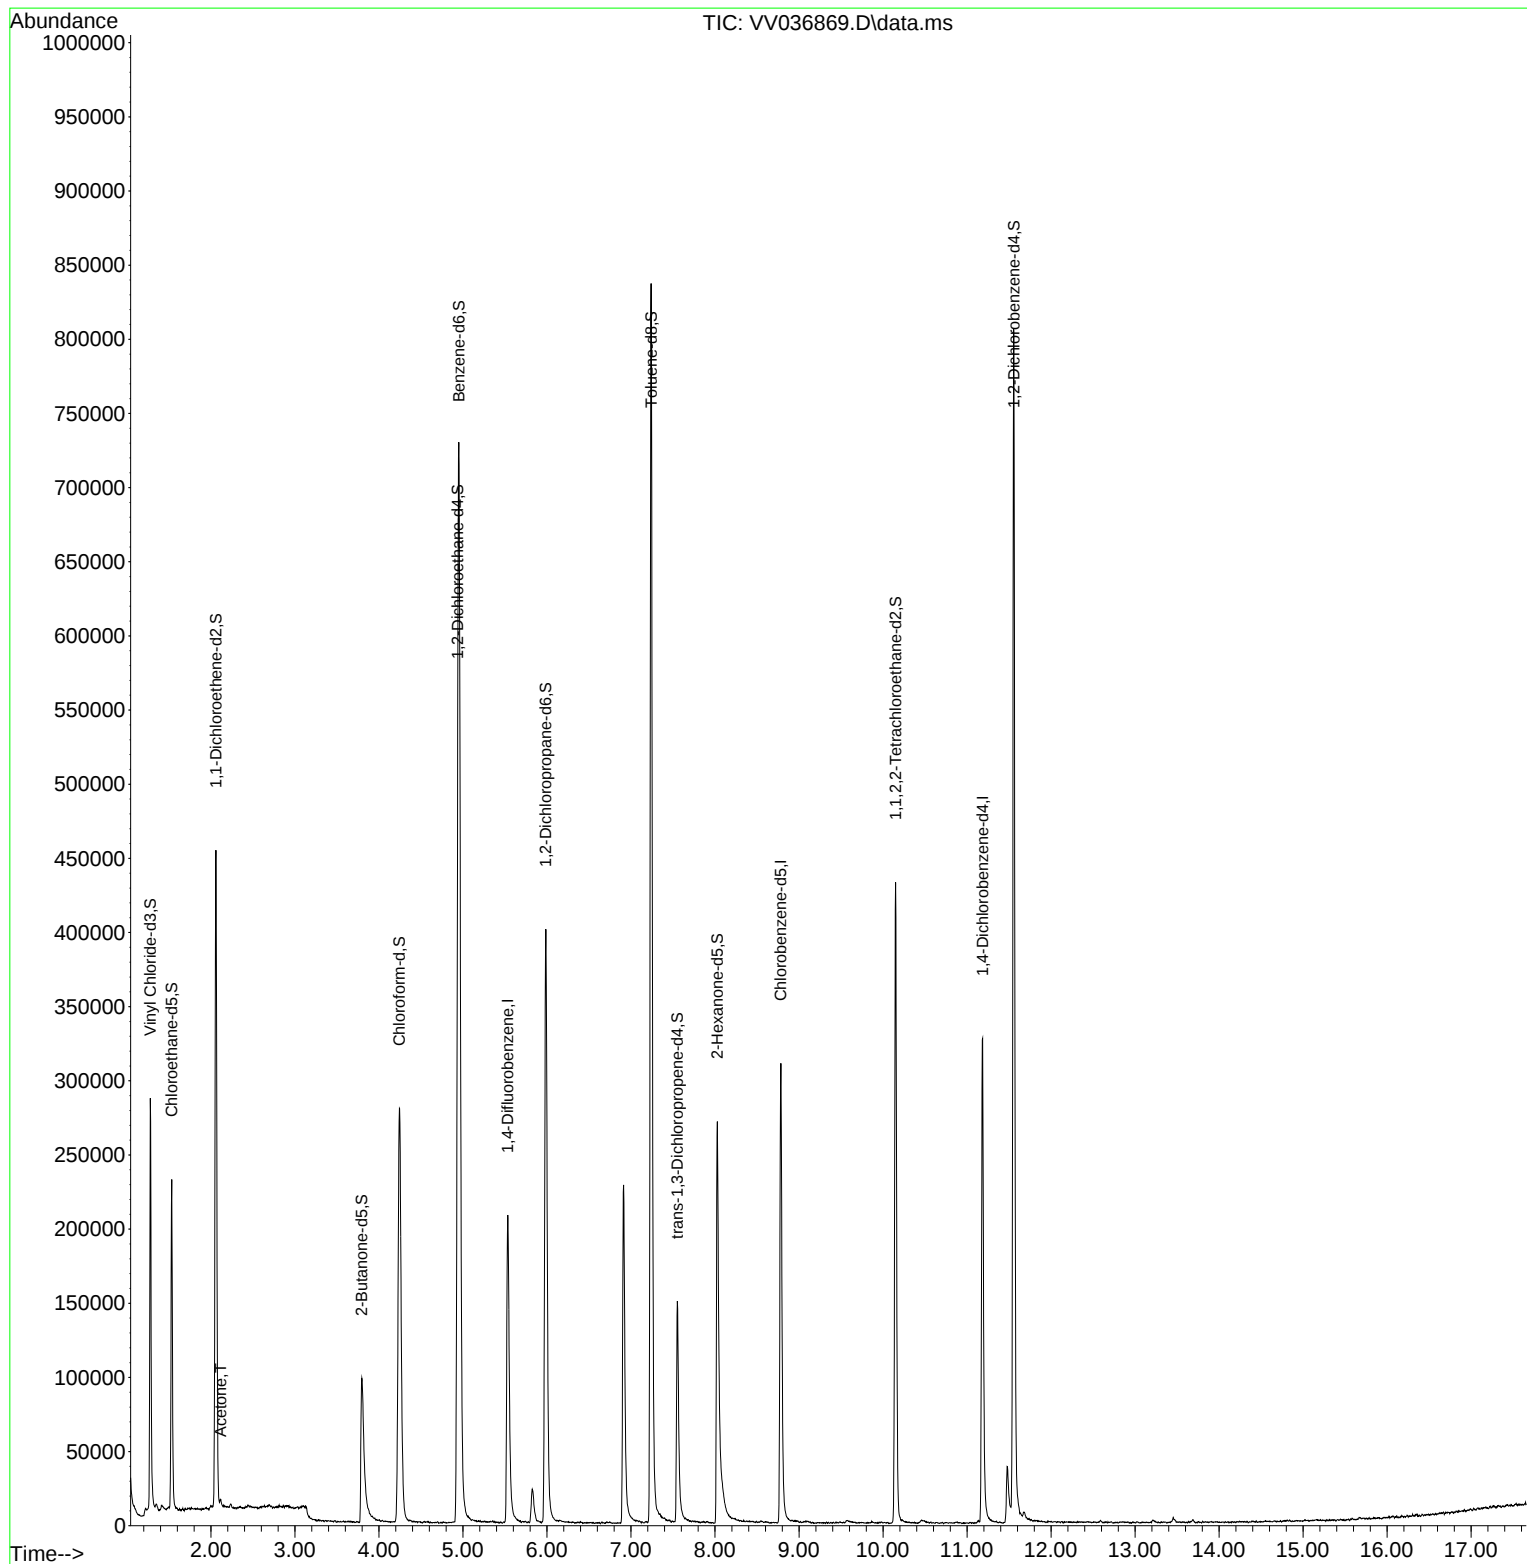

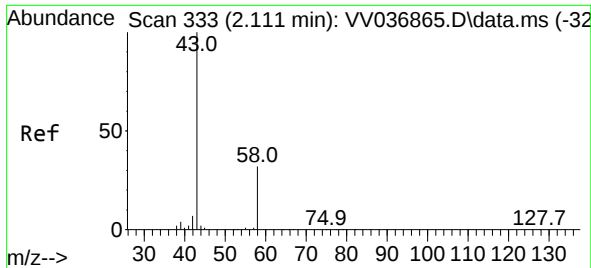

#13

Acetone

Concen: 8.862 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036869.D


Acq: 09 Aug 2024 11:52

Instrument :

MSVOA_V

ClientSampleId :

E0AB5RE

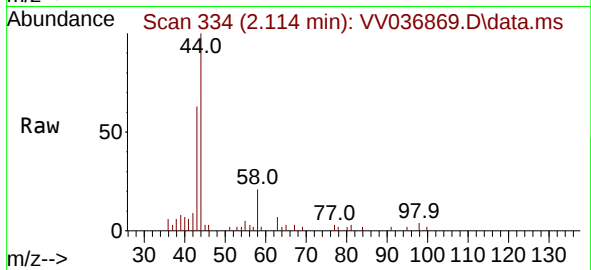

Tgt Ion: 43 Resp: 5698

Ion Ratio Lower Upper

43 100

58 38.5 0.0 63.4

