

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036872.D
 Acq On : 09 Aug 2024 12:59
 Operator : SY/MD
 Sample : P3480-23
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC3

Quant Time: Aug 10 01:17:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	621837	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	585310	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	281809	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	282338	56.846	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 113.700%		
7) Chloroethane-d5	1.532	69	216656	55.315	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 110.640%		
11) 1,1-Dichloroethene-d2	2.060	65	116360	54.770	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 109.540%		
21) 2-Butanone-d5	3.799	46	259940	98.780	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 98.780%		
24) Chloroform-d	4.246	84	458533	51.446	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 102.900%		
26) 1,2-Dichloroethane-d4	4.940	65	302727	52.826	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 105.660%		
32) Benzene-d6	4.953	84	970493	54.897	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.800%		
36) 1,2-Dichloropropane-d6	5.985	67	308743	54.134	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 108.260%		
41) Toluene-d8	7.239	98	866440	53.429	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 106.860%		
43) trans-1,3-Dichloroprop...	7.551	79	137511	46.328	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 92.660%		
47) 2-Hexanone-d5	8.027	63	141435	86.247	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 86.250%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	304552	46.506	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 93.020%		
66) 1,2-Dichlorobenzene-d4	11.558	152	312459	54.411	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 108.820%		
Target Compounds						
13) Acetone	2.114	43	39888	18.117	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036872.D
Acq On : 09 Aug 2024 12:59
Operator : SY/MD
Sample : P3480-23
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Quant Time: Aug 10 01:17:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

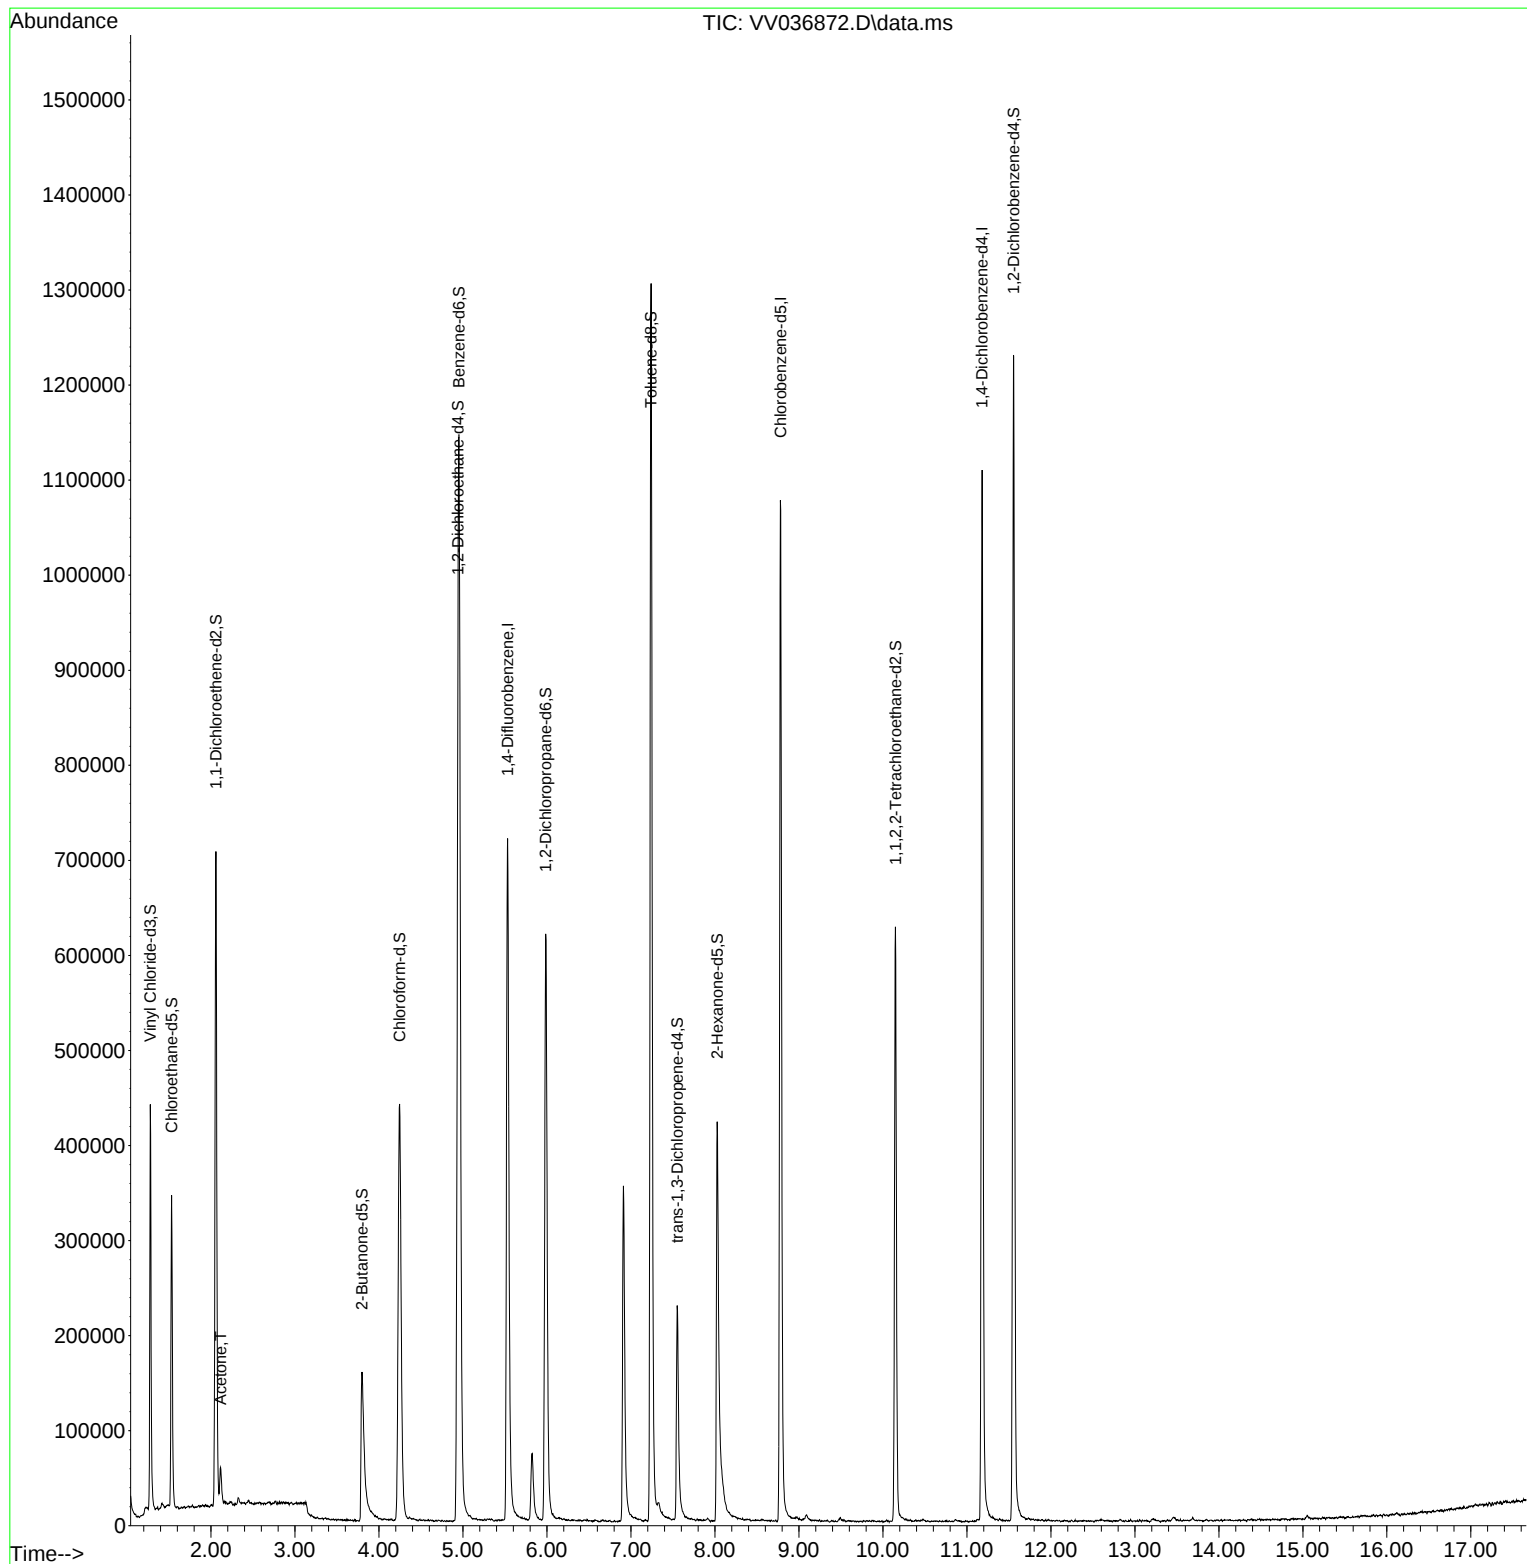

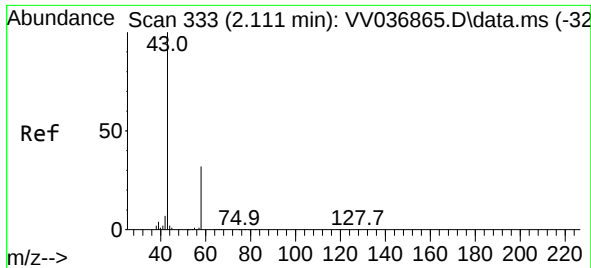

#13
Acetone
Concen: 18.117 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV036872.D
Acq: 09 Aug 2024 12:59

Instrument :
MSVOA_V
ClientSampleId :
E0AC3

Tgt Ion: 43 Resp: 39888
Ion Ratio Lower Upper
43 100
58 31.8 0.0 63.4

