

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036873.D
 Acq On : 09 Aug 2024 13:30
 Operator : SY/MD
 Sample : P3533-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AC4

Quant Time: Aug 10 01:17:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.529	114	491971	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.780	117	468831	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.182	152	231753	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.278	65	304487	77.489	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	154.980%#	
7) Chloroethane-d5		1.532	69	232153	74.918	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	149.840%#	
11) 1,1-Dichloroethene-d2		2.057	65	126399	75.201	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	150.400%#	
21) 2-Butanone-d5		3.796	46	270200	129.783	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	129.780%	
24) Chloroform-d		4.240	84	501654	71.141	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	142.280%#	
26) 1,2-Dichloroethane-d4		4.937	65	325820	71.865	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	143.720%#	
32) Benzene-d6		4.950	84	1053258	74.381	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	148.760%#	
36) 1,2-Dichloropropane-d6		5.982	67	336173	73.587	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	147.180%#	
41) Toluene-d8		7.236	98	944657	72.725	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	145.440%#	
43) trans-1,3-Dichloroprop...		7.551	79	153837	64.705	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	129.420%#	
47) 2-Hexanone-d5		8.024	63	146030	111.173	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	111.170%	
56) 1,1,2,2-Tetrachloroeth...		10.149	84	326806	62.303	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	124.600%#	
66) 1,2-Dichlorobenzene-d4		11.555	152	339609	71.913	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	143.820%#	
Target Compounds							
13) Acetone		2.114	43	38817	22.284	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036873.D
Acq On : 09 Aug 2024 13:30
Operator : SY/MD
Sample : P3533-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AC4

Quant Time: Aug 10 01:17:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

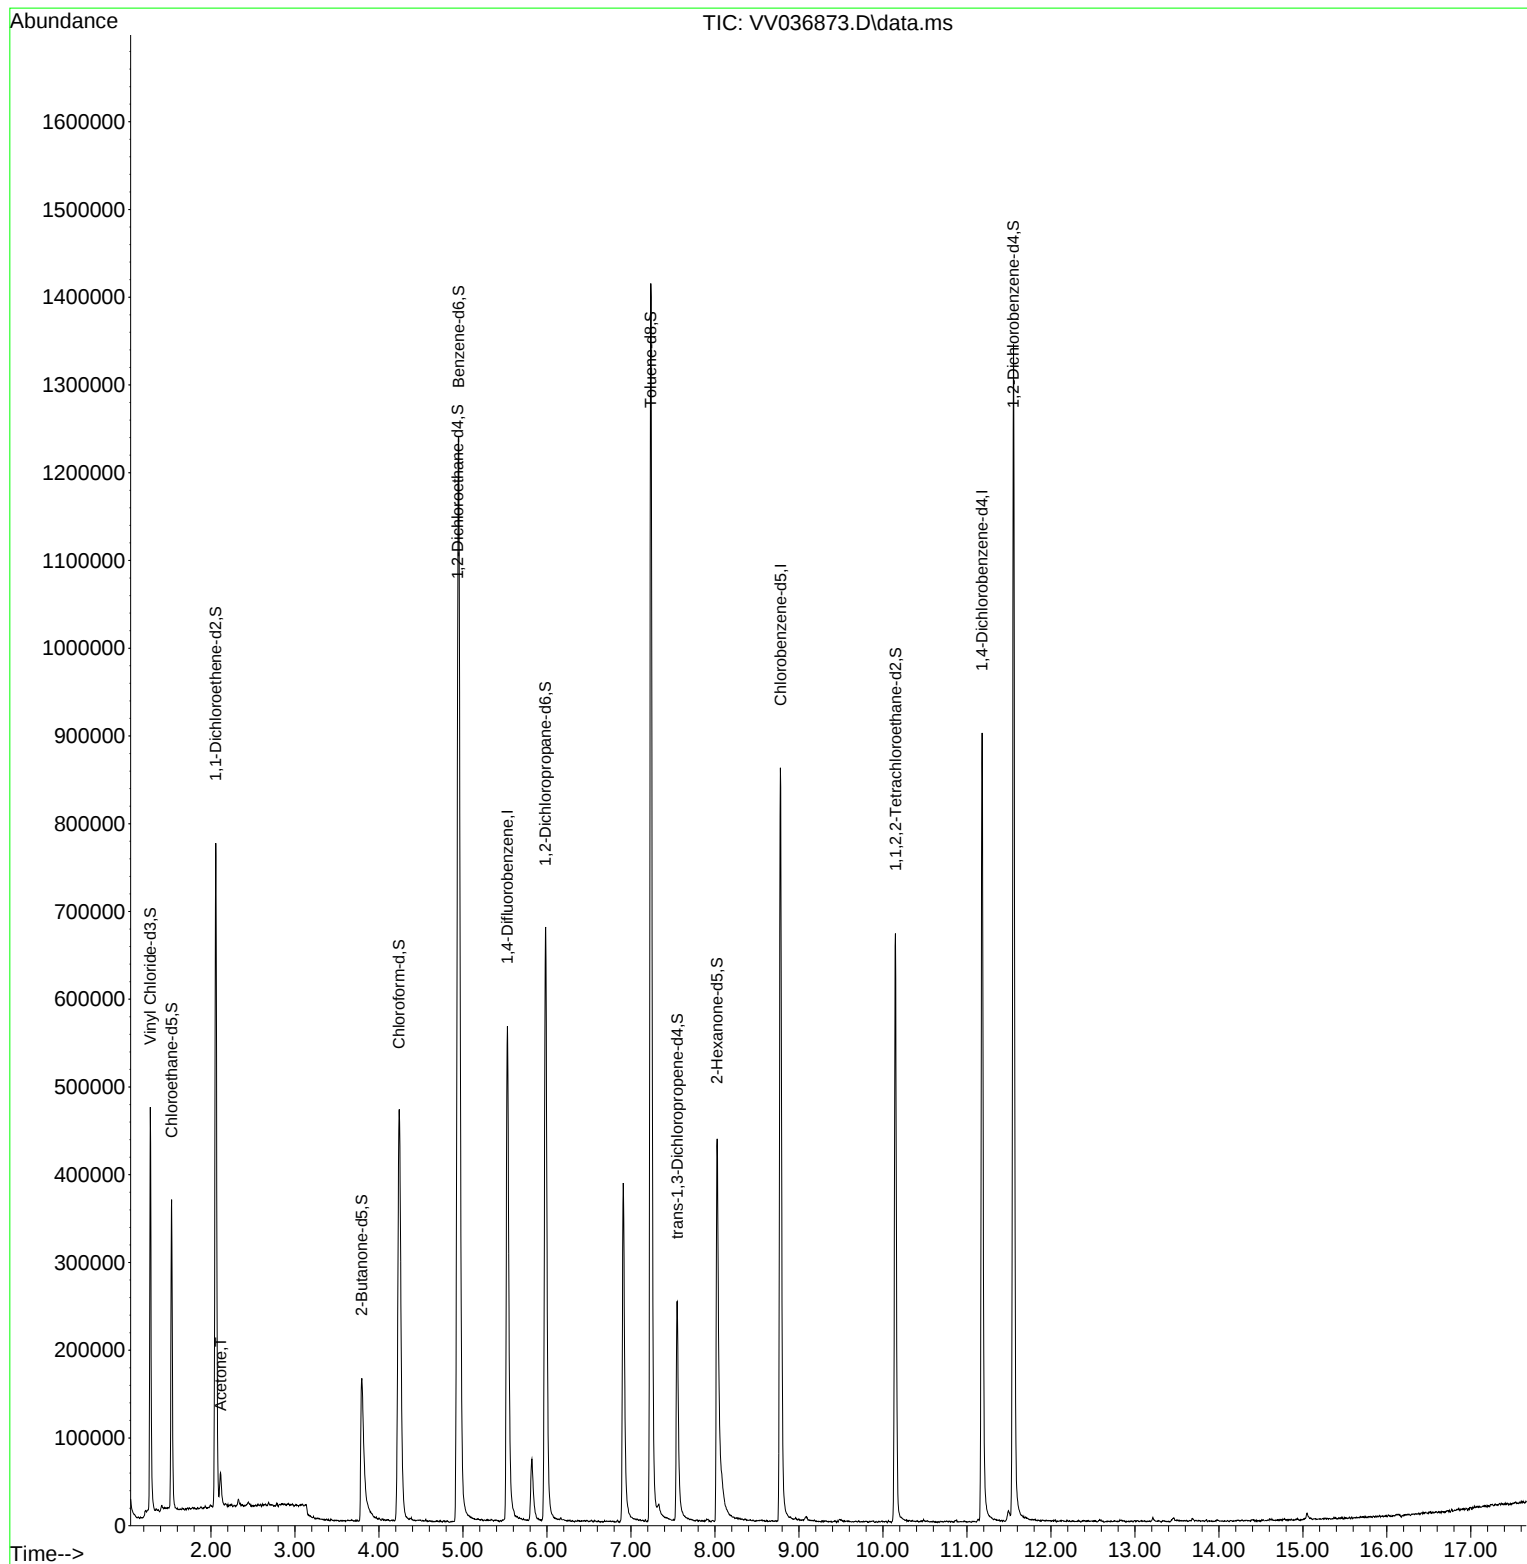

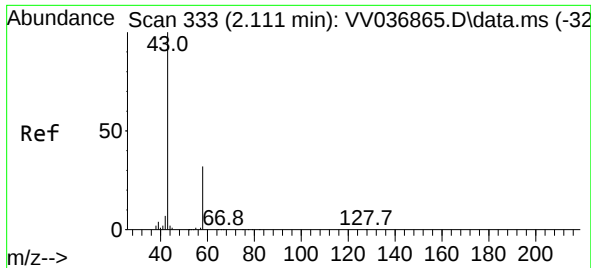

#13
Acetone
Concen: 22.284 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV036873.D
Acq: 09 Aug 2024 13:30

Instrument :
MSVOA_V
ClientSampleId :
E0AC4

Tgt Ion: 43 Resp: 38817
Ion Ratio Lower Upper
43 100
58 30.6 0.0 63.4

