

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036874.D
 Acq On : 09 Aug 2024 13:54
 Operator : SY/MD
 Sample : P3533-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AF7

Quant Time: Aug 10 01:18:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	554522	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	534761	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	260234	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	262364	59.237	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 118.480%		
7) Chloroethane-d5	1.532	69	203803	58.350	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 116.700%		
11) 1,1-Dichloroethene-d2	2.060	65	115845	61.147	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 122.300%		
21) 2-Butanone-d5	3.796	46	254638	108.511	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 108.510%		
24) Chloroform-d	4.243	84	453394	57.045	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 114.080%		
26) 1,2-Dichloroethane-d4	4.937	65	296691	58.058	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 116.120%		
32) Benzene-d6	4.953	84	963083	59.627	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 119.260%		
36) 1,2-Dichloropropane-d6	5.986	67	311956	59.867	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 119.740%		
41) Toluene-d8	7.239	98	870028	58.722	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 117.440%		
43) trans-1,3-Dichloroprop...	7.551	79	140617	51.853	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 103.700%		
47) 2-Hexanone-d5	8.024	63	139077	92.826	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 92.830%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	303536	50.733	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 101.460%		
66) 1,2-Dichlorobenzene-d4	11.554	152	312645	58.958	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 117.920%		
Target Compounds						
13) Acetone	2.114	43	37725	19.214	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036874.D
Acq On : 09 Aug 2024 13:54
Operator : SY/MD
Sample : P3533-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AF7

Quant Time: Aug 10 01:18:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

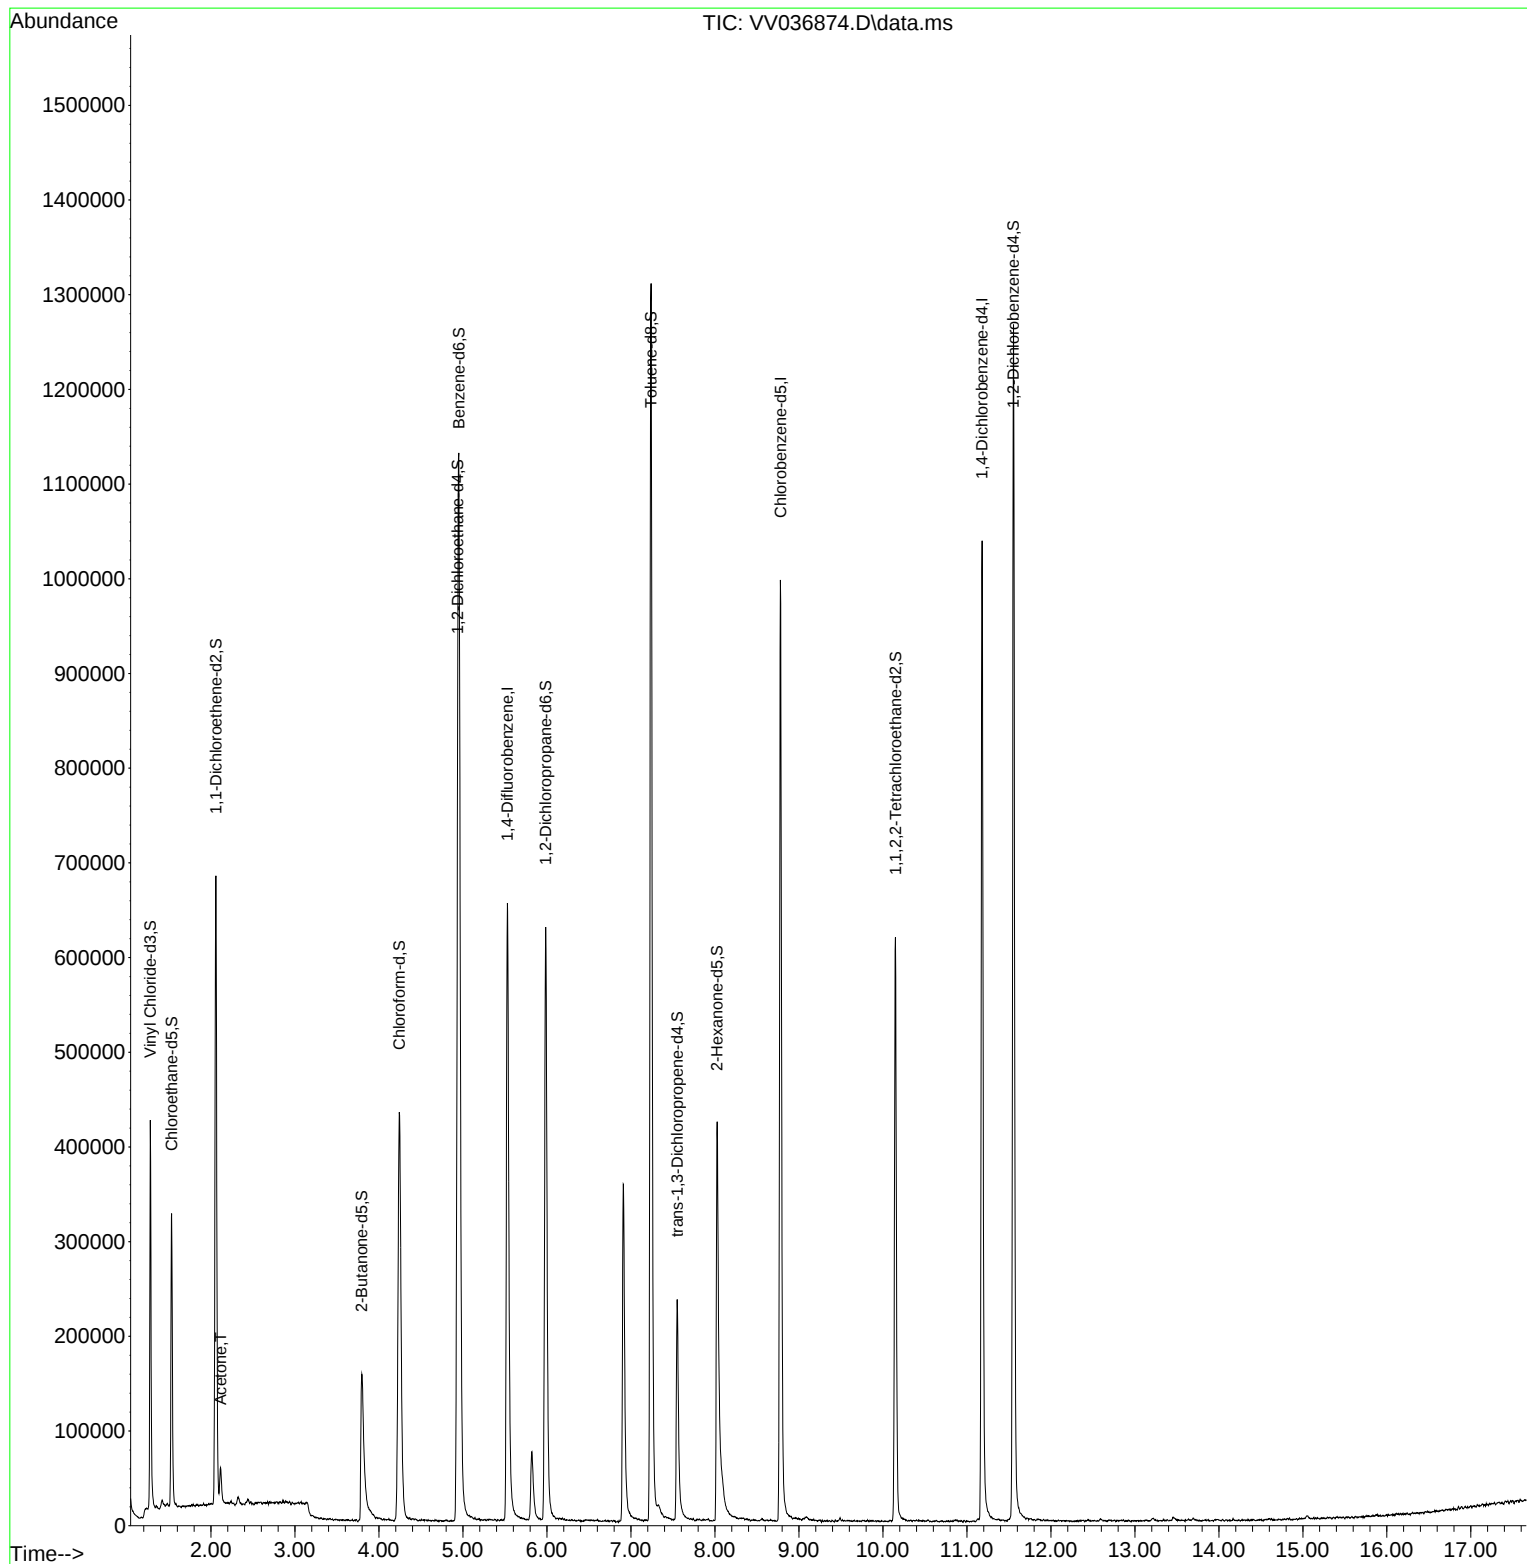

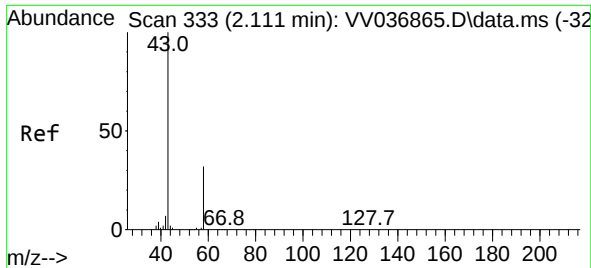

#13

Acetone

Concen: 19.214 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV036874.D

Acq: 09 Aug 2024 13:54

Instrument :

MSVOA_V

ClientSampleId :

E0AF7

Tgt Ion: 43 Resp: 37725

Ion Ratio Lower Upper

43 100

58 36.4 0.0 63.4

