

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036879.D
 Acq On : 09 Aug 2024 16:22
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Quant Time: Aug 10 01:19:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	705549	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	661958	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	321225	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	267294	47.432	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.860%		
7) Chloroethane-d5	1.532	69	208455	46.907	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.820%		
11) 1,1-Dichloroethene-d2	2.060	65	114802	47.626	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.260%		
21) 2-Butanone-d5	3.799	46	253607	84.938	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.940%		
24) Chloroform-d	4.246	84	450945	44.592	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.180%		
26) 1,2-Dichloroethane-d4	4.937	65	298591	45.923	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.840%		
32) Benzene-d6	4.953	84	952004	47.616	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.240%		
36) 1,2-Dichloropropane-d6	5.985	67	303211	47.008	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.020%		
41) Toluene-d8	7.239	98	848119	46.243	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.480%		
43) trans-1,3-Dichloroprop...	7.551	79	134121	39.954	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.900%		
47) 2-Hexanone-d5	8.027	63	144969	78.166	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.170%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	316971	42.798	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.600%		
66) 1,2-Dichlorobenzene-d4	11.558	152	305942	46.739	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.480%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	14319	5.732	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036879.D
Acq On : 09 Aug 2024 16:22
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Time: Aug 10 01:19:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

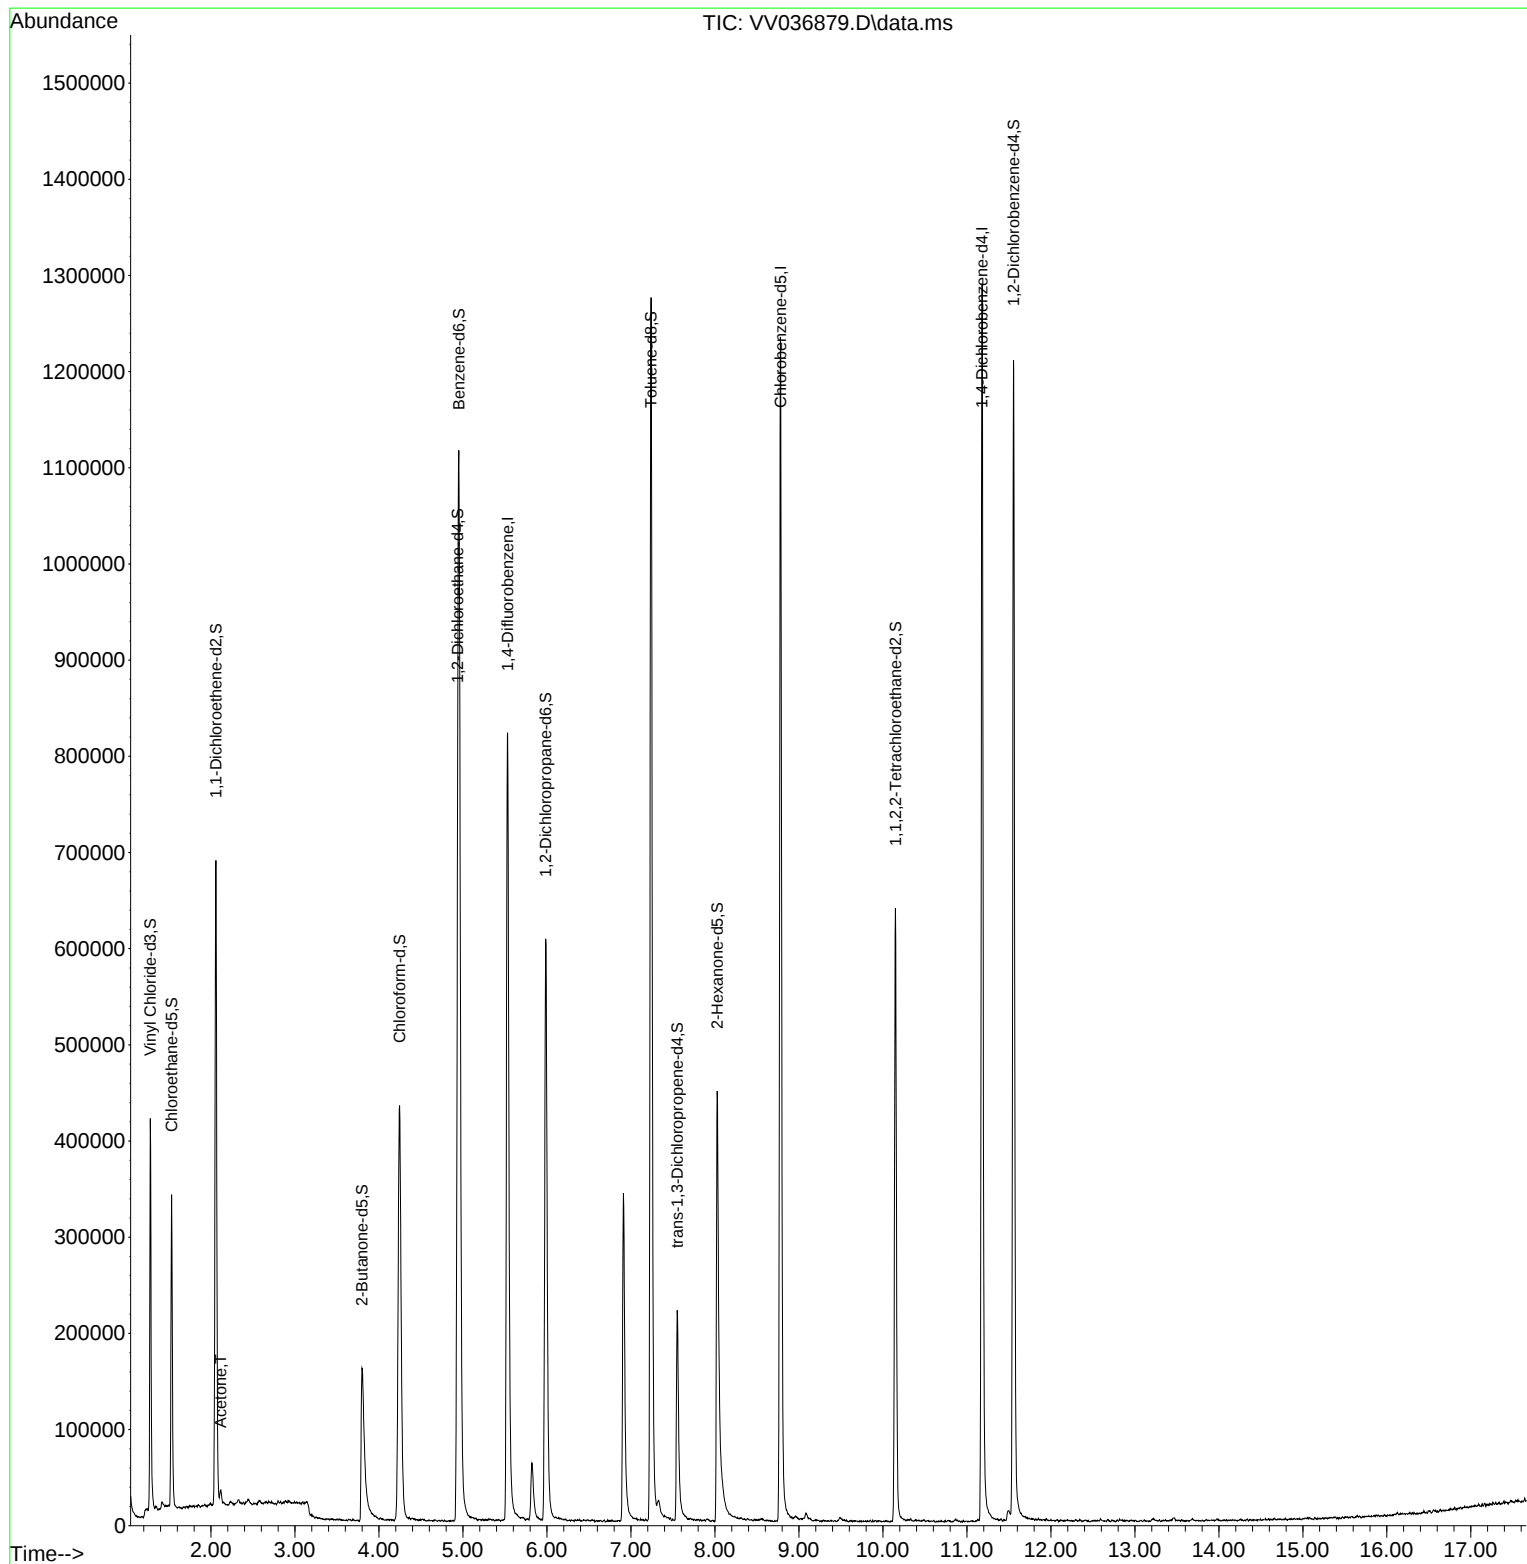

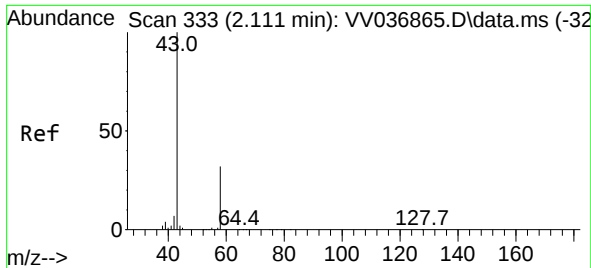

#13

Acetone

Concen: 5.732 ug/L

RT: 2.117 min Scan# 31

Delta R.T. 0.007 min

Lab File: VV036879.D


Acq: 09 Aug 2024 16:22

Instrument :

MSVOA_V

ClientSampleId :

E0AD5

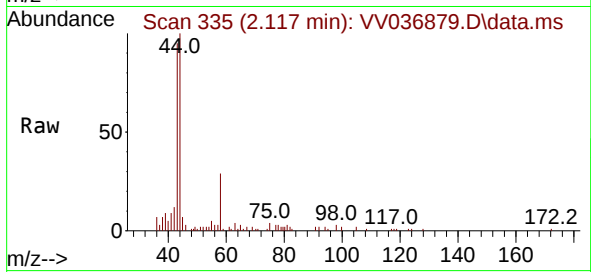

Tgt Ion: 43 Resp: 14319

Ion Ratio Lower Upper

43 100

58 31.6 0.0 63.4

