

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036888.D
 Acq On : 09 Aug 2024 19:41
 Operator : SY/MD
 Sample : P3533-07
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD6

Quant Time: Aug 10 01:21:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 10 01:11:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	702303	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	670115	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	323982	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	268421	47.852	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	95.700%	
7) Chloroethane-d5	1.532	69	210034	47.481	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.960%	
11) 1,1-Dichloroethene-d2	2.056	65	115331	48.066	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	96.140%	
21) 2-Butanone-d5	3.799	46	258368	86.933	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	86.930%	
24) Chloroform-d	4.246	84	452702	44.972	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	89.940%	
26) 1,2-Dichloroethane-d4	4.941	65	298240	46.081	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.160%	
32) Benzene-d6	4.953	84	947687	46.823	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.640%	
36) 1,2-Dichloropropane-d6	5.986	67	301829	46.224	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	92.440%	
41) Toluene-d8	7.239	98	851325	45.853	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.700%	
43) trans-1,3-Dichloroprop...	7.551	79	129742	38.179	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	76.360%	
47) 2-Hexanone-d5	8.027	63	148937	79.328	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	79.330%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	324104	43.229	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	86.460%	
66) 1,2-Dichlorobenzene-d4	11.554	152	306526	46.430	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.860%	
Target Compounds						
13) Acetone	2.114	43	9654	3.882	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036888.D
Acq On : 09 Aug 2024 19:41
Operator : SY/MD
Sample : P3533-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD6

Quant Time: Aug 10 01:21:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 10 01:11:12 2024
Response via : Initial Calibration

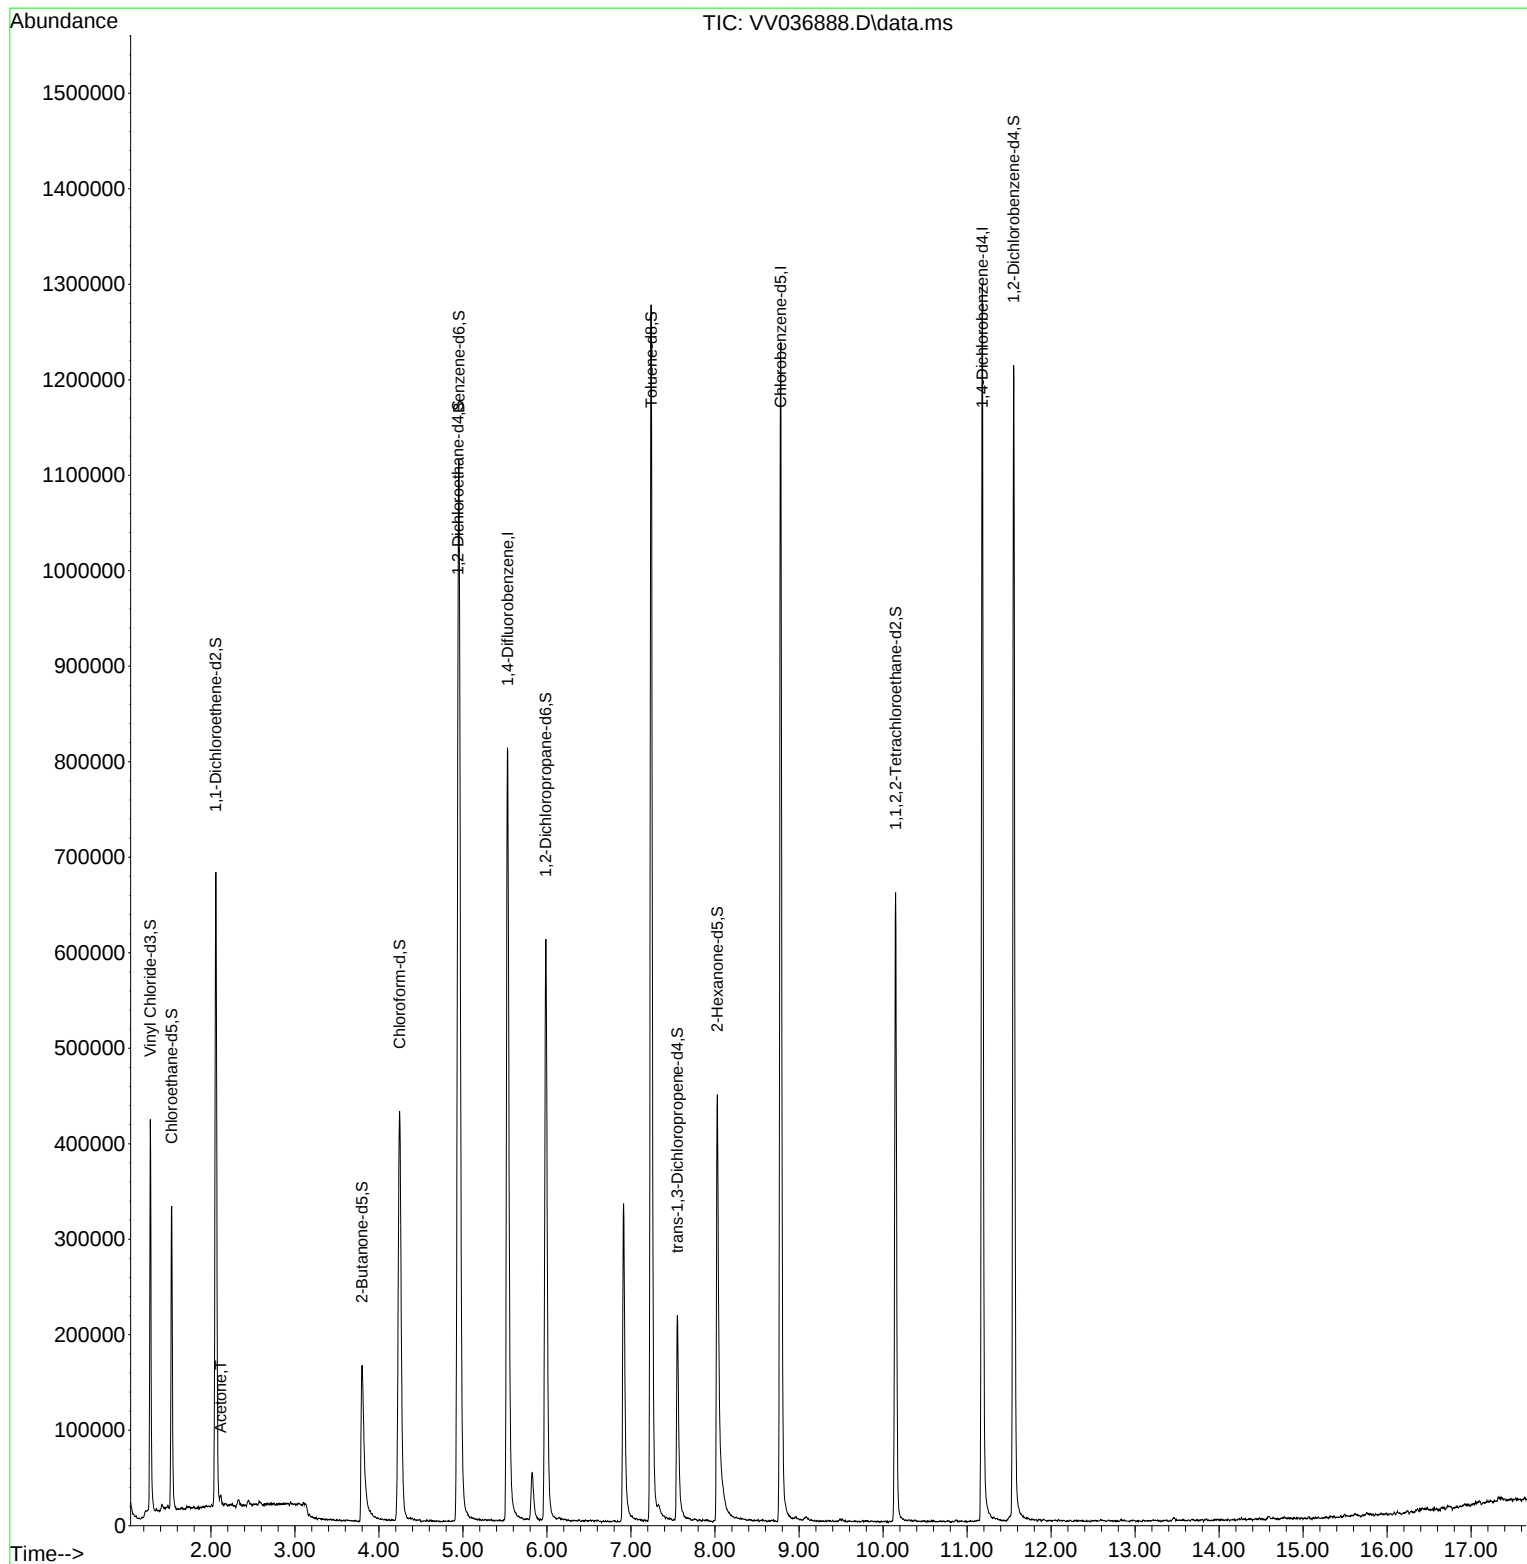

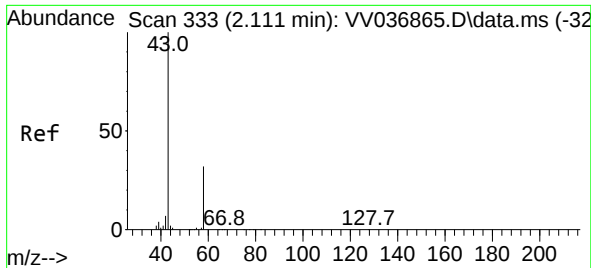

#13
 Acetone
 Concen: 3.882 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV036888.D
 Acq: 09 Aug 2024 19:41

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD6

Tgt Ion: 43 Resp: 9654
 Ion Ratio Lower Upper
 43 100
 58 30.0 0.0 63.4

