

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036867.D
 Acq On : 09 Aug 2024 11:08
 Operator : SY/MD
 Sample : VV0809WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	211775	226306	13.40%	1.793%
2	1.532	146	153	167	rVB	188339	218517	12.94%	1.731%
3	2.056	307	316	333	rBV	357276	516596	30.59%	4.093%
4	3.384	726	729	730	rBV2	977	497	0.03%	0.004%
5	3.477	755	758	759	rBV3	846	461	0.03%	0.004%
6	3.519	769	771	774	rBV	558	430	0.03%	0.003%
7	3.735	835	838	841	rBV3	628	424	0.03%	0.003%
8	3.796	849	857	896	rBV	108656	301391	17.85%	2.388%
9	4.092	946	949	952	rVB2	899	634	0.04%	0.005%
10	4.114	952	956	958	rBV2	815	578	0.03%	0.005%
11	4.243	980	996	1024	rBV	270493	685316	40.58%	5.430%
12	4.548	1089	1091	1096	rVB3	673	486	0.03%	0.004%
13	4.641	1118	1120	1124	rVB3	827	526	0.03%	0.004%
14	4.950	1200	1216	1249	rBV2	673744	1688659	100.00%	13.379%
15	5.529	1385	1396	1427	rBV	508423	1033761	61.22%	8.190%
16	5.825	1477	1488	1507	rBV	24834	55183	3.27%	0.437%
17	5.985	1524	1538	1565	rBV	382689	793064	46.96%	6.283%
18	6.500	1696	1698	1702	rVB3	794	523	0.03%	0.004%
19	6.545	1709	1712	1718	rBV4	1092	1218	0.07%	0.010%
20	6.587	1722	1725	1732	rVB6	799	701	0.04%	0.006%
21	6.911	1815	1826	1863	rBV	209915	405427	24.01%	3.212%
22	7.156	1897	1902	1903	rBV5	653	518	0.03%	0.004%
23	7.239	1917	1928	1962	rBV	725345	1294813	76.68%	10.259%
24	7.551	2016	2025	2051	rBV	138460	256526	15.19%	2.032%
25	7.902	2132	2134	2137	rVV3	653	427	0.03%	0.003%
26	7.982	2155	2159	2161	rBV3	881	772	0.05%	0.006%
27	8.027	2164	2173	2208	rBV2	285733	614533	36.39%	4.869%
28	8.664	2367	2371	2376	rVV5	579	590	0.03%	0.005%
29	8.735	2390	2393	2397	rBV5	604	566	0.03%	0.004%
30	8.780	2397	2407	2441	rBV	744529	1255774	74.37%	9.949%
31	9.037	2483	2487	2489	rBV3	816	560	0.03%	0.004%
32	9.053	2489	2492	2493	rBV2	796	421	0.02%	0.003%
33	9.136	2514	2518	2522	rVB5	1289	849	0.05%	0.007%
34	9.162	2522	2526	2530	rBV5	808	699	0.04%	0.006%
35	9.239	2546	2550	2553	rVB4	677	469	0.03%	0.004%
36	9.255	2553	2555	2559	rVB5	739	556	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036867.D
 Acq On : 09 Aug 2024 11:08
 Operator : SY/MD
 Sample : VV0809WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.284	2560	2564	2567	rBV5	739	512	0.03%	0.004%
38	9.384	2590	2595	2596	rBV3	745	547	0.03%	0.004%
39	9.413	2602	2604	2611	rVB5	761	768	0.05%	0.006%
40	9.464	2616	2620	2623	rBV3	591	551	0.03%	0.004%
41	9.487	2623	2627	2632	rBV4	681	604	0.04%	0.005%
42	9.615	2664	2667	2672	rBV4	517	438	0.03%	0.003%
43	9.641	2672	2675	2677	rVV4	895	463	0.03%	0.004%
44	9.767	2708	2714	2716	rBV2	659	501	0.03%	0.004%
45	9.786	2716	2720	2722	rBV3	804	469	0.03%	0.004%
46	9.802	2722	2725	2730	rVB4	681	485	0.03%	0.004%
47	9.837	2733	2736	2741	rBV4	823	697	0.04%	0.006%
48	9.870	2743	2746	2748	rBV3	930	592	0.04%	0.005%
49	9.931	2762	2765	2766	rBV3	783	472	0.03%	0.004%
50	10.050	2796	2802	2804	rBV4	713	762	0.05%	0.006%
51	10.149	2822	2833	2856	rBV	443397	705693	41.79%	5.591%
52	10.300	2875	2880	2884	rBV4	842	864	0.05%	0.007%
53	10.458	2923	2929	2930	rBV4	745	604	0.04%	0.005%
54	10.484	2935	2937	2941	rVV4	608	476	0.03%	0.004%
55	10.603	2969	2974	2976	rBV2	592	541	0.03%	0.004%
56	10.625	2976	2981	2984	rVV5	888	786	0.05%	0.006%
57	10.664	2987	2993	2997	rVV5	763	884	0.05%	0.007%
58	10.696	3001	3003	3010	rVB4	779	660	0.04%	0.005%
59	10.770	3020	3026	3031	rBV4	744	798	0.05%	0.006%
60	10.866	3048	3056	3062	rBV5	1436	2181	0.13%	0.017%
61	10.953	3080	3083	3089	rVB2	939	1036	0.06%	0.008%
62	11.005	3094	3099	3102	rBV5	577	552	0.03%	0.004%
63	11.033	3105	3108	3114	rVB3	910	822	0.05%	0.007%
64	11.130	3133	3138	3140	rBV3	1598	1390	0.08%	0.011%
65	11.181	3143	3154	3177	rBV	786501	1243235	73.62%	9.850%
66	11.500	3249	3253	3255	rBV3	1291	861	0.05%	0.007%
67	11.554	3259	3270	3296	rBV	784646	1256604	74.41%	9.956%
68	11.831	3352	3356	3358	rBV5	811	668	0.04%	0.005%
69	11.863	3362	3366	3368	rBV4	703	579	0.03%	0.005%
70	12.011	3408	3412	3414	rBV4	578	415	0.02%	0.003%
71	12.088	3433	3436	3438	rVB2	940	438	0.03%	0.003%
72	12.130	3447	3449	3453	rVB3	968	566	0.03%	0.004%
73	12.197	3466	3470	3474	rBV6	755	786	0.05%	0.006%
74	12.284	3494	3497	3502	rVV2	829	507	0.03%	0.004%
75	12.397	3529	3532	3536	rVV3	903	786	0.05%	0.006%
76	12.522	3568	3571	3577	rBV5	634	556	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036867.D
 Acq On : 09 Aug 2024 11:08
 Operator : SY/MD
 Sample : VV0809WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.590	3585	3592	3593	rBV4	1510	1291	0.08%	0.010%
78	12.702	3622	3627	3631	rBV3	658	683	0.04%	0.005%
79	12.998	3717	3719	3723	rBV2	758	601	0.04%	0.005%
80	13.027	3726	3728	3732	rVV4	684	452	0.03%	0.004%
81	13.049	3732	3735	3739	rVB5	791	545	0.03%	0.004%
82	13.210	3778	3785	3798	rBV5	3178	5899	0.35%	0.047%
83	13.355	3825	3830	3831	rBV3	589	454	0.03%	0.004%
84	13.387	3836	3840	3841	rBV3	516	417	0.02%	0.003%
85	13.458	3852	3862	3871	rBV5	4212	8714	0.52%	0.069%
86	13.577	3893	3899	3903	rBV8	1078	1343	0.08%	0.011%
87	13.628	3911	3915	3919	rVV6	754	725	0.04%	0.006%
88	13.670	3922	3928	3929	rBV5	951	989	0.06%	0.008%
89	13.689	3929	3934	3939	rVB6	2621	3215	0.19%	0.025%
90	13.741	3948	3950	3954	rBV3	747	435	0.03%	0.003%
91	13.802	3964	3969	3972	rVB4	853	639	0.04%	0.005%
92	13.966	4017	4020	4021	rBV2	1151	639	0.04%	0.005%
93	14.082	4054	4056	4059	rVV3	1061	700	0.04%	0.006%
94	14.194	4088	4091	4093	rBV3	647	418	0.02%	0.003%
95	14.226	4097	4101	4102	rBV2	782	521	0.03%	0.004%
96	14.274	4112	4116	4119	rBV4	646	470	0.03%	0.004%
97	14.297	4119	4123	4127	rBV3	795	980	0.06%	0.008%
98	14.528	4192	4195	4196	rBV3	778	436	0.03%	0.003%
99	14.975	4330	4334	4338	rBV4	733	679	0.04%	0.005%
100	15.641	4539	4541	4543	rBV3	999	581	0.03%	0.005%




Sum of corrected areas: 12621746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036867.D
Acq On : 09 Aug 2024 11:08
Operator : SY/MD
Sample : VV0809WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

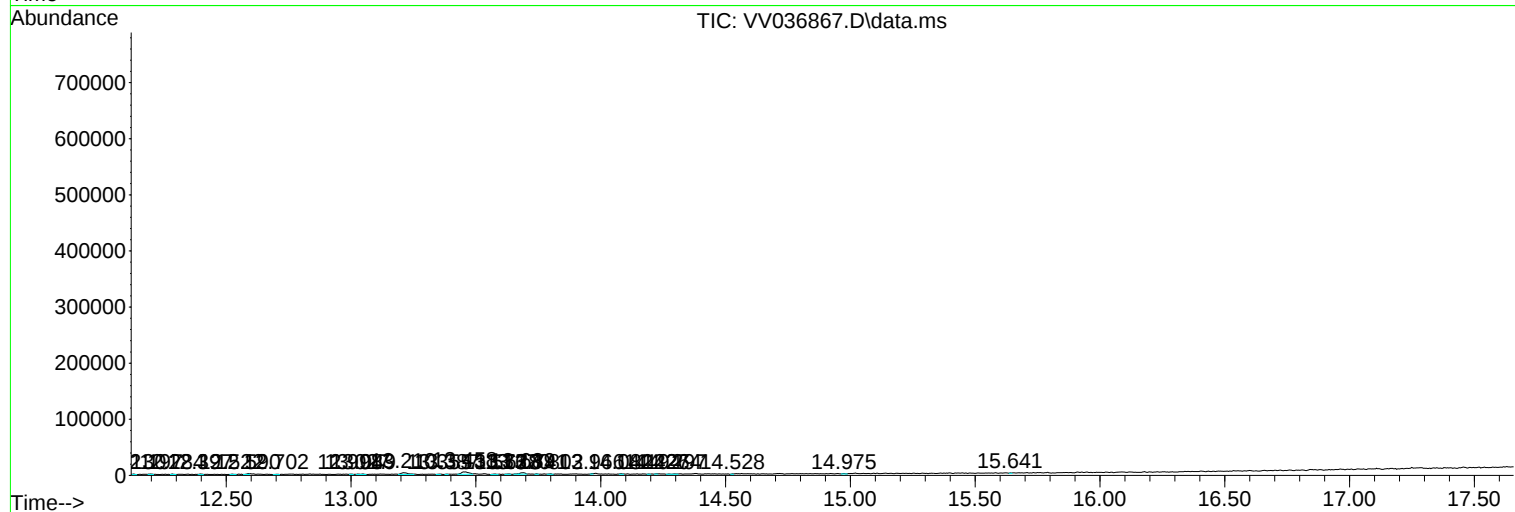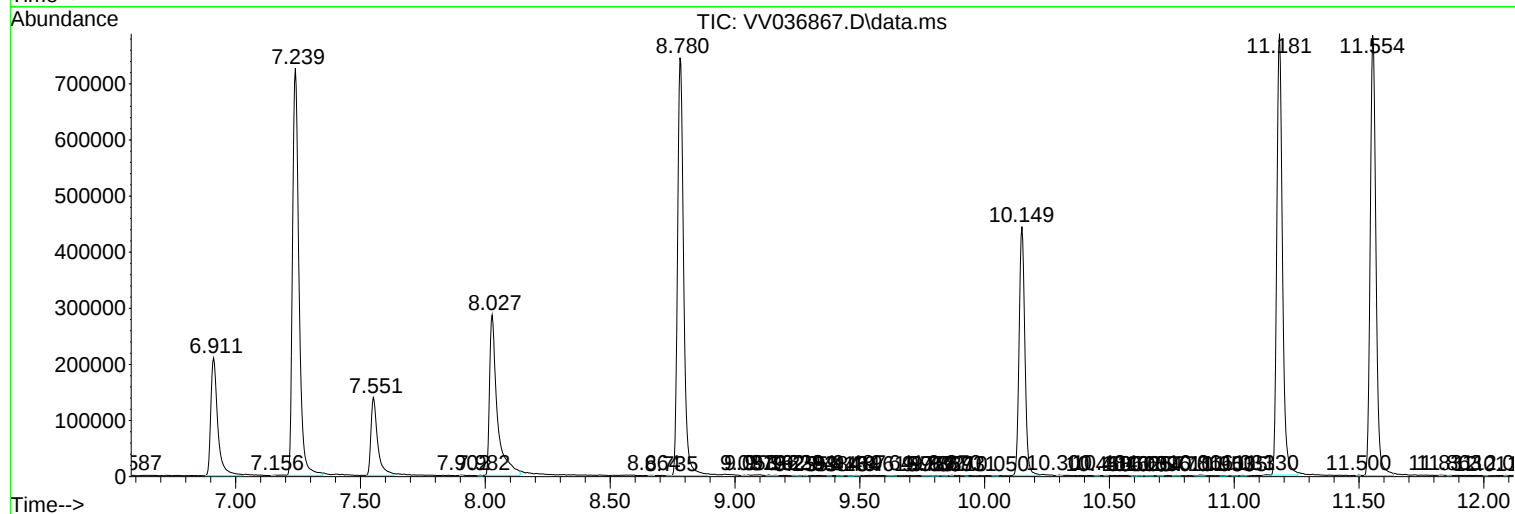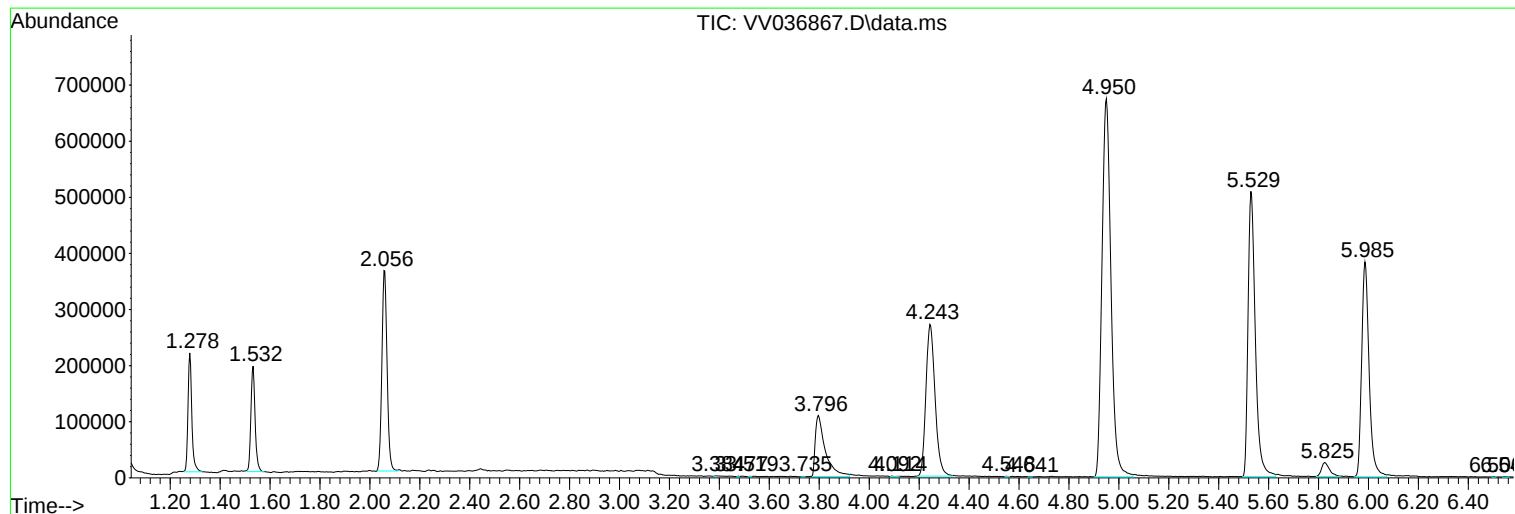

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036867.D
Acq On : 09 Aug 2024 11:08
Operator : SY/MD
Sample : VV0809WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036867.D
Acq On : 09 Aug 2024 11:08
Operator : SY/MD
Sample : VV0809WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK366

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------