

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036879.D
 Acq On : 09 Aug 2024 16:22
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	405557	434116	15.56%	2.116%
2	1.532	146	153	170	rVB	324642	378707	13.57%	1.846%
3	2.060	308	317	329	rBV	664618	942733	33.79%	4.596%
4	3.799	850	858	894	rBV	157840	453725	16.26%	2.212%
5	4.246	982	997	1026	rVB	428910	1071875	38.42%	5.226%
6	4.950	1201	1216	1251	rBV2	1112674	2790054	100.00%	13.603%
7	5.532	1385	1397	1425	rBV	818254	1667363	59.76%	8.129%
8	5.821	1476	1487	1505	rBV2	59388	135505	4.86%	0.661%
9	5.985	1526	1538	1572	rBV	604351	1253414	44.92%	6.111%
10	6.333	1644	1646	1648	rBV3	1401	819	0.03%	0.004%
11	6.590	1720	1726	1730	rBV7	1687	2101	0.08%	0.010%
12	6.635	1736	1740	1747	rVB7	1517	1932	0.07%	0.009%
13	6.674	1749	1752	1754	rBV4	1355	968	0.03%	0.005%
14	6.709	1759	1763	1764	rBV4	829	425	0.02%	0.002%
15	6.722	1764	1767	1772	rBV7	1705	1389	0.05%	0.007%
16	6.773	1780	1783	1787	rVB6	1533	1150	0.04%	0.006%
17	6.838	1802	1803	1804	rBV	678	212	0.01%	0.001%
18	6.911	1815	1826	1857	rBV	340829	652910	23.40%	3.183%
19	7.239	1917	1928	1949	rBV	1270651	2221712	79.63%	10.832%
20	7.551	2016	2025	2052	rBV	218241	411497	14.75%	2.006%
21	7.905	2129	2135	2137	rBV6	2263	2741	0.10%	0.013%
22	7.973	2150	2156	2159	rBV6	1459	1739	0.06%	0.008%
23	8.027	2164	2173	2217	rBV2	447581	992404	35.57%	4.838%
24	8.464	2307	2309	2310	rBV2	1450	555	0.02%	0.003%
25	8.715	2383	2387	2390	rBV4	1150	1031	0.04%	0.005%
26	8.780	2396	2407	2435	rBV	1231191	2037917	73.04%	9.936%
27	9.259	2553	2556	2559	rBV3	1037	610	0.02%	0.003%
28	9.275	2559	2561	2562	rBV2	1143	463	0.02%	0.002%
29	9.461	2617	2619	2621	rBV2	1090	511	0.02%	0.002%
30	9.567	2651	2652	2655	rVB4	1519	709	0.03%	0.003%
31	9.609	2662	2665	2666	rBV3	1230	639	0.02%	0.003%
32	9.648	2675	2677	2678	rBV2	929	459	0.02%	0.002%
33	9.728	2699	2702	2706	rBV6	1660	1221	0.04%	0.006%
34	9.747	2706	2708	2710	rBV3	1171	652	0.02%	0.003%
35	9.770	2713	2715	2716	rBV2	822	271	0.01%	0.001%
36	9.812	2726	2728	2731	rBV4	1355	863	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036879.D
 Acq On : 09 Aug 2024 16:22
 Operator : SY/MD
 Sample : P3480-21
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.850	2735	2740	2746	rVB9	2053	2255	0.08%	0.011%
38	9.879	2746	2749	2752	rBV5	2028	1075	0.04%	0.005%
39	9.892	2752	2753	2754	rBV	403	117	0.00%	0.001%
40	9.905	2754	2757	2760	rVV4	1360	1113	0.04%	0.005%
41	9.937	2764	2767	2769	rBV4	1315	849	0.03%	0.004%
42	9.985	2780	2782	2784	rBV3	638	313	0.01%	0.002%
43	10.037	2793	2798	2801	rBV4	1463	1259	0.05%	0.006%
44	10.066	2805	2807	2813	rVB5	1293	1356	0.05%	0.007%
45	10.095	2813	2816	2818	rBV4	1548	976	0.03%	0.005%
46	10.149	2822	2833	2853	rBV	637723	1020022	36.56%	4.973%
47	10.461	2928	2930	2932	rBV3	978	356	0.01%	0.002%
48	10.513	2945	2946	2950	rBV4	890	730	0.03%	0.004%
49	10.570	2961	2964	2965	rBV3	769	391	0.01%	0.002%
50	10.641	2982	2986	2989	rBV6	1078	941	0.03%	0.005%
51	10.664	2991	2993	2995	rBV3	1006	427	0.02%	0.002%
52	10.693	3000	3002	3005	rVB3	1155	622	0.02%	0.003%
53	10.744	3014	3018	3020	rVB5	1317	817	0.03%	0.004%
54	10.773	3024	3027	3028	rBV3	1196	779	0.03%	0.004%
55	10.824	3039	3043	3045	rBV4	1038	605	0.02%	0.003%
56	10.940	3075	3079	3081	rBV3	1439	1010	0.04%	0.005%
57	10.956	3083	3084	3089	rVB5	1335	809	0.03%	0.004%
58	10.979	3089	3091	3093	rBV2	651	426	0.02%	0.002%
59	11.107	3128	3131	3132	rBV3	1150	667	0.02%	0.003%
60	11.130	3135	3138	3140	rVV5	1790	1001	0.04%	0.005%
61	11.181	3143	3154	3185	rBV	1286174	2024348	72.56%	9.870%
62	11.493	3243	3251	3259	rBV6	9727	22018	0.79%	0.107%
63	11.554	3260	3270	3297	rVV	1201631	1937017	69.43%	9.444%
64	11.947	3388	3392	3394	rBV5	2485	1886	0.07%	0.009%
65	12.098	3437	3439	3440	rBV2	1087	445	0.02%	0.002%
66	12.159	3455	3458	3460	rVB3	1387	722	0.03%	0.004%
67	12.181	3461	3465	3468	rBV5	1347	1343	0.05%	0.007%
68	12.323	3507	3509	3512	rBV3	824	612	0.02%	0.003%
69	12.377	3523	3526	3528	rBV4	1076	816	0.03%	0.004%
70	12.487	3555	3560	3562	rBV6	1026	921	0.03%	0.004%
71	12.525	3570	3572	3575	rVB4	1272	666	0.02%	0.003%
72	12.677	3614	3619	3622	rBV5	2210	2075	0.07%	0.010%
73	12.728	3632	3635	3638	rBV5	1510	946	0.03%	0.005%
74	12.776	3648	3650	3651	rBV2	583	282	0.01%	0.001%
75	12.789	3651	3654	3659	rVV4	1799	1586	0.06%	0.008%
76	12.818	3660	3663	3668	rVV6	2216	1632	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036879.D
Acq On : 09 Aug 2024 16:22
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	12.895	3683	3687	3690	rBV6	1427	1393	0.05%	0.007%
78	13.001	3717	3720	3721	rBV2	1539	807	0.03%	0.004%
79	13.130	3758	3760	3762	rBV4	719	266	0.01%	0.001%
80	13.168	3770	3772	3774	rBV3	879	377	0.01%	0.002%
81	13.178	3774	3775	3778	rBV3	801	386	0.01%	0.002%
82	13.320	3817	3819	3821	rBV3	840	367	0.01%	0.002%
83	13.455	3857	3861	3862	rBV4	2412	1736	0.06%	0.008%
84	13.561	3889	3894	3895	rBV5	1977	1552	0.06%	0.008%
85	13.619	3909	3912	3916	rBV5	1460	1213	0.04%	0.006%
86	13.953	4014	4016	4019	rBV4	958	646	0.02%	0.003%
87	14.326	4129	4132	4133	rBV3	1377	731	0.03%	0.004%




Sum of corrected areas: 20511097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036879.D
Acq On : 09 Aug 2024 16:22
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

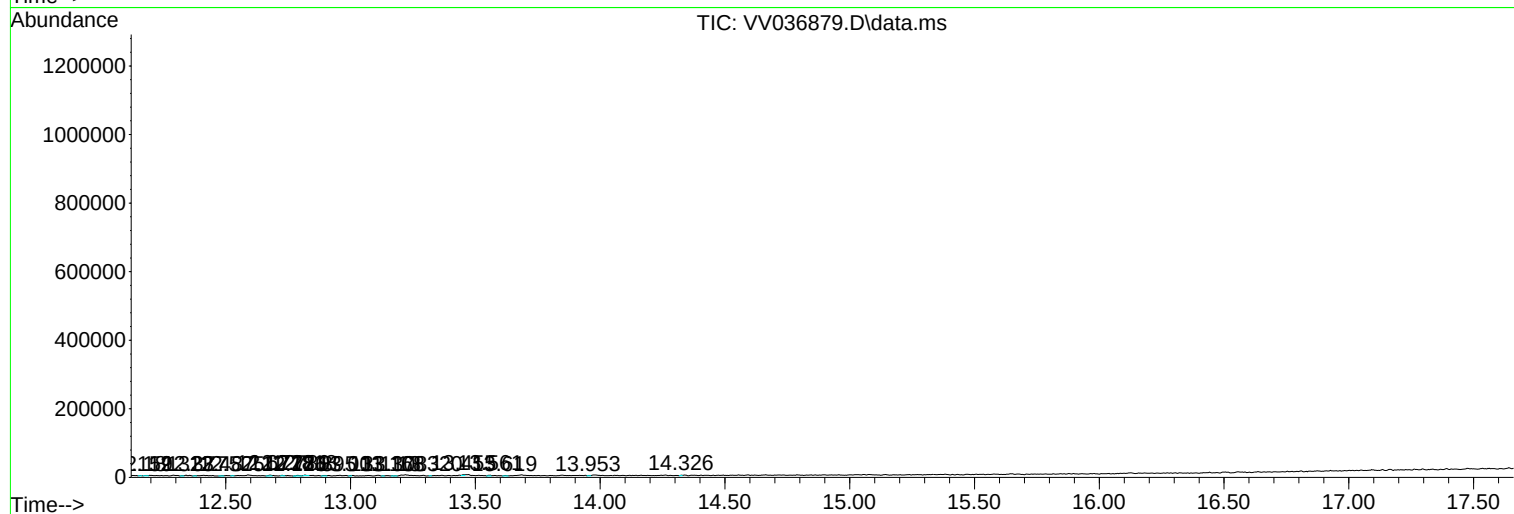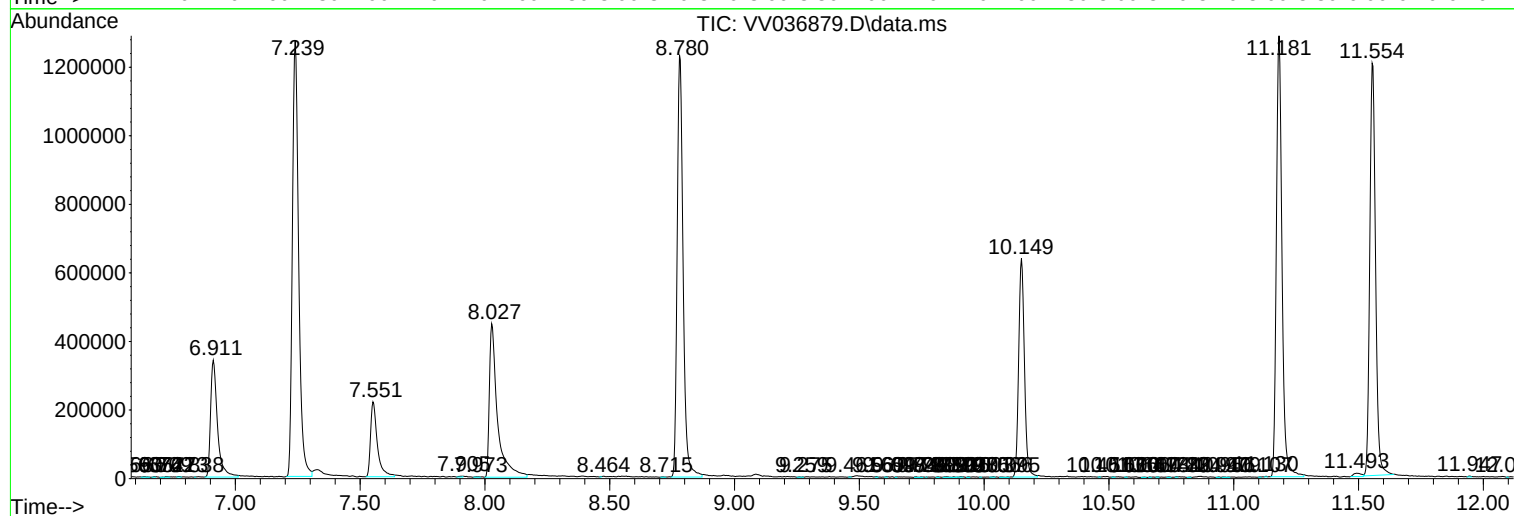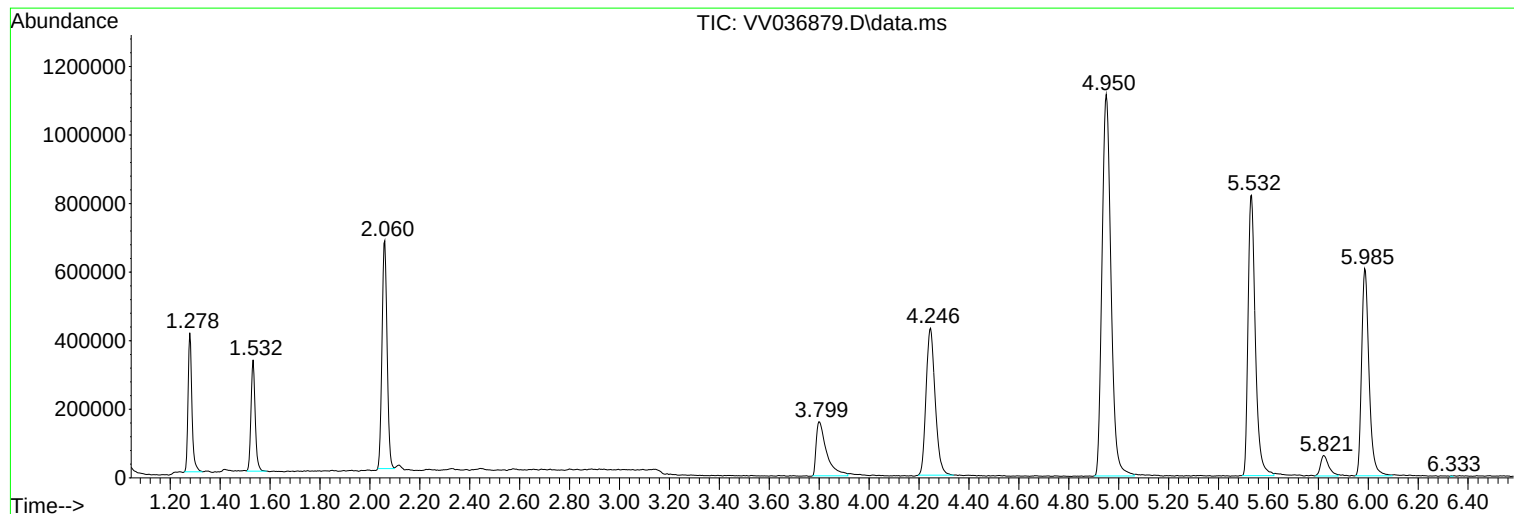

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036879.D
Acq On : 09 Aug 2024 16:22
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036879.D
Acq On : 09 Aug 2024 16:22
Operator : SY/MD
Sample : P3480-21
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------