

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036887.D
 Acq On : 09 Aug 2024 19:19
 Operator : SY/MD
 Sample : P3533-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	410355	435020	15.58%	2.137%
2	1.532	146	153	168	rVB	313122	375558	13.45%	1.845%
3	2.056	308	316	330	rBV	655944	940828	33.69%	4.622%
4	3.799	849	858	889	rBV	161622	439363	15.73%	2.158%
5	4.117	955	957	961	rBV4	1408	1405	0.05%	0.007%
6	4.246	982	997	1027	rBV	428199	1078817	38.64%	5.300%
7	4.751	1152	1154	1157	rBV4	1529	871	0.03%	0.004%
8	4.805	1169	1171	1175	rBV4	1465	885	0.03%	0.004%
9	4.828	1175	1178	1179	rBV3	1130	555	0.02%	0.003%
10	4.950	1201	1216	1244	rBV2	1124844	2792310	100.00%	13.717%
11	5.468	1375	1377	1380	rBV4	1666	934	0.03%	0.005%
12	5.532	1385	1397	1436	rVV	790530	1633332	58.49%	8.024%
13	5.825	1480	1488	1508	rVB2	40241	90516	3.24%	0.445%
14	5.985	1526	1538	1566	rBV	600286	1244638	44.57%	6.114%
15	6.281	1628	1630	1631	rBV	1662	800	0.03%	0.004%
16	6.336	1645	1647	1649	rBV2	939	453	0.02%	0.002%
17	6.606	1727	1731	1733	rBV4	1413	1285	0.05%	0.006%
18	6.635	1738	1740	1743	rVV3	1153	779	0.03%	0.004%
19	6.664	1747	1749	1751	rBV	1088	467	0.02%	0.002%
20	6.677	1751	1753	1756	rBV3	804	418	0.01%	0.002%
21	6.751	1772	1776	1779	rVB5	1354	995	0.04%	0.005%
22	6.799	1787	1791	1793	rBV5	1213	1086	0.04%	0.005%
23	6.821	1797	1798	1801	rBV3	998	499	0.02%	0.002%
24	6.863	1809	1811	1813	rBV2	667	384	0.01%	0.002%
25	6.911	1816	1826	1850	rBV	338381	634591	22.73%	3.117%
26	7.239	1917	1928	1949	rBV	1280023	2233967	80.00%	10.974%
27	7.551	2016	2025	2055	rBV	214921	404108	14.47%	1.985%
28	7.998	2160	2164	2165	rBV3	1884	1194	0.04%	0.006%
29	8.027	2165	2173	2213	rVV2	447367	964103	34.53%	4.736%
30	8.529	2326	2329	2331	rBV4	1708	1137	0.04%	0.006%
31	8.609	2352	2354	2359	rBV6	1170	822	0.03%	0.004%
32	8.728	2389	2391	2393	rVB3	835	348	0.01%	0.002%
33	8.779	2396	2407	2435	rBV	1187754	1988455	71.21%	9.768%
34	9.323	2575	2576	2580	rBV4	1064	585	0.02%	0.003%
35	9.374	2589	2592	2594	rBV3	1156	820	0.03%	0.004%
36	9.423	2605	2607	2611	rVB5	1304	606	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
 Data File : VV036887.D
 Acq On : 09 Aug 2024 19:19
 Operator : SY/MD
 Sample : P3533-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.603	2660	2663	2668	rBV7	1194	1124	0.04%	0.006%
38	9.644	2673	2676	2679	rBV4	1312	1203	0.04%	0.006%
39	9.699	2691	2693	2695	rBV2	926	545	0.02%	0.003%
40	9.715	2695	2698	2699	rBV3	1038	557	0.02%	0.003%
41	9.757	2709	2711	2713	rVB3	688	306	0.01%	0.002%
42	9.770	2713	2715	2716	rBV2	523	221	0.01%	0.001%
43	9.779	2716	2718	2719	rVV2	758	239	0.01%	0.001%
44	9.815	2727	2729	2734	rBV5	1122	1204	0.04%	0.006%
45	9.895	2753	2754	2756	rVB2	780	270	0.01%	0.001%
46	9.924	2761	2763	2764	rBV2	1255	520	0.02%	0.003%
47	9.947	2768	2770	2771	rVB2	1112	353	0.01%	0.002%
48	9.960	2771	2774	2776	rBV4	1331	819	0.03%	0.004%
49	9.988	2781	2783	2788	rBV6	1651	1072	0.04%	0.005%
50	10.062	2804	2806	2809	rVB2	1680	1056	0.04%	0.005%
51	10.082	2809	2812	2813	rVB	1123	507	0.02%	0.002%
52	10.095	2813	2816	2817	rBV3	1300	690	0.02%	0.003%
53	10.149	2822	2833	2851	rBV	678119	1070411	38.33%	5.258%
54	10.635	2982	2984	2988	rVB5	1318	798	0.03%	0.004%
55	10.657	2988	2991	2992	rBV3	873	539	0.02%	0.003%
56	10.686	2997	3000	3001	rVV3	908	657	0.02%	0.003%
57	10.709	3005	3007	3009	rBV3	494	220	0.01%	0.001%
58	10.728	3009	3013	3017	rVB6	1684	1399	0.05%	0.007%
59	10.750	3017	3020	3023	rBV6	698	535	0.02%	0.003%
60	10.773	3023	3027	3029	rBV4	940	887	0.03%	0.004%
61	10.812	3037	3039	3043	rVB5	1334	942	0.03%	0.005%
62	10.834	3043	3046	3049	rBV4	1108	950	0.03%	0.005%
63	10.866	3052	3056	3060	rVV7	2259	2032	0.07%	0.010%
64	10.937	3076	3078	3083	rVB5	1379	888	0.03%	0.004%
65	10.959	3083	3085	3086	rBV2	1096	491	0.02%	0.002%
66	10.998	3096	3097	3098	rBV	432	110	0.00%	0.001%
67	11.014	3100	3102	3104	rBV4	793	375	0.01%	0.002%
68	11.046	3110	3112	3114	rVB3	885	264	0.01%	0.001%
69	11.107	3128	3131	3132	rBV2	1255	707	0.03%	0.003%
70	11.181	3142	3154	3181	rBV	1263467	1986312	71.14%	9.758%
71	11.461	3237	3241	3242	rBV4	1606	1189	0.04%	0.006%
72	11.554	3258	3270	3302	rBV	1241412	1991734	71.33%	9.784%
73	12.117	3440	3445	3446	rBV4	1329	1135	0.04%	0.006%
74	12.271	3491	3493	3497	rVB4	1089	748	0.03%	0.004%
75	12.320	3506	3508	3510	rBV2	1220	698	0.02%	0.003%
76	12.365	3519	3522	3526	rVB5	1453	1282	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036887.D
Acq On : 09 Aug 2024 19:19
Operator : SY/MD
Sample : P3533-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	12.387	3526	3529	3531	rBV4	1925	1340	0.05%	0.007%
78	12.686	3621	3622	3623	rBV	885	209	0.01%	0.001%
79	12.696	3623	3625	3628	rVV4	863	595	0.02%	0.003%
80	12.914	3691	3693	3694	rBV2	702	191	0.01%	0.001%
81	12.943	3700	3702	3703	rBV2	1181	499	0.02%	0.002%
82	13.085	3744	3746	3750	rVB3	1348	497	0.02%	0.002%
83	13.265	3799	3802	3804	rBV4	1464	1101	0.04%	0.005%
84	13.348	3827	3828	3831	rBV2	1235	647	0.02%	0.003%
85	13.451	3857	3860	3863	rBV4	2729	2463	0.09%	0.012%




Sum of corrected areas: 20356465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036887.D
Acq On : 09 Aug 2024 19:19
Operator : SY/MD
Sample : P3533-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

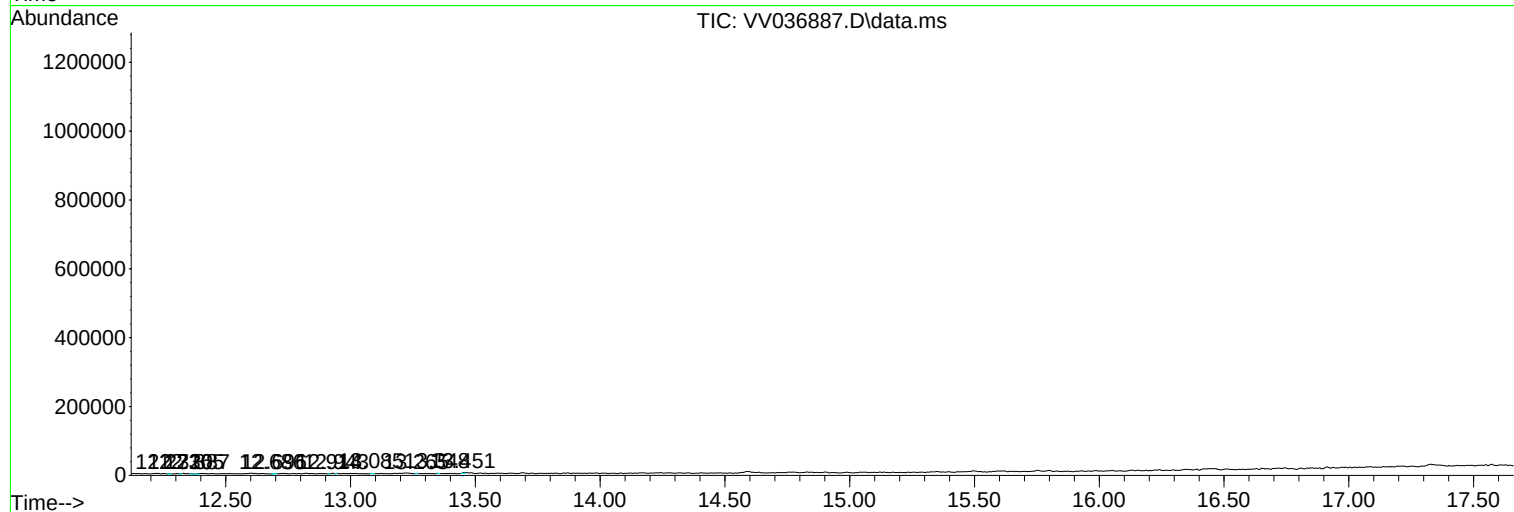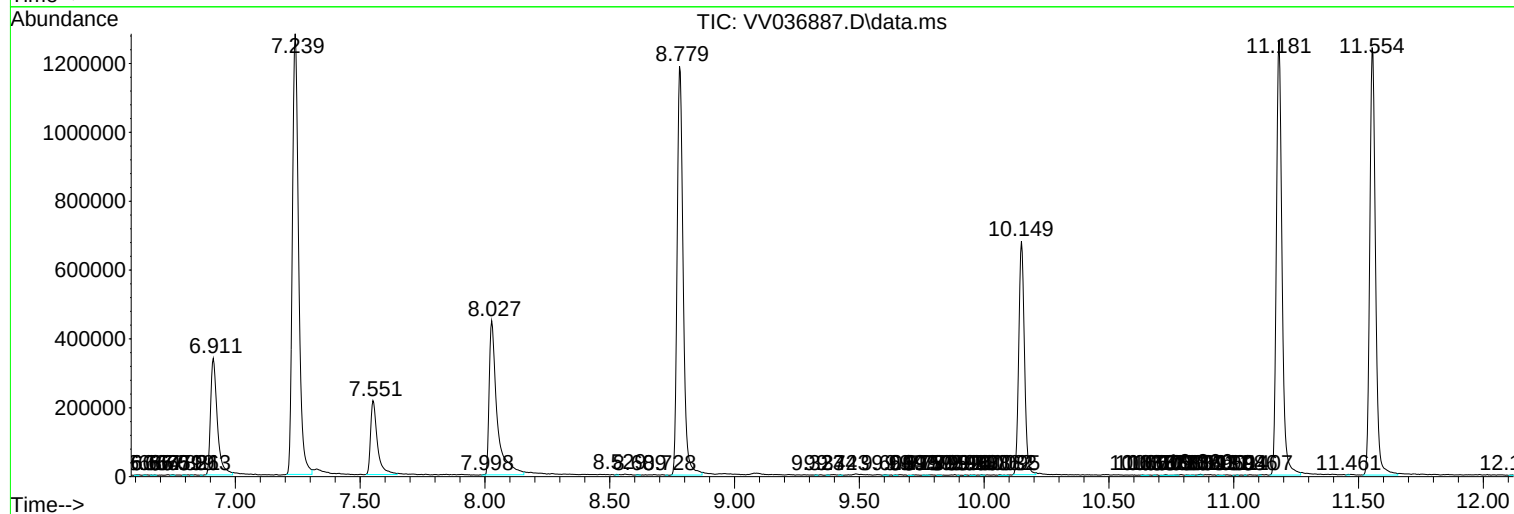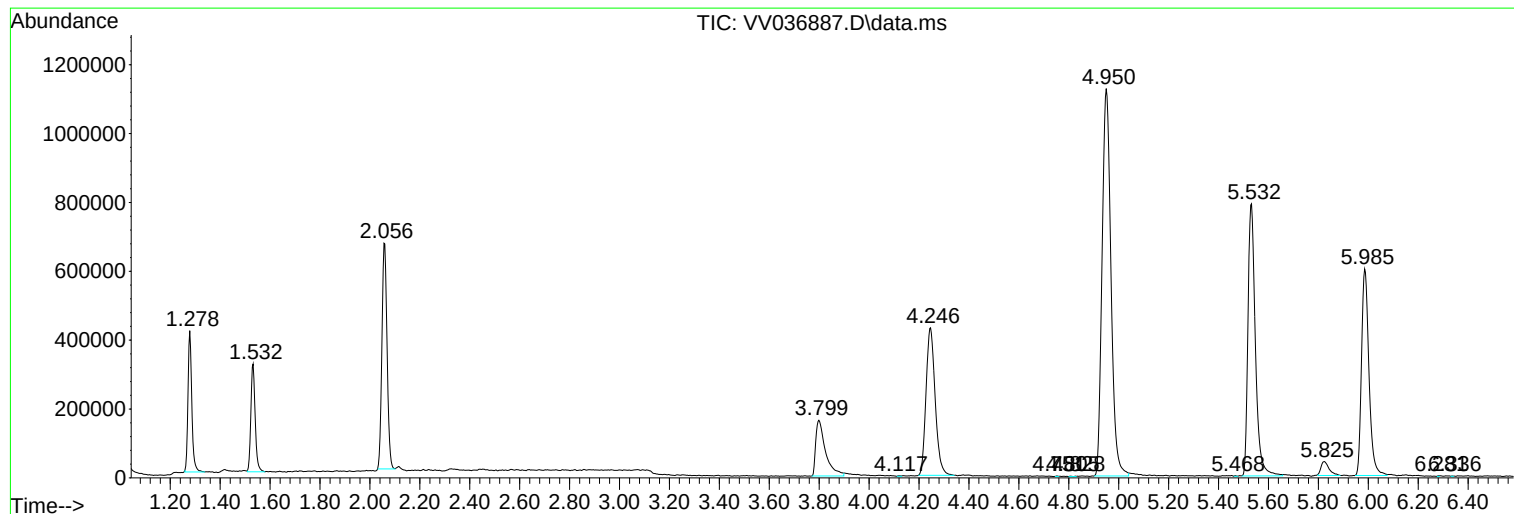

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036887.D
Acq On : 09 Aug 2024 19:19
Operator : SY/MD
Sample : P3533-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036887.D
Acq On : 09 Aug 2024 19:19
Operator : SY/MD
Sample : P3533-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AG0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc