


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV080924\
Data File : VV036864.D
Acq On : 09 Aug 2024 09:28
Operator : SY/MD
Sample : BFB358
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB358

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Tue Aug 13 02:57:00 2024

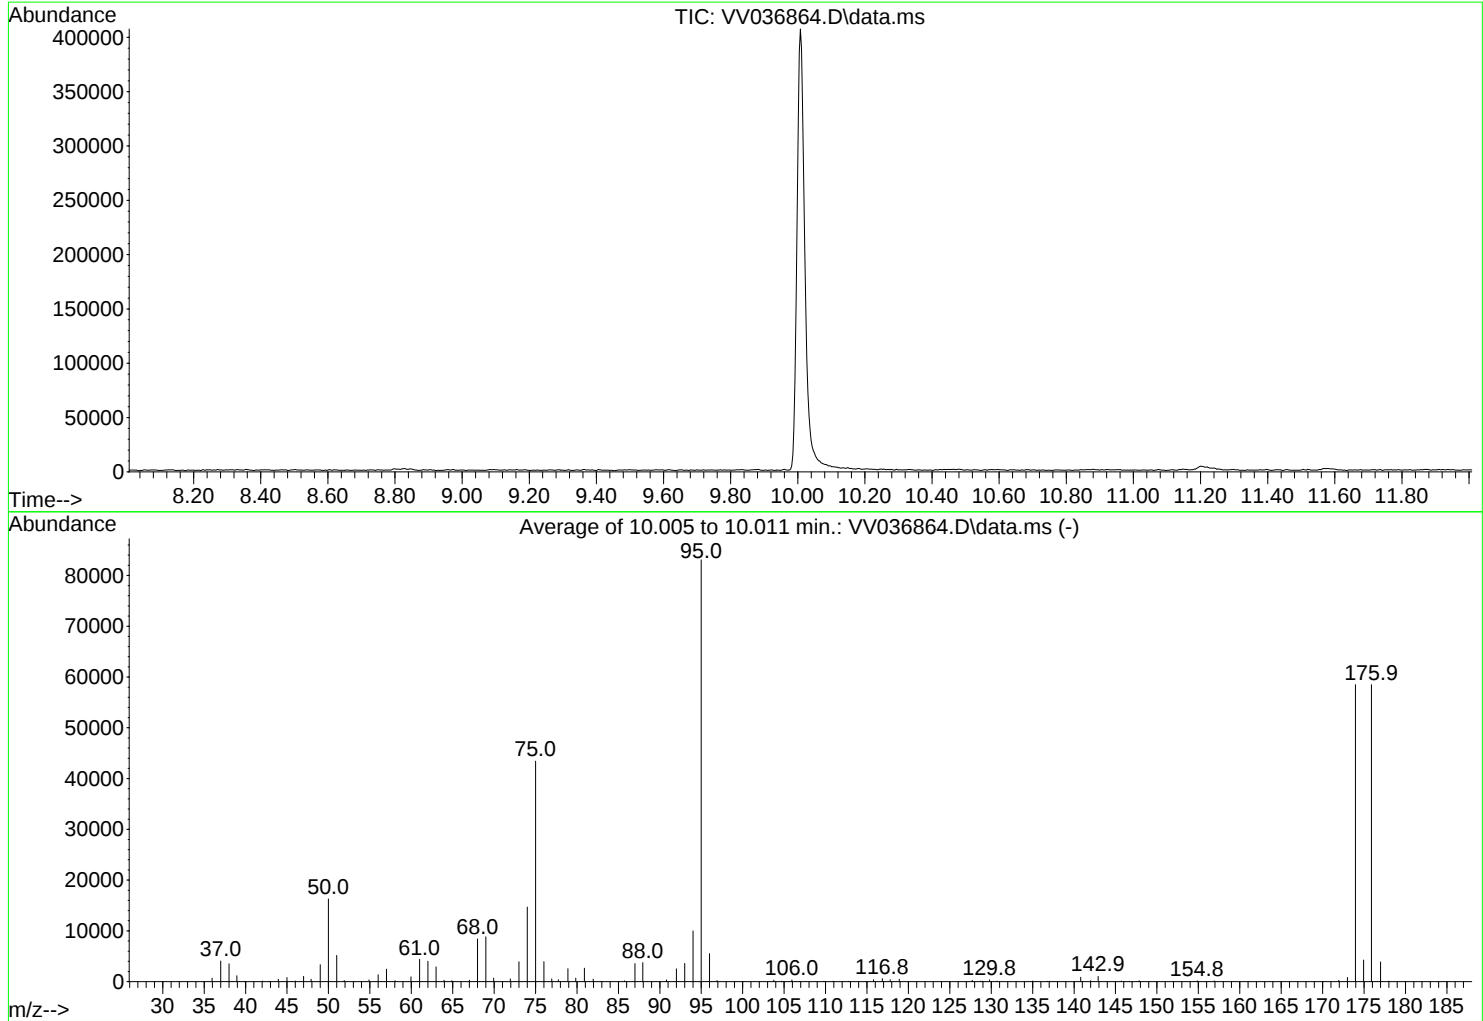

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	16281	PASS
75	95	30	80	52.3	43435	PASS
95	95	100	100	100.0	83077	PASS
96	95	5	9	6.6	5513	PASS
173	174	0.00	2	1.4	837	PASS
174	95	50	120	70.4	58477	PASS
175	174	5	9	7.3	4270	PASS
176	174	95	105	100.0	58504	PASS
177	176	5	10	6.7	3893	PASS

m/z	Abundance
38.90	113.0
39.90	275.0
41.10	124.0
42.90	150.0
43.90	936.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
36.00	640.0
37.00	4080.0
38.00	3527.0
39.00	1330.0
39.80	325.0
40.90	108.0
42.10	110.0
42.80	194.0
44.00	1387.0
45.00	859.0
46.00	103.0
47.00	985.0
47.90	460.0
49.00	3409.0
50.00	16155.0
51.00	5381.0
51.90	206.0
54.90	353.0
56.00	1391.0
57.00	2484.0
58.00	181.0
60.00	910.0
61.00	4205.0
62.00	4101.0
63.00	2704.0
63.90	286.0
64.80	172.0
67.00	253.0
68.00	8516.0
69.00	8758.0
69.90	688.0
71.90	567.0
73.00	3866.0
74.00	14579.0
75.00	43264.0
76.00	4079.0
77.00	557.0
77.70	377.0
78.90	2485.0
79.90	723.0
80.90	2741.0
81.90	552.0
85.80	148.0
87.00	3491.0
87.90	3889.0
90.80	322.0
92.00	2443.0
93.00	3523.0
94.00	9695.0
95.00	81288.0
96.00	5410.0
96.90	265.0
103.70	271.0
104.70	156.0
105.90	342.0
106.90	108.0
110.90	140.0
115.80	380.0
116.80	577.0
117.80	383.0
118.90	479.0
127.70	273.0
128.80	133.0
128.90	134.0
129.80	270.0
130.70	127.0
135.00	125.0
137.10	122.0
140.80	847.0
142.00	168.0
142.90	989.0
145.70	113.0
147.90	203.0
154.80	161.0
156.90	121.0
172.00	301.0
173.00	814.0
173.90	55880.0
174.90	4241.0
175.90	55768.0
177.00	3875.0
178.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	689.0
37.00	4181.0
38.00	3597.0
39.00	1316.0
39.90	318.0
42.00	127.0
42.80	186.0
44.00	1424.0
45.00	834.0
46.00	121.0
47.00	1068.0
47.90	503.0
49.00	3393.0
50.00	16872.0
51.00	5335.0
51.90	235.0
54.90	344.0
56.00	1400.0
57.00	2570.0
58.10	196.0
60.00	1006.0
61.00	4585.0
62.00	4092.0
63.00	3010.0
63.90	294.0
64.90	186.0
67.00	284.0
68.00	8662.0
69.00	9140.0
69.90	712.0
71.90	536.0
73.00	4051.0
74.00	15316.0
75.00	44928.0
76.00	4113.0
77.00	547.0
77.80	394.0
78.90	2616.0
79.90	724.0
80.90	2745.0
81.90	511.0
85.80	151.0
87.00	3737.0
87.90	3907.0
90.80	350.0
92.00	2583.0
93.00	3718.0
94.00	10345.0
95.00	86080.0
96.00	5650.0
96.90	234.0
103.80	308.0
104.70	156.0
106.00	368.0
110.90	137.0
112.70	107.0
115.80	393.0
116.90	611.0
117.80	417.0
118.90	525.0
127.70	303.0
129.00	154.0
129.80	354.0
130.70	123.0
135.00	138.0
137.00	127.0
140.80	880.0
142.00	215.0
142.90	1092.0
145.70	146.0
146.70	114.0
147.90	171.0
154.80	156.0
156.90	176.0
171.90	239.0
173.00	848.0
173.90	60400.0
174.90	4386.0
175.90	60648.0
177.00	3958.0
178.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358

m/z	Abundance
35.90	720.0
37.00	3980.0
38.00	3370.0
39.00	1220.0
39.90	296.0
40.90	106.0
42.00	139.0
42.90	178.0
44.00	1380.0
45.00	755.0
46.00	133.0
47.00	1061.0
47.90	508.0
49.00	3244.0
50.00	15816.0
51.00	4829.0
51.90	249.0
54.90	326.0
56.00	1272.0
57.00	2364.0
58.00	187.0
59.90	964.0
61.00	4330.0
62.00	3777.0
63.00	2967.0
64.00	291.0
65.00	188.0
67.00	278.0
68.00	8099.0
69.00	8592.0
70.00	664.0
71.00	111.0
72.00	500.0
73.00	3851.0
74.00	14213.0
75.00	42112.0
76.00	3654.0
76.90	505.0
77.80	411.0
78.90	2531.0
79.80	658.0
80.90	2489.0
82.00	479.0
82.80	128.0
85.70	142.0
86.00	107.0
87.00	3471.0
88.00	3427.0
90.80	362.0
92.00	2512.0
93.00	3531.0
94.00	9893.0
95.00	81864.0
96.00	5479.0
96.90	168.0
103.80	358.0
104.90	139.0
105.90	326.0
109.80	115.0
112.80	106.0
114.80	119.0
115.80	350.0
116.80	568.0
117.80	372.0
118.90	458.0
127.70	298.0
128.70	141.0
129.80	398.0
135.00	138.0
136.80	164.0
140.80	807.0
142.00	227.0
142.90	1071.0
145.70	163.0
146.70	118.0
147.80	162.0
154.90	176.0
156.90	196.0
171.90	199.0
173.00	848.0
174.00	59152.0
175.00	4184.0
175.90	59096.0
177.00	3847.0
178.00	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB358