

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
 Data File : VV027367.D
 Acq On : 13 Aug 2022 14:16
 Operator : SY/MD
 Sample : N4115-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 13 21:52:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 21:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)

Internal Standards					
1) 1,4-Difluorobenzene	5.612	114	155239	5.000 ug/L	0.00
28) Chlorobenzene-d5	8.850	117	172053	5.000 ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77536	5.000 ug/L	0.00

System Monitoring Compounds					
4) Vinyl Chloride-d3	1.304	65	58672	4.350 ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	= 87.000%
7) Chloroethane-d5	1.561	69	43839	4.476 ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	= 89.600%
11) 1,1-Dichloroethene-d2	2.101	63	66066	2.701 ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	= 54.000%#
20) 2-Butanone-d5	3.867	46	200580	87.814 ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	= 175.620%#
24) Chloroform-d	4.342	84	129305	5.228 ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 104.600%
26) 1,2-Dichloroethane-d4	5.027	65	64119	5.441 ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 108.800%
32) Benzene-d6	5.047	84	199537	3.931 ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	= 78.600%
36) 1,2-Dichloropropane-d6	6.066	67	79327	5.055 ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	= 101.200%
41) Toluene-d8	7.313	98	157540	3.391 ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	= 67.800%#
43) trans-1,3-Dichloroprop...	7.622	79	20834	3.833 ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	= 76.600%
46) 2-Hexanone-d5	8.085	63	147154	69.952 ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	= 139.900%#
56) 1,1,2,2-Tetrachloroeth...	10.214	84	68935	6.072 ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	= 121.400%#
66) 1,2-Dichlorobenzene-d4	11.622	152	72770	5.438 ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	= 108.800%


Target Compounds				Qvalue	
6) Bromomethane	1.513	94	542	0.067 ug/L	74
8) Chloroethane	1.339	64	689323	72.031 ug/L #	52
13) Acetone	2.159	43	11563	6.850 ug/L	99
14) Carbon disulfide	2.288	76	4573	0.102 ug/L #	93
18) trans-1,2-Dichloroethene	2.757	96	1273	0.093 ug/L	96
22) cis-1,2-Dichloroethene	3.908	96	11857	0.877 ug/L	94
33) Benzene	5.104	78	8315	0.141 ug/L	100
35) Methylcyclohexane	6.066	83	18559	0.921 ug/L #	16
42) Toluene	7.384	91	179877	3.066 ug/L	99
52) Ethylbenzene	9.017	91	4187	0.071 ug/L	85
53) m,p-Xylene	9.140	106	2680	0.119 ug/L	98
60) Isopropylbenzene	10.455	105	2221	0.045 ug/L #	88
61) 1,2,3-Trichloropropane	11.246	75	9520	1.275 ug/L #	66
62) 1,3,5-Trimethylbenzene	10.542	105	1946	0.144 ug/L	98
63) 1,2,4-Trimethylbenzene	10.918	105	2693	0.070 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027367.D
Acq On : 13 Aug 2022 14:16
Operator : SY/MD
Sample : N4115-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Aug 13 21:52:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 21:49:38 2022
Response via : Initial Calibration




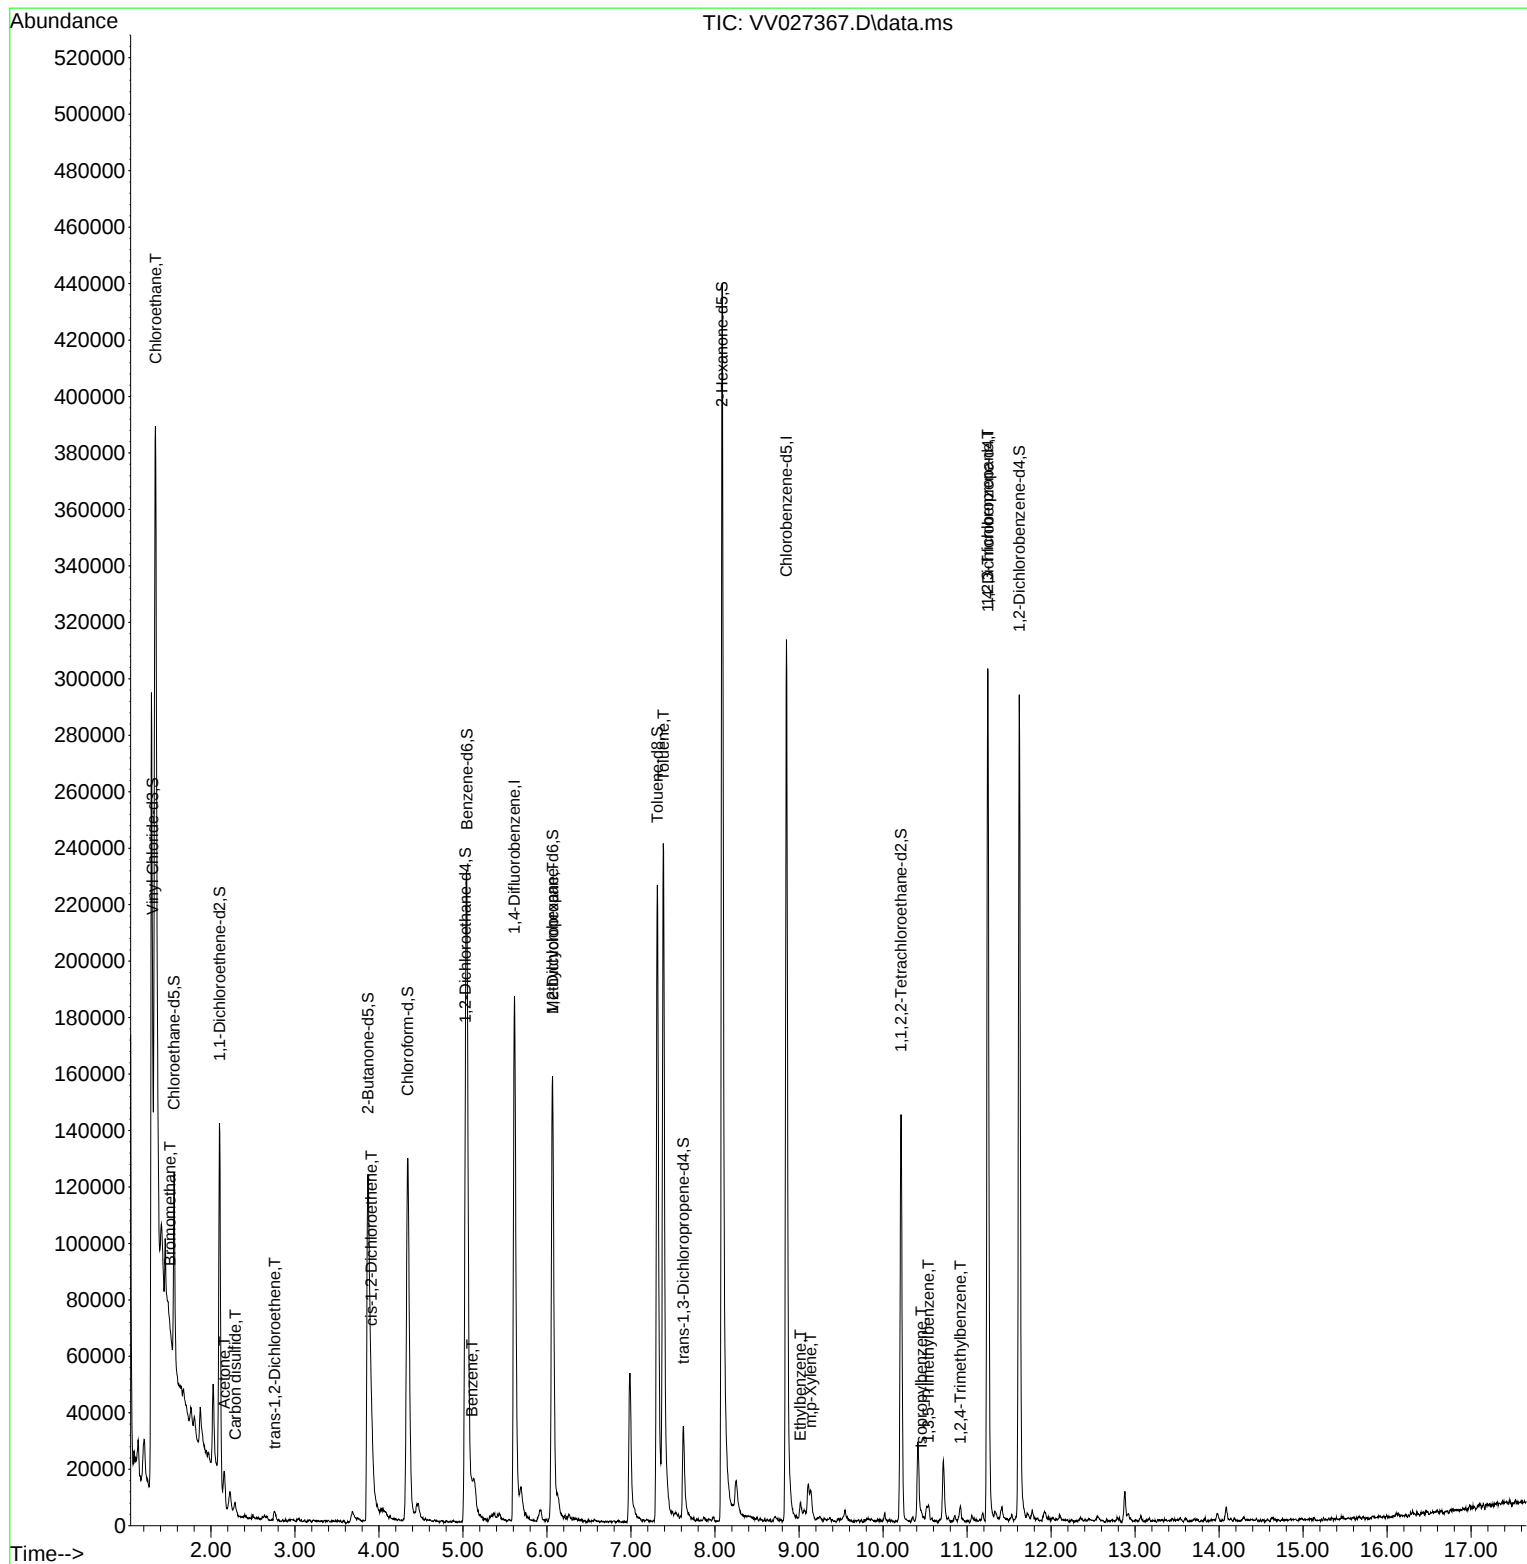


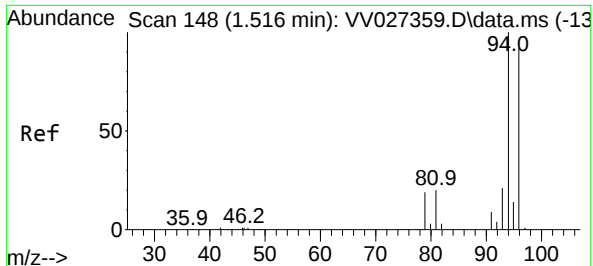

#6
Bromomethane
Concen: 0.067 ug/L
RT: 1.513 min Scan# 14
Delta R.T. -0.003 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 94 Resp: 542
Ion Ratio Lower Upper
94 100
96 71.1 67.2 124.8

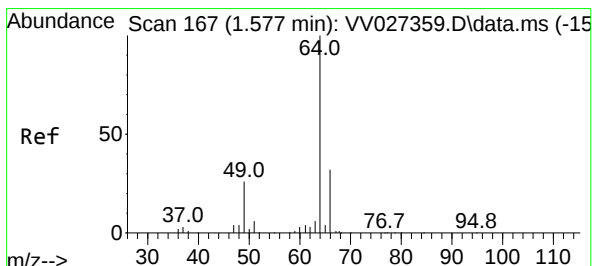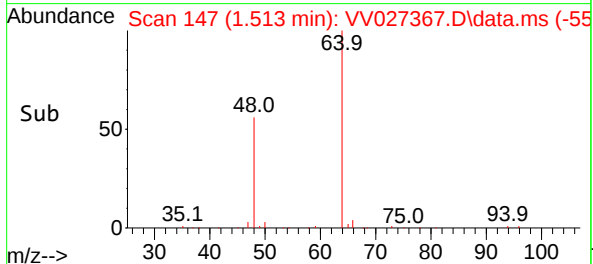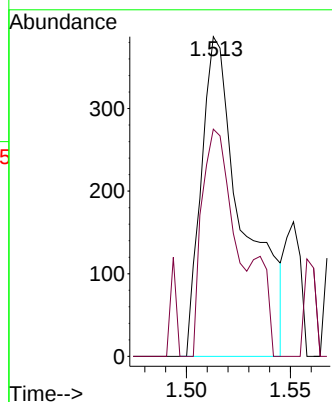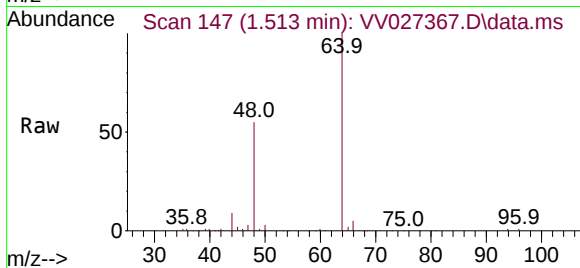

#8
Chloroethane
Concen: 72.031 ug/L
RT: 1.339 min Scan# 93
Delta R.T. -0.238 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Tgt Ion: 64 Resp: 689323
Ion Ratio Lower Upper
64 100
66 4.9 22.3 41.5#

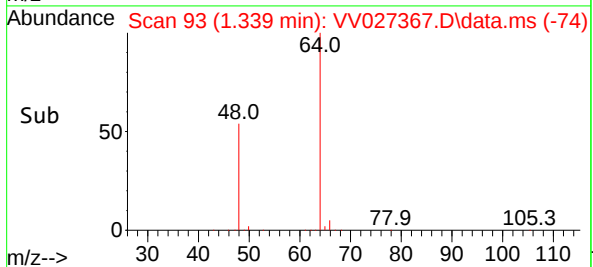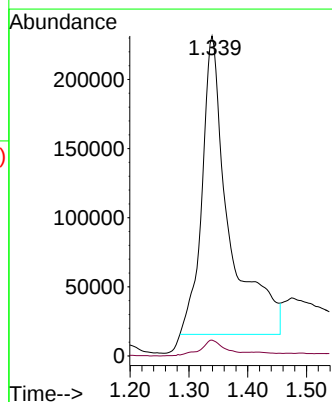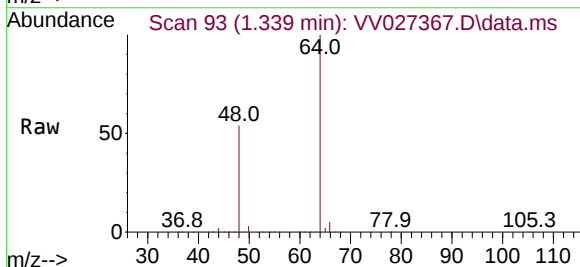

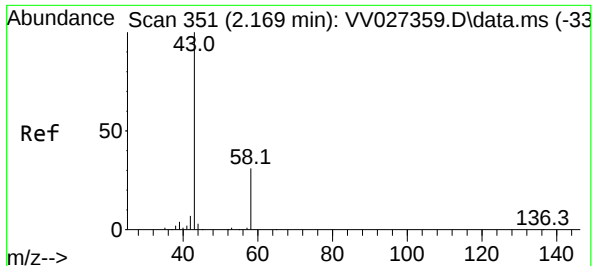

#13

Acetone

Concen: 6.850 ug/L

RT: 2.159 min Scan# 34

Delta R.T. -0.010 min

Lab File: VV027367.D

Acq: 13 Aug 2022 14:16

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 11563

Ion Ratio Lower Upper

43 100

58 30.9 0.0 63.2

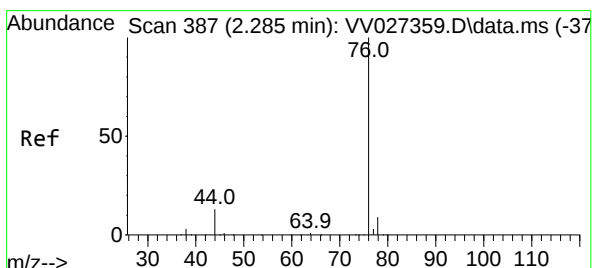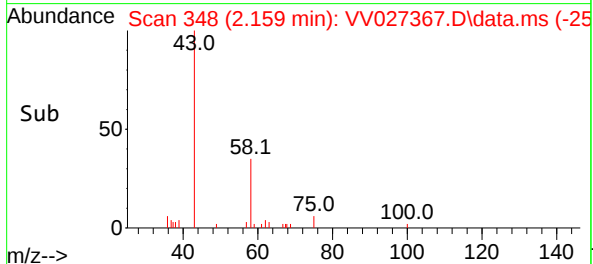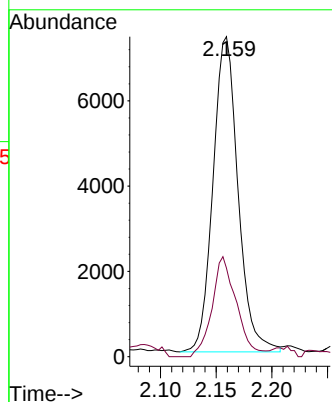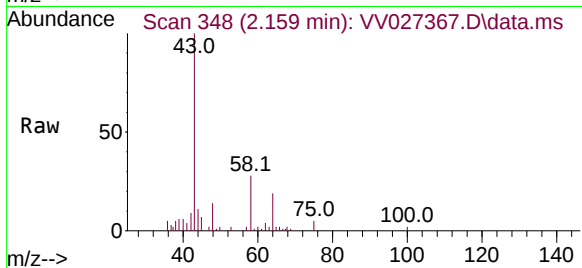

#14

Carbon disulfide

Concen: 0.102 ug/L

RT: 2.288 min Scan# 388

Delta R.T. 0.003 min

Lab File: VV027367.D




Acq: 13 Aug 2022 14:16


Tgt Ion: 76 Resp: 4573

Ion Ratio Lower Upper

76 100


78 11.5 7.2 10.8#

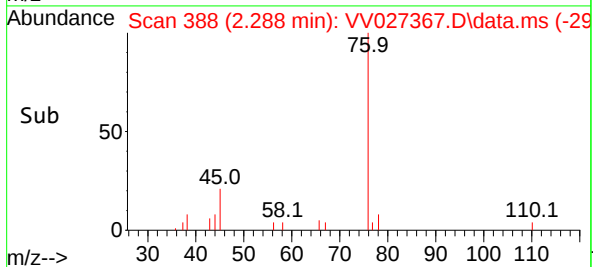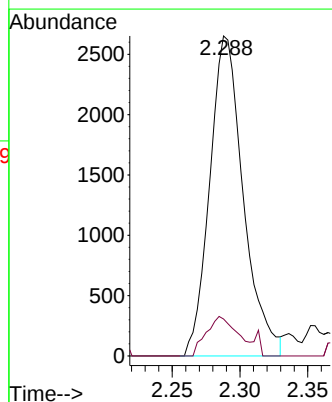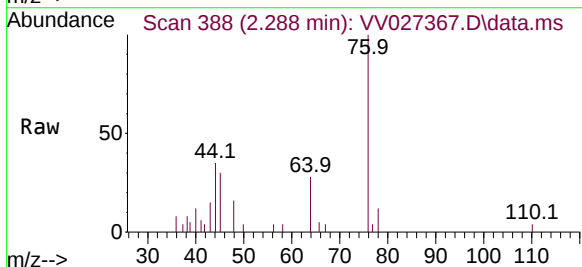

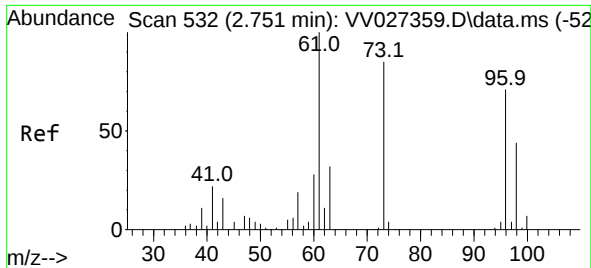




#18
trans-1,2-Dichloroethene
Concen: 0.093 ug/L
RT: 2.757 min Scan# 511
Delta R.T. 0.006 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Instrument :
MSVOA_V
ClientSampleId :

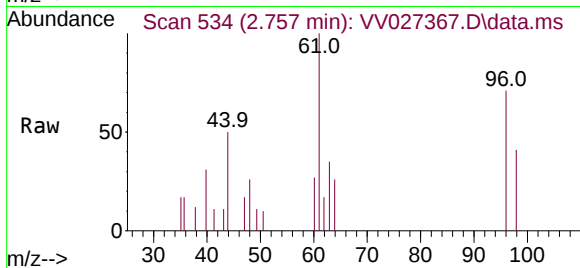

Tgt Ion: 96 Resp: 1273




Ion	Ratio	Lower	Upper
96	100		
61	140.3	99.6	185.0
98	57.2	45.1	83.7

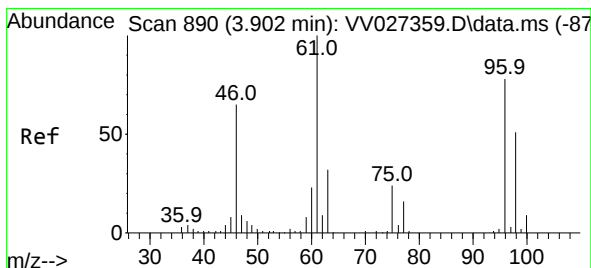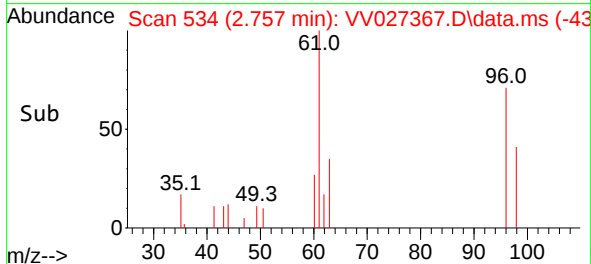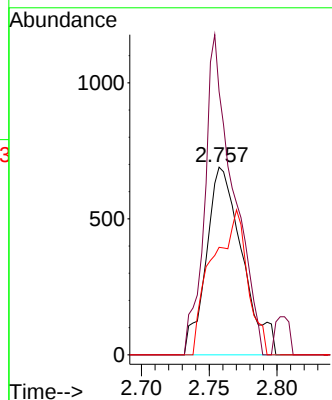


#22
cis-1,2-Dichloroethene
Concen: 0.877 ug/L
RT: 3.908 min Scan# 892
Delta R.T. 0.006 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Tgt Ion: 96 Resp: 11857

Ion	Ratio	Lower	Upper
96	100		
61	136.8	91.3	169.5
68	0.0	0.0	0.0


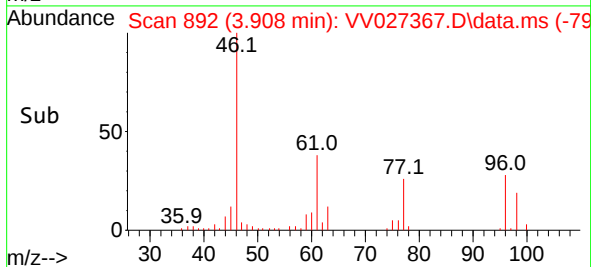
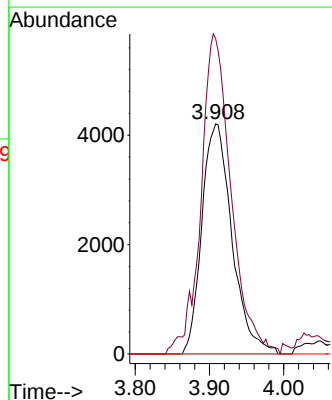
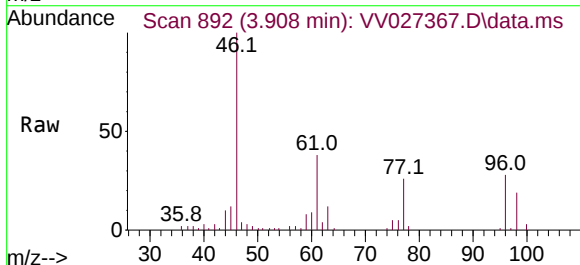


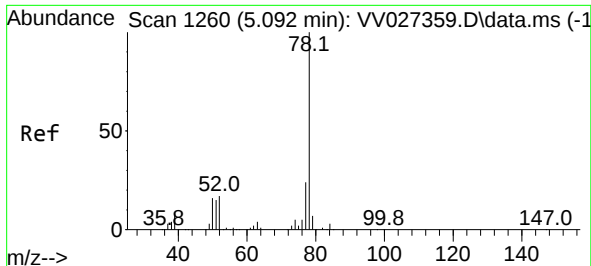

#33
Benzene
Concen: 0.141 ug/L
RT: 5.104 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 78 Resp: 8315

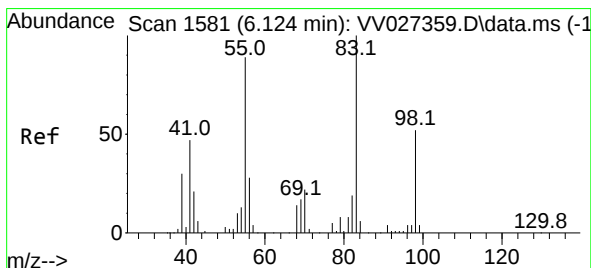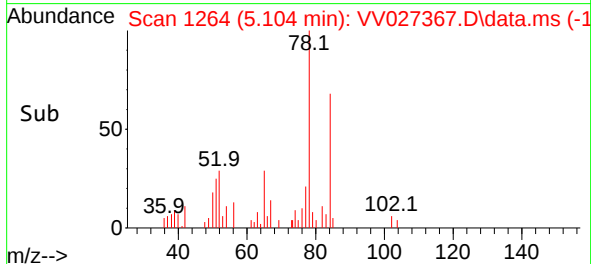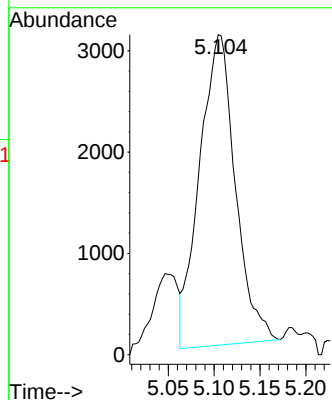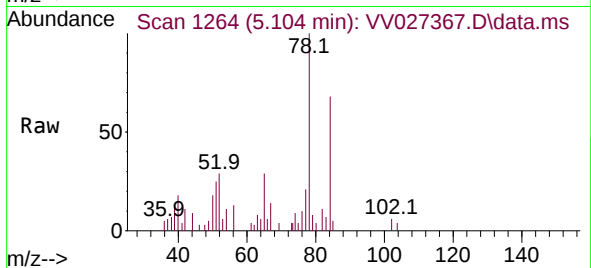

#35
Methylcyclohexane
Concen: 0.921 ug/L
RT: 6.066 min Scan# 1563
Delta R.T. -0.058 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Tgt Ion: 83 Resp: 18559
Ion Ratio Lower Upper
83 100
55 0.1 67.0 100.6#
98 1.2 38.7 58.1#


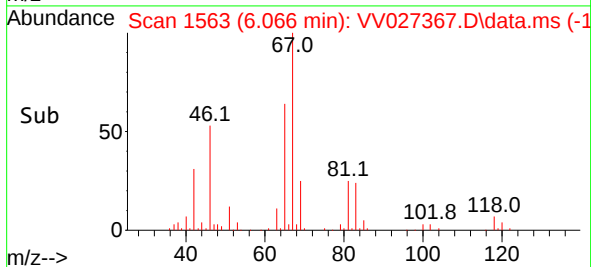
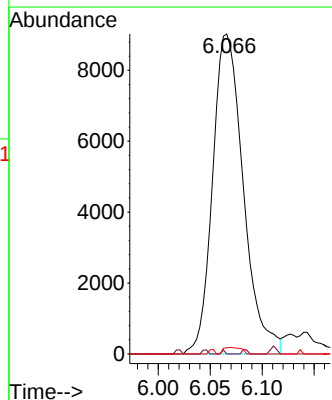
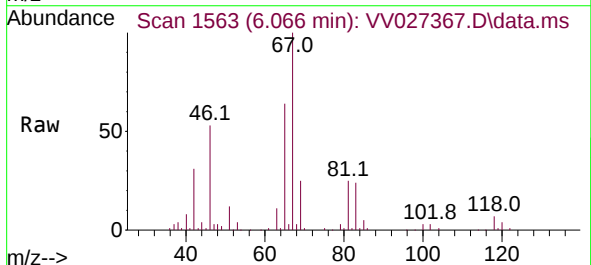


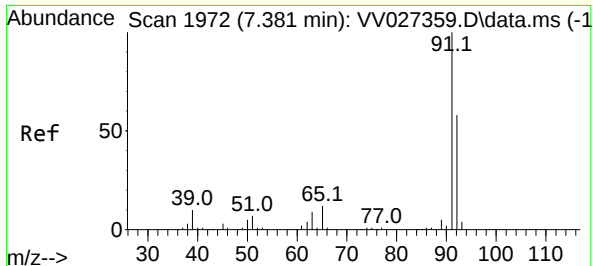

#42
Toluene
Concen: 3.066 ug/L
RT: 7.384 min Scan# 1972
Delta R.T. 0.003 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 91 Resp: 179877
Ion Ratio Lower Upper
91 100
92 56.1 39.9 74.1

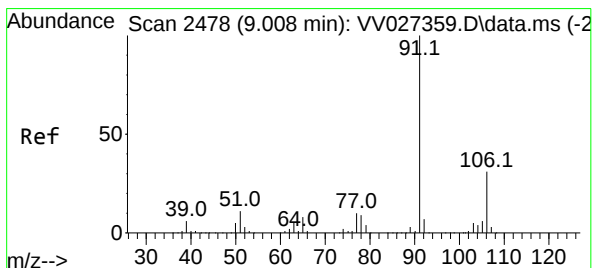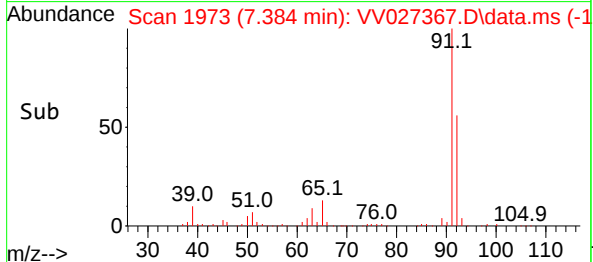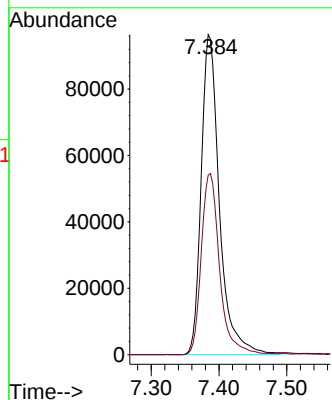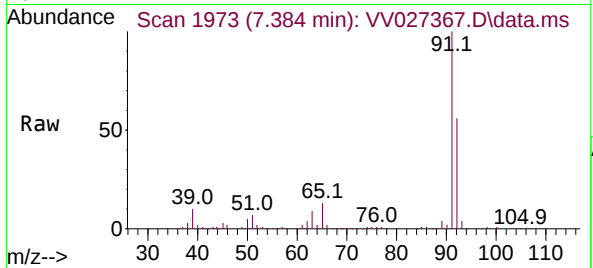

#52
Ethylbenzene
Concen: 0.071 ug/L
RT: 9.017 min Scan# 2481
Delta R.T. 0.010 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Tgt Ion: 91 Resp: 4187
Ion Ratio Lower Upper
91 100
106 39.0 21.5 39.9


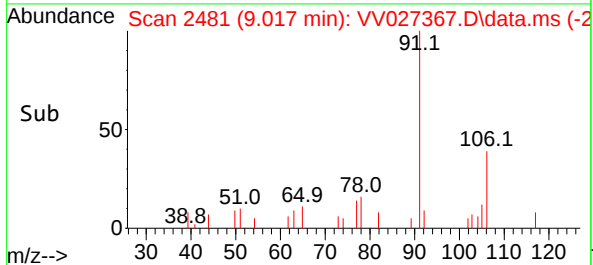
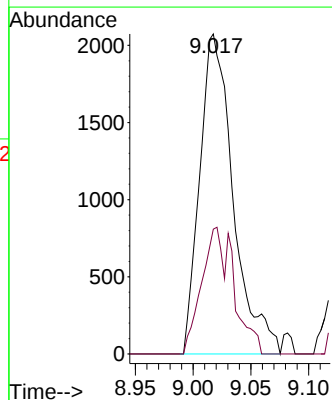
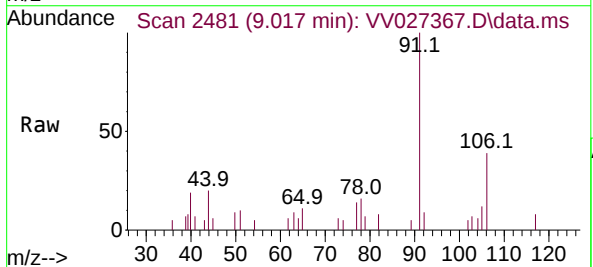


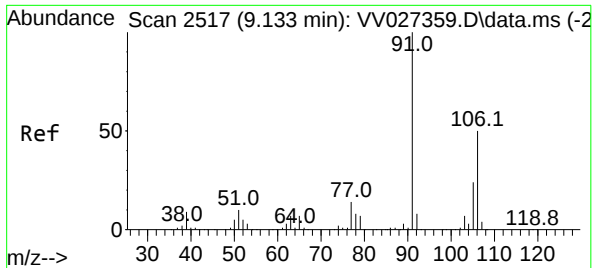

#53
m,p-Xylene
Concen: 0.119 ug/L
RT: 9.140 min Scan# 21
Delta R.T. 0.006 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:106 Resp: 2680
Ion Ratio Lower Upper
106 100
91 204.9 141.5 262.9

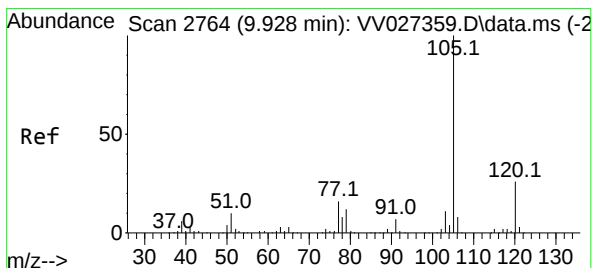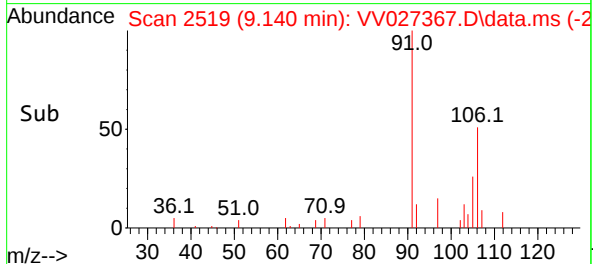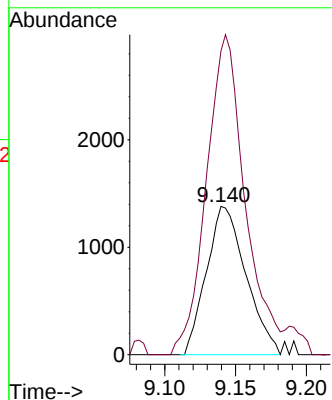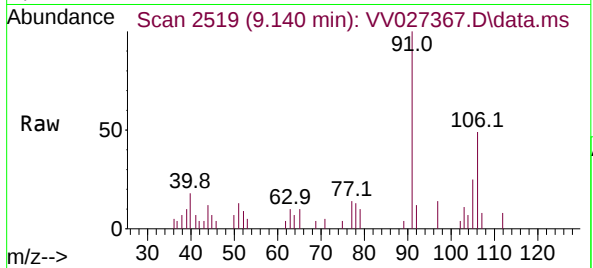

#60
Isopropylbenzene
Concen: 0.045 ug/L
RT: 10.455 min Scan# 2928
Delta R.T. 0.527 min
Lab File: VV027367.D
Acq: 13 Aug 2022 14:16

Tgt Ion:105 Resp: 2221
Ion Ratio Lower Upper
105 100
120 35.7 21.0 31.4#
77 16.7 13.2 19.8


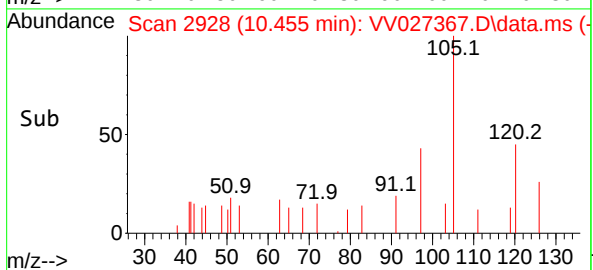
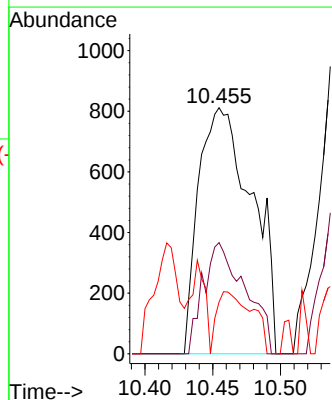
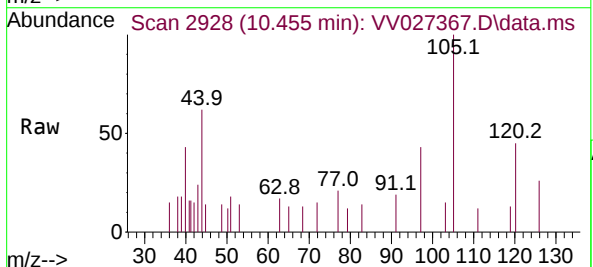


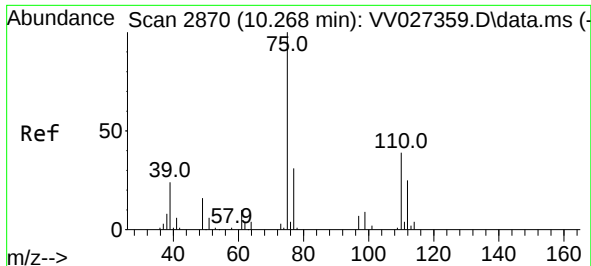

#61
 1,2,3-Trichloropropane
 Concen: 1.275 ug/L
 RT: 11.246 min Scan# 3174
 Delta R.T. 0.977 min
 Lab File: VV027367.D
 Acq: 13 Aug 2022 14:16




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion: 75 Resp: 9520
 Ion Ratio Lower Upper
 75 100
 77 35.3 26.6 39.8
 110 2.4 31.0 46.6#

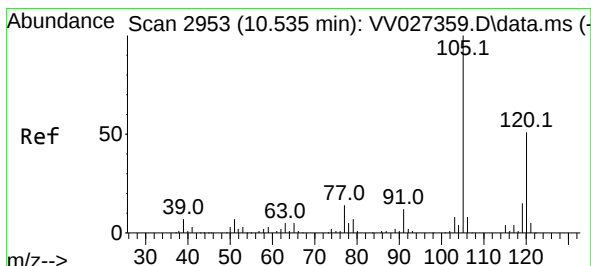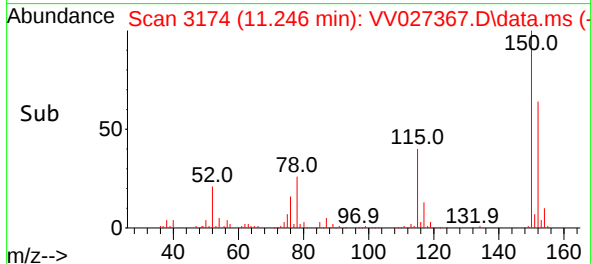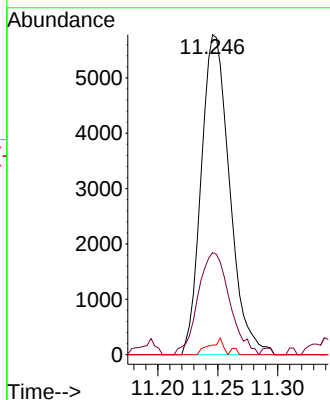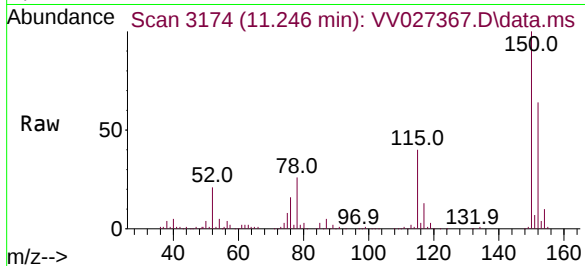

#62
 1,3,5-Trimethylbenzene
 Concen: 0.144 ug/L
 RT: 10.542 min Scan# 2955
 Delta R.T. 0.006 min
 Lab File: VV027367.D
 Acq: 13 Aug 2022 14:16


Tgt Ion: 105 Resp: 1946
 Ion Ratio Lower Upper
 105 100
 120 46.6 38.2 57.4

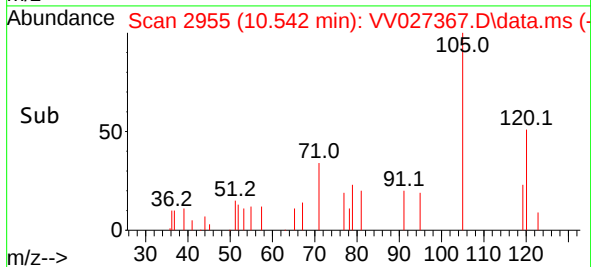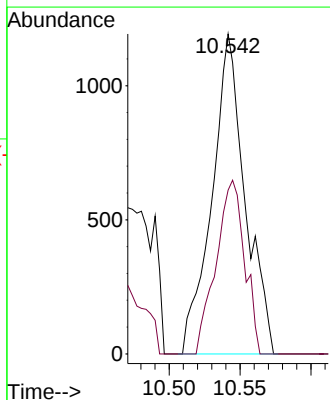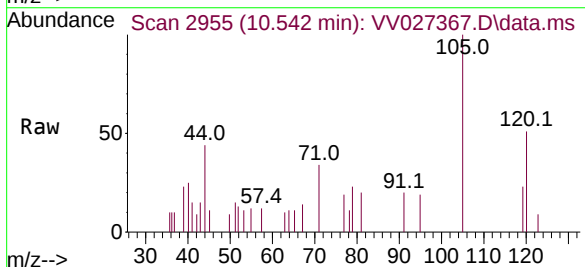

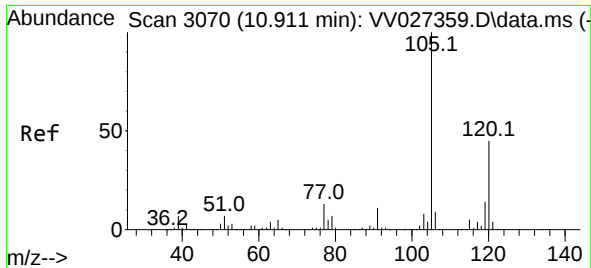

#63
 1,2,4-Trimethylbenzene
 Concen: 0.070 ug/L
 RT: 10.918 min Scan# 3072
 Delta R.T. 0.006 min
 Lab File: VV027367.D
 Acq: 13 Aug 2022 14:16

Instrument :
 MSVOA_V
 ClientSampleId :

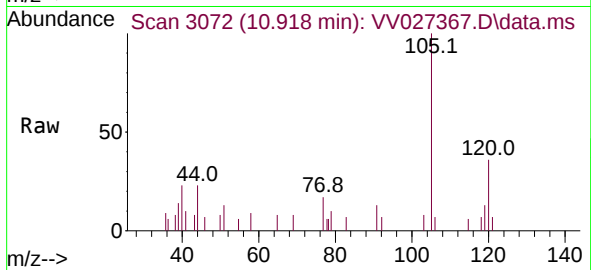

Tgt Ion:105 Resp: 2693
 Ion Ratio Lower Upper
 105 100
 120 43.9 36.2 54.2

