

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
 Data File : VV027360.D
 Acq On : 13 Aug 2022 10:51
 Operator : SY/MD
 Sample : VV0813WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK203

Quant Time: Aug 13 21:50:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 21:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	174745	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	186123	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	80086	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	59954	3.949	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.000%
7) Chloroethane-d5	1.564	69	45039	4.085	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.600%
11) 1,1-Dichloroethene-d2	2.101	63	84343	3.063	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.200%
20) 2-Butanone-d5	3.883	46	101786	39.588	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.180%
24) Chloroform-d	4.342	84	118163	4.244	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.800%
26) 1,2-Dichloroethane-d4	5.027	65	60694	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
32) Benzene-d6	5.043	84	235380	4.287	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
36) 1,2-Dichloropropane-d6	6.066	67	74355	4.380	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.313	98	189184	3.764	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.200%
43) trans-1,3-Dichloroprop...	7.622	79	21448	3.647	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.000%
46) 2-Hexanone-d5	8.088	63	85650	37.637	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.280%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48136	3.919	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	65457	4.735	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.800%
Target Compounds						
16) Methylene chloride	2.500	84	8013	0.397	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027360.D
Acq On : 13 Aug 2022 10:51
Operator : SY/MD
Sample : VV0813WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK203

Quant Time: Aug 13 21:50:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 21:49:38 2022
Response via : Initial Calibration

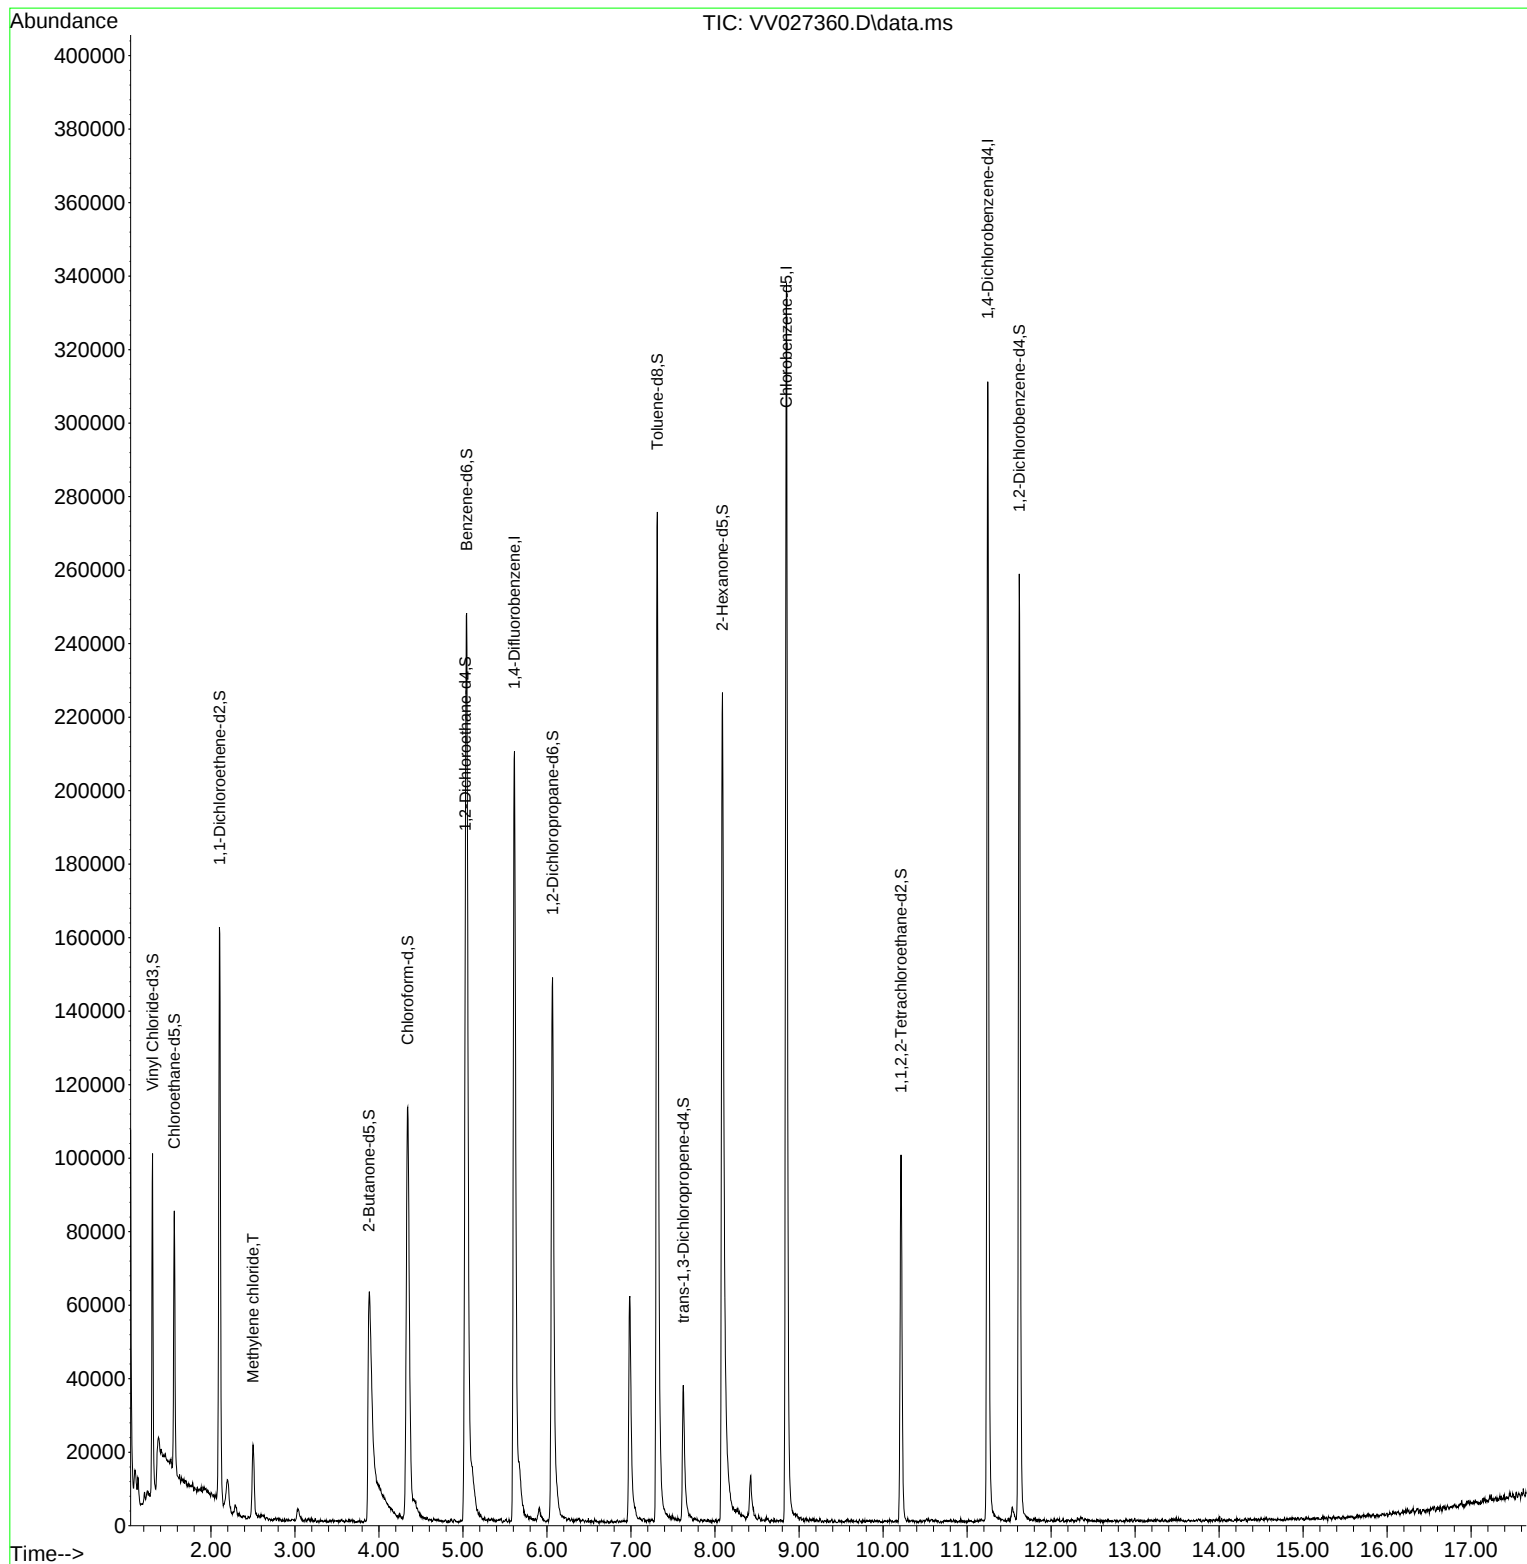

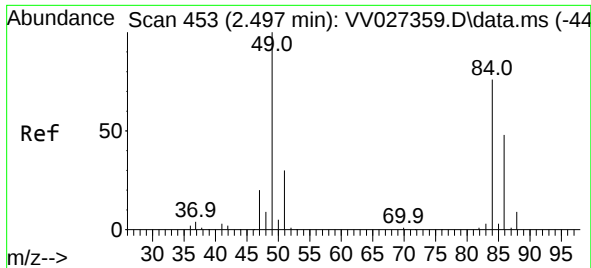

#16
Methylene chloride
Concen: 0.397 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV027360.D
Acq: 13 Aug 2022 10:51

Instrument :
MSVOA_V
ClientSampleId :
VBLK203

Tgt Ion:	84	Resp:	8013
Ion	Ratio	Lower	Upper
84	100		
86	63.5	45.1	83.9
49	123.2	91.2	169.4

