

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
 Data File : VV027368.D
 Acq On : 13 Aug 2022 14:40
 Operator : SY/MD
 Sample : VIBLK279
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK279

Quant Time: Aug 13 21:52:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 13 21:49:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	152169	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	164197	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71273	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	36384	2.752	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.000%
7) Chloroethane-d5	1.561	69	28667	2.986	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	59.800%#
11) 1,1-Dichloroethene-d2	2.101	63	46638	1.945	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	39.000%#
20) 2-Butanone-d5	3.883	46	123262	55.053	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.100%
24) Chloroform-d	4.342	84	91621	3.779	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.600%
26) 1,2-Dichloroethane-d4	5.027	65	45631	3.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.000%
32) Benzene-d6	5.047	84	142302	2.938	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	58.800%#
36) 1,2-Dichloropropane-d6	6.069	67	52447	3.502	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	70.000%
41) Toluene-d8	7.313	98	105132	2.371	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	47.400%#
43) trans-1,3-Dichloroprop...	7.625	79	12733	2.455	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	49.000%#
46) 2-Hexanone-d5	8.088	63	82118	40.904	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.800%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44183	4.078	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	45404	3.691	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	73.800%#
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	4325	0.246	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027368.D
Acq On : 13 Aug 2022 14:40
Operator : SY/MD
Sample : VIBLK279
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279


Quant Time: Aug 13 21:52:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 13 21:49:38 2022
Response via : Initial Calibration

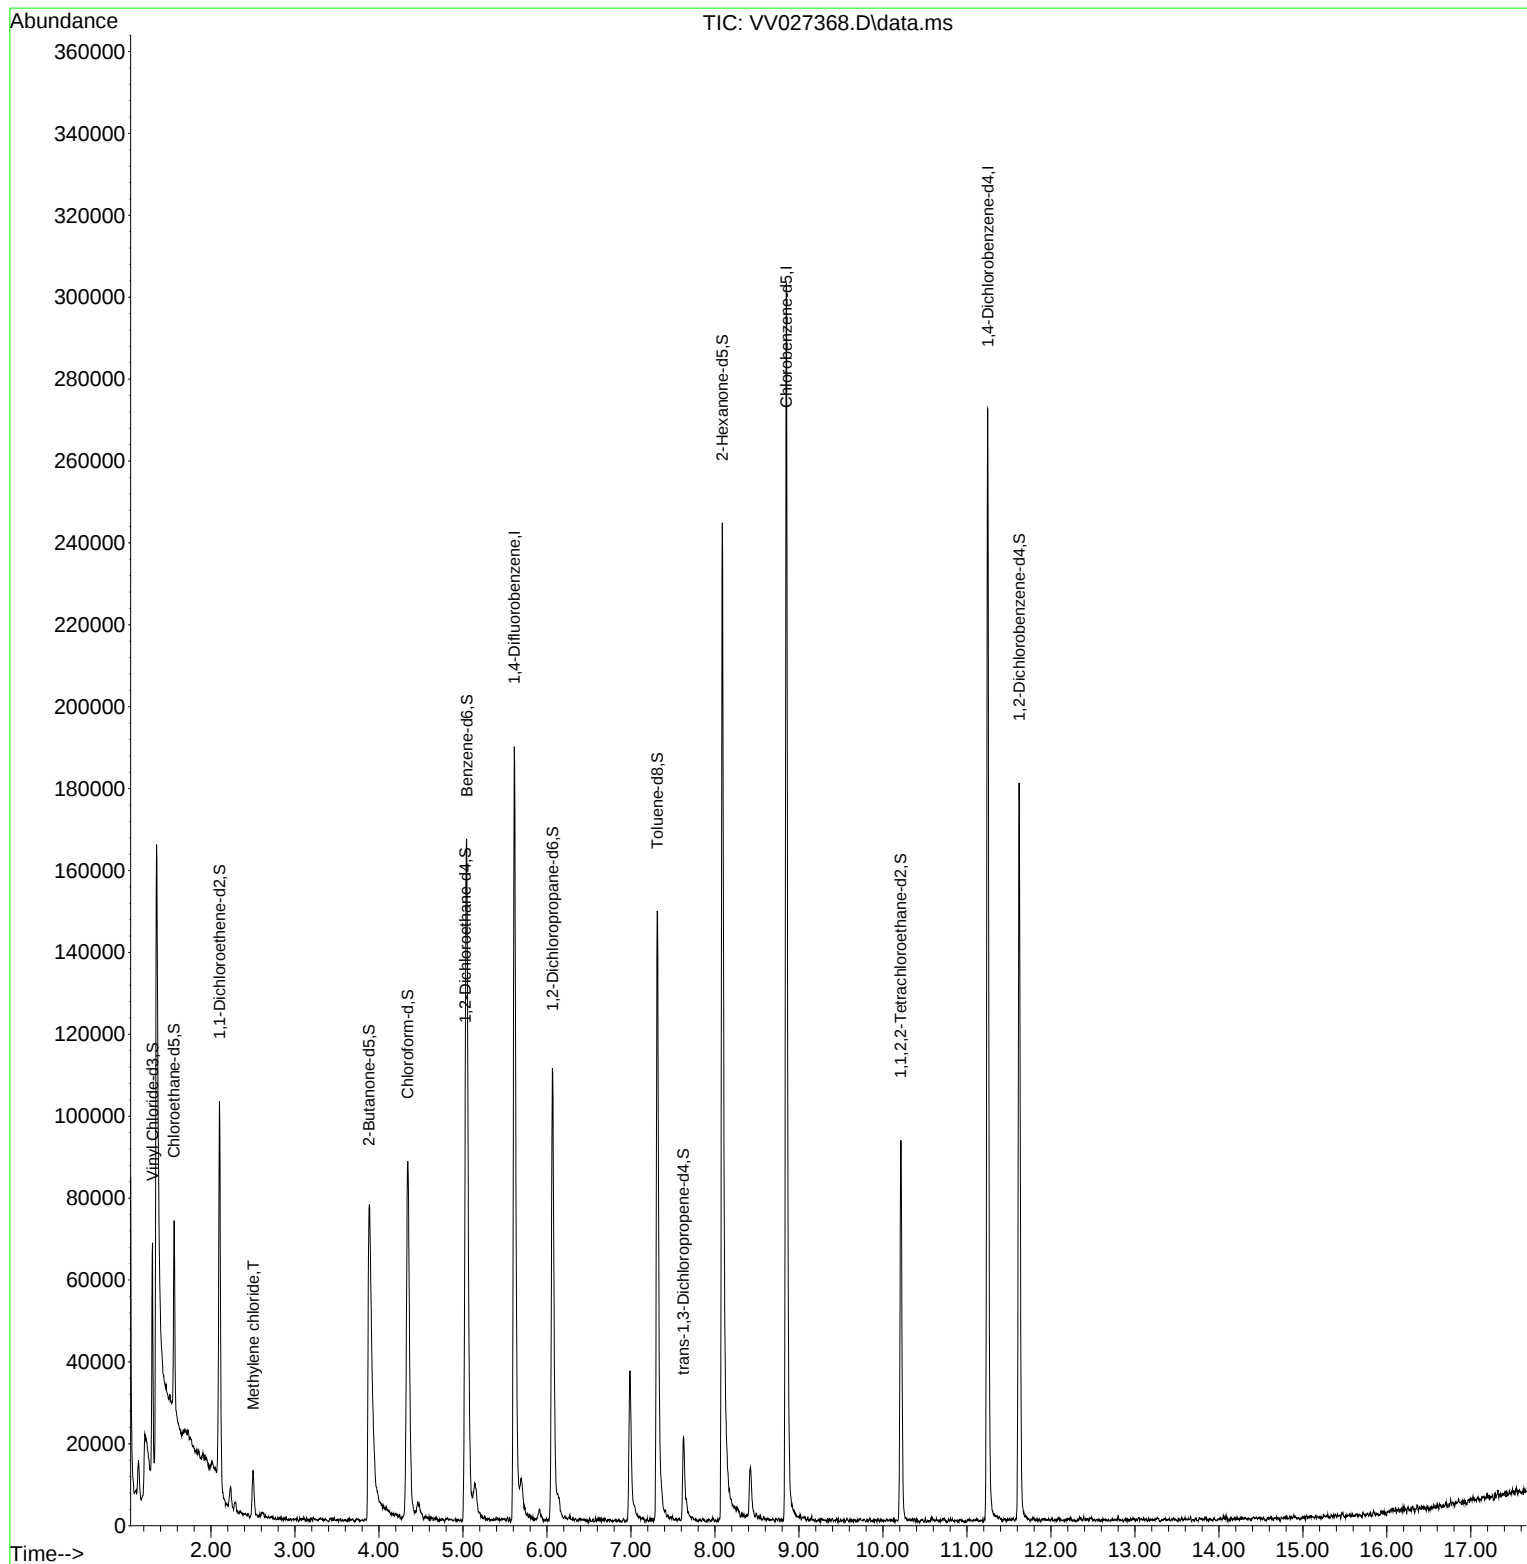

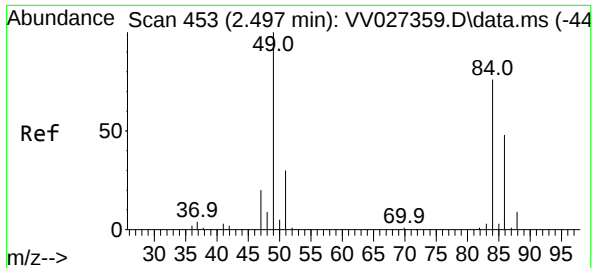

#16
Methylene chloride
Concen: 0.246 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV027368.D
Acq: 13 Aug 2022 14:40

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

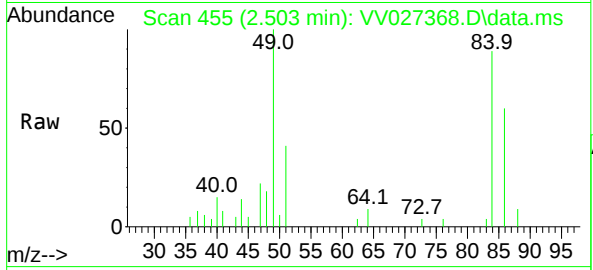

Tgt Ion:	84	Resp:	4325
Ion	Ratio	Lower	Upper
84	100		
86	67.8	45.1	83.9
49	112.1	91.2	169.4

