

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
 Data File : VV027361.D
 Acq On : 13 Aug 2022 11:39
 Operator : SY/MD
 Sample : N4161-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rBV	91179	98023	14.14%	1.840%
2	1.381	97	106	111	rBV2	7253	14015	2.02%	0.263%
3	1.564	156	163	173	rVB	74523	84353	12.17%	1.583%
4	2.101	320	330	343	rVB	168667	241513	34.84%	4.533%
5	2.195	348	359	372	rVB8	9387	24789	3.58%	0.465%
6	2.500	442	454	468	rBV	24366	41618	6.00%	0.781%
7	3.889	873	886	908	rBV3	50971	181369	26.17%	3.404%
8	4.339	1008	1026	1047	rBV	118352	305560	44.09%	5.735%
9	5.040	1226	1244	1283	rBV2	262117	693109	100.00%	13.009%
10	5.609	1410	1421	1457	rBV	197654	441135	63.65%	8.280%
11	6.063	1549	1562	1593	rBV	153666	338732	48.87%	6.358%
12	6.982	1836	1848	1868	rBV2	65167	132781	19.16%	2.492%
13	7.310	1936	1950	1979	rBV	284337	537527	77.55%	10.089%
14	7.619	2036	2046	2064	rBV2	37514	74647	10.77%	1.401%
15	8.088	2180	2192	2222	rBV	218603	521220	75.20%	9.783%
16	8.847	2415	2428	2450	rBV	314315	534058	77.05%	10.024%
17	10.214	2842	2853	2867	rBV	101471	166525	24.03%	3.126%
18	11.246	3161	3174	3193	rBV	290770	461726	66.62%	8.666%
19	11.538	3256	3265	3278	rBV10	4765	10278	1.48%	0.193%
20	11.622	3280	3291	3314	rVB	267093	424753	61.28%	7.972%




Sum of corrected areas: 5327731

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027361.D
Acq On : 13 Aug 2022 11:39
Operator : SY/MD
Sample : N4161-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

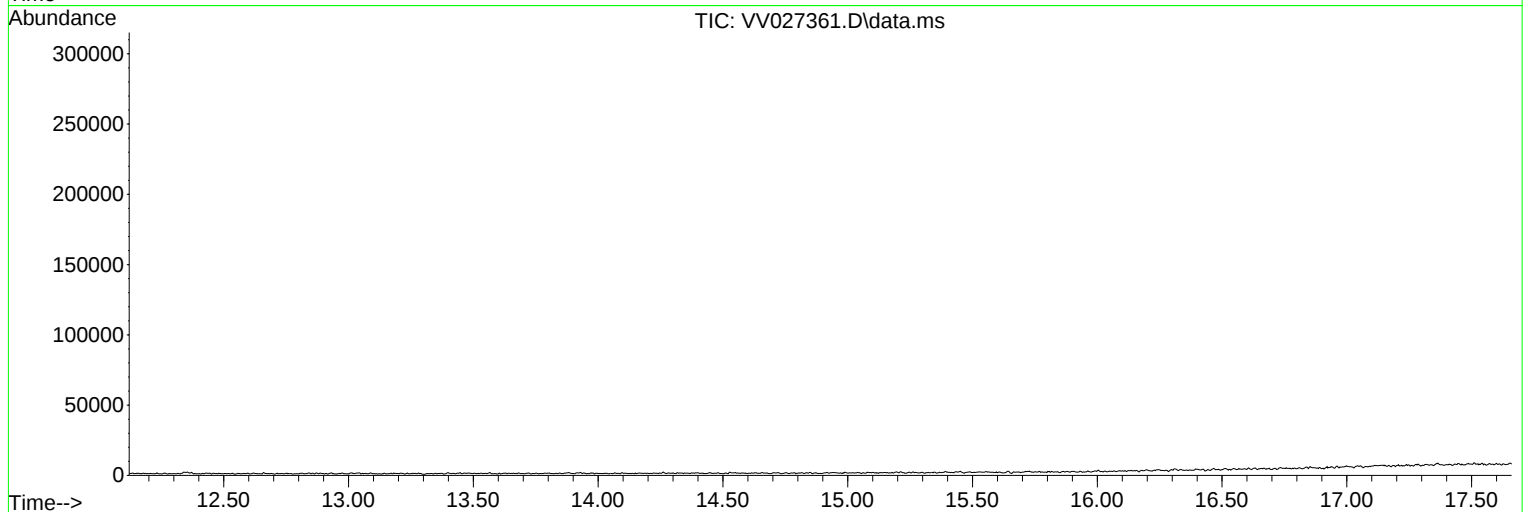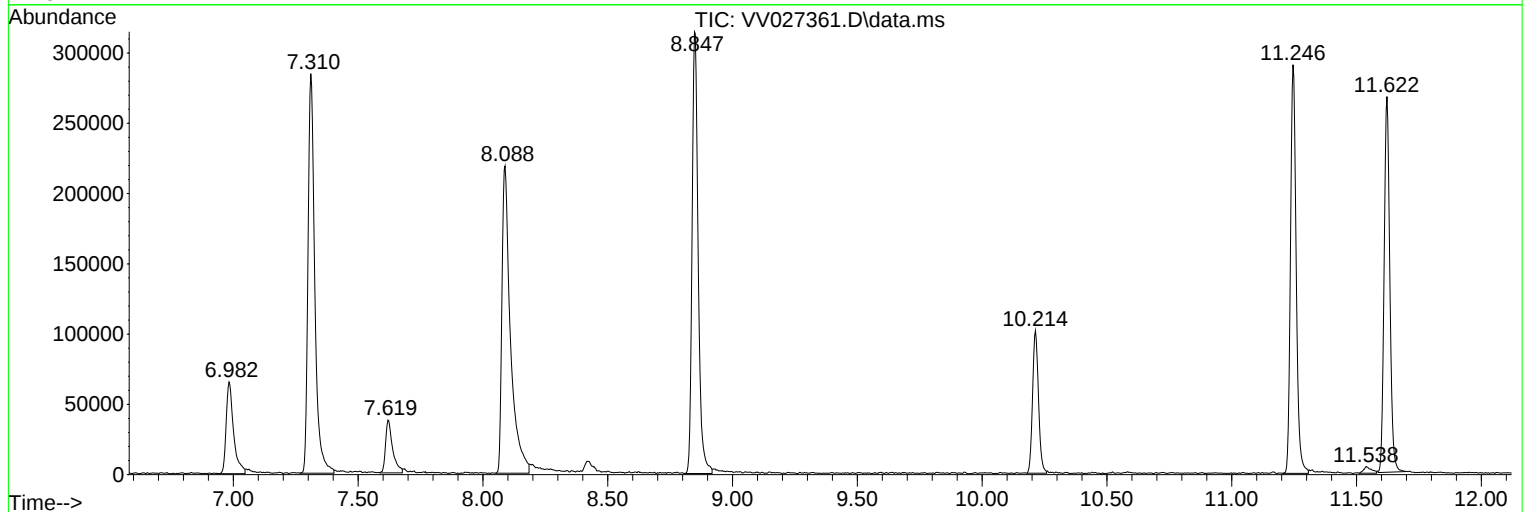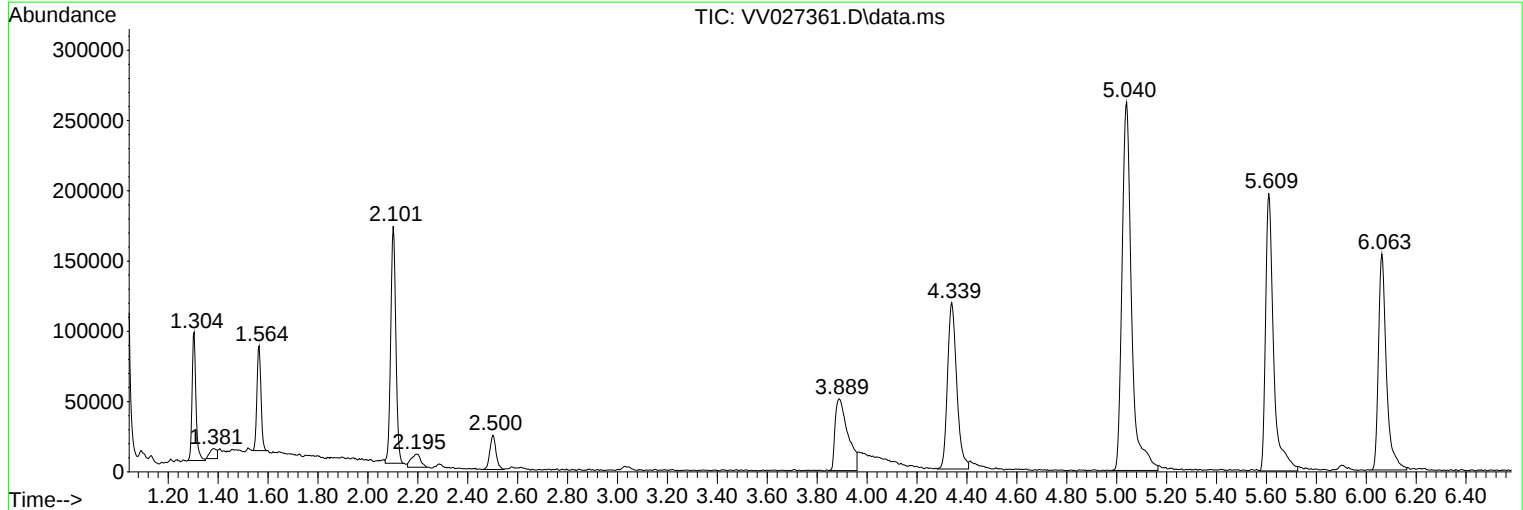

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027361.D
Acq On : 13 Aug 2022 11:39
Operator : SY/MD
Sample : N4161-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
Data File : VV027361.D
Acq On : 13 Aug 2022 11:39
Operator : SY/MD
Sample : N4161-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
