
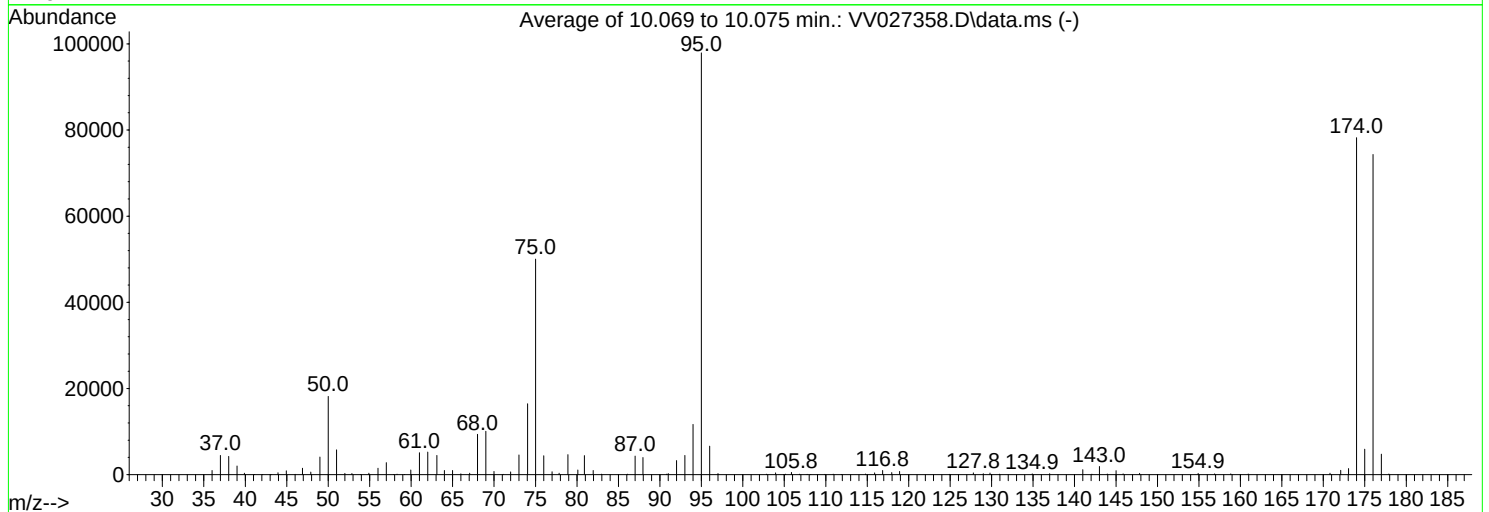


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081322\
 Data File : VV027358.D
 Acq On : 13 Aug 2022 08:32
 Operator : SY/MD
 Sample : BFB352
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB352

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Aug 13 21:49:38 2022

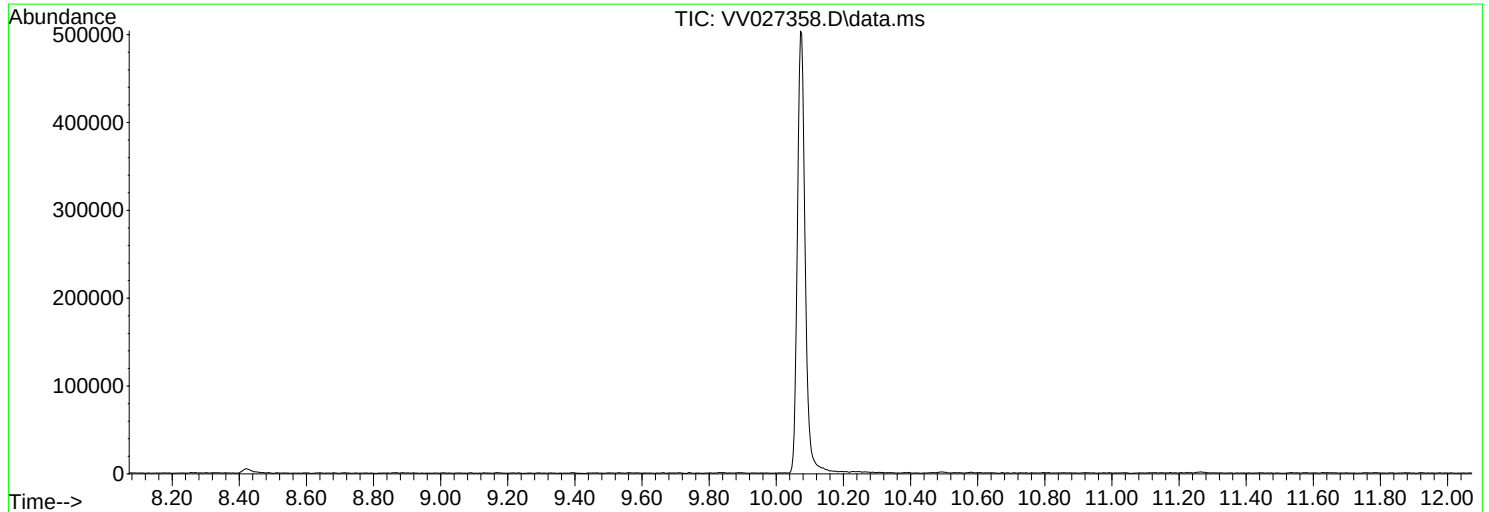

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	18179	PASS
75	95	30	80	51.1	50024	PASS
95	95	100	100	100.0	97909	PASS
96	95	5	9	6.8	6616	PASS
173	174	0.00	2	1.8	1429	PASS
174	95	50	120	79.9	78211	PASS
175	174	5	9	7.5	5904	PASS
176	174	95	105	95.0	74317	PASS
177	176	5	10	6.4	4745	PASS

Scan 2796 (10.030 min): VV027358.D\data.ms
BFB352

m/z	Abundance
40.10	389.0
43.10	110.0
44.00	460.0
47.60	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.00	908.0
37.00	4252.0
38.00	4217.0
39.00	1866.0
39.90	532.0
43.00	119.0
44.00	1010.0
44.90	800.0
46.90	1497.0
47.90	558.0
49.00	3804.0
50.00	17896.0
51.00	5584.0
52.00	280.0
52.80	272.0
54.90	324.0
56.00	1456.0
57.00	2677.0
57.90	170.0
59.20	106.0
60.00	960.0
61.00	4747.0
62.00	4928.0
63.10	4303.0
64.00	989.0
65.00	900.0
66.00	173.0
67.00	247.0
68.00	8728.0
69.00	9543.0
70.00	670.0
71.10	128.0
72.00	665.0
73.00	4227.0
74.00	15464.0
75.00	47344.0
76.00	4023.0
77.00	742.0
78.90	4334.0
80.10	1016.0
80.90	4201.0
82.00	840.0
82.90	125.0
87.00	4187.0
88.00	3948.0
90.80	392.0
92.00	3173.0
93.00	3951.0
94.00	11080.0
95.00	92200.0
96.00	6196.0
97.00	271.0
103.00	125.0
104.00	403.0
104.90	145.0
105.80	486.0
106.80	110.0
107.80	150.0
109.90	107.0
110.90	135.0
114.80	126.0
116.00	376.0
116.80	906.0
117.90	427.0
118.90	652.0
127.80	397.0
129.00	189.0
129.80	331.0
130.90	107.0
134.90	187.0
137.00	247.0
141.00	1106.0
142.10	151.0
143.00	1707.0
143.90	136.0
145.00	902.0
145.80	201.0
147.80	210.0
154.90	263.0
156.90	134.0
158.90	149.0
161.00	126.0
170.90	348.0
172.20	961.0
173.00	1309.0
174.00	72528.0
175.00	5573.0
176.00	68016.0
177.00	4737.0
177.90	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.00	979.0
37.00	4570.0
38.00	4332.0
39.00	2113.0
40.10	540.0
43.00	110.0
44.00	901.0
45.00	914.0
46.90	1567.0
47.90	585.0
49.00	4251.0
50.00	18888.0
51.00	5969.0
52.00	302.0
52.90	253.0
54.90	340.0
56.00	1591.0
57.00	2884.0
58.30	152.0
60.00	1113.0
61.00	5308.0
62.00	5431.0
63.10	4615.0
64.00	1004.0
65.00	1034.0
66.00	206.0
67.10	328.0
68.00	9606.0
69.00	10457.0
70.00	771.0
71.10	132.0
72.00	643.0
73.00	4720.0
74.10	17080.0
75.00	51864.0
76.00	4523.0
77.00	692.0
77.90	512.0
78.90	4822.0
80.10	1139.0
80.90	4549.0
81.90	1008.0
83.00	138.0
86.10	207.0
87.00	4487.0
87.90	4016.0
91.00	374.0
92.00	3391.0
93.00	4612.0
94.00	12012.0
95.00	101112.0
96.00	6895.0
97.00	273.0
102.80	137.0
104.00	393.0
105.10	166.0
105.90	558.0
106.80	112.0
107.70	110.0
109.90	104.0
110.90	142.0
114.80	148.0
115.90	445.0
116.80	997.0
118.00	516.0
118.90	789.0
124.90	104.0
127.80	428.0
129.00	211.0
129.80	372.0
130.90	135.0
134.90	181.0
137.00	217.0
141.00	1201.0
142.10	156.0
143.00	2016.0
144.00	155.0
145.00	989.0
145.90	191.0
147.90	326.0
154.90	340.0
156.90	174.0
158.80	213.0
160.90	165.0
170.80	345.0
172.10	1009.0
173.10	1502.0
174.00	80880.0
175.00	6079.0
176.00	76768.0
177.00	4930.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.00	1009.0
37.00	4607.0
38.00	4160.0
39.00	2049.0
39.90	499.0
41.10	116.0
42.10	106.0
42.90	105.0
43.90	822.0
45.00	939.0
46.00	255.0
46.90	1370.0
47.90	621.0
49.00	4191.0
50.00	17752.0
51.00	5688.0
52.00	328.0
52.90	244.0
53.90	121.0
54.90	369.0
56.00	1454.0
57.00	2837.0
58.30	145.0
59.90	1134.0
61.00	5205.0
62.00	5374.0
63.10	4428.0
64.00	933.0
65.00	982.0
66.00	195.0
67.10	384.0
68.00	9733.0
69.00	10219.0
70.00	814.0
72.00	563.0
73.00	4753.0
74.00	16848.0
75.00	50864.0
76.00	4567.0
77.00	589.0
77.80	541.0
78.90	4752.0
80.10	1107.0
80.90	4545.0
81.90	1062.0
83.00	122.0
86.10	169.0
87.00	4236.0
88.00	4018.0
91.00	388.0
92.00	3254.0
93.00	4758.0
94.00	11936.0
95.00	100416.0
96.00	6758.0
97.00	213.0
102.70	118.0
103.80	403.0
105.20	199.0
105.90	509.0
106.90	131.0
108.20	113.0
110.90	106.0
111.90	116.0
114.80	171.0
115.80	457.0
116.90	1026.0
118.00	530.0
118.90	817.0
124.90	107.0
127.80	445.0
129.00	233.0
129.80	407.0
131.00	145.0
134.90	176.0
137.00	205.0
141.00	1180.0
143.00	2019.0
144.00	163.0
145.00	945.0
145.90	174.0
147.90	381.0
150.00	126.0
154.90	334.0
156.90	211.0
158.80	244.0
161.00	163.0
170.70	331.0
172.00	1055.0
173.10	1477.0
174.00	81224.0
175.00	6060.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

176.00	78168.0
177.00	4567.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352