
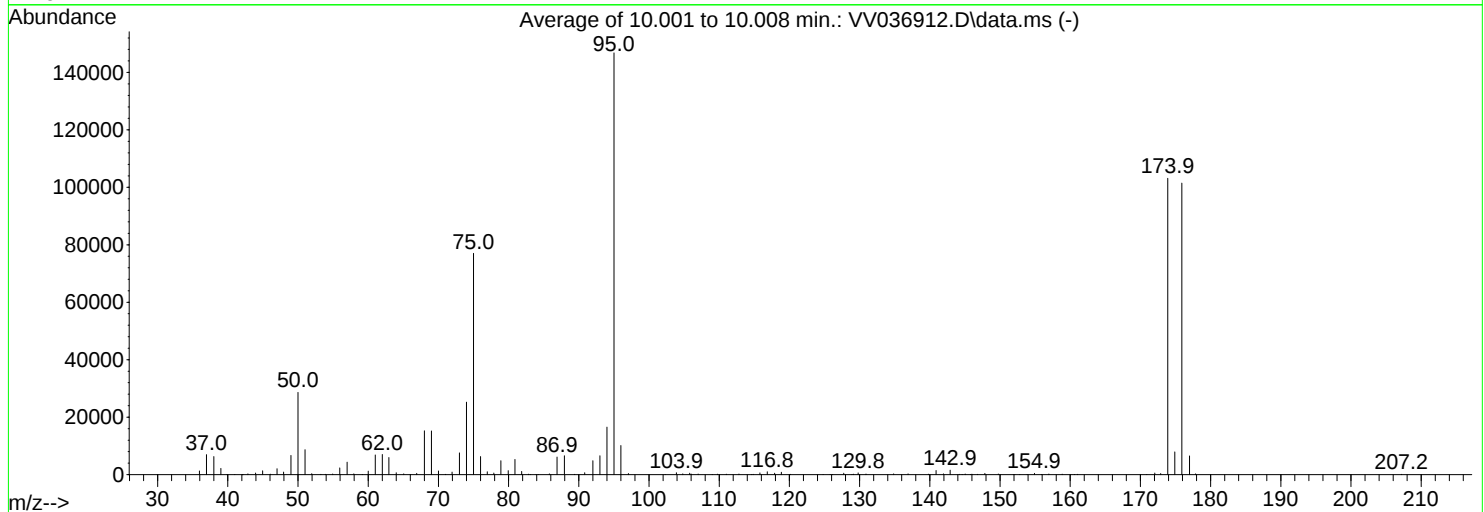


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081324\
Data File : VV036912.D
Acq On : 13 Aug 2024 08:33
Operator : SY/MD
Sample : BFB360
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB360

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Wed Aug 14 04:10:20 2024

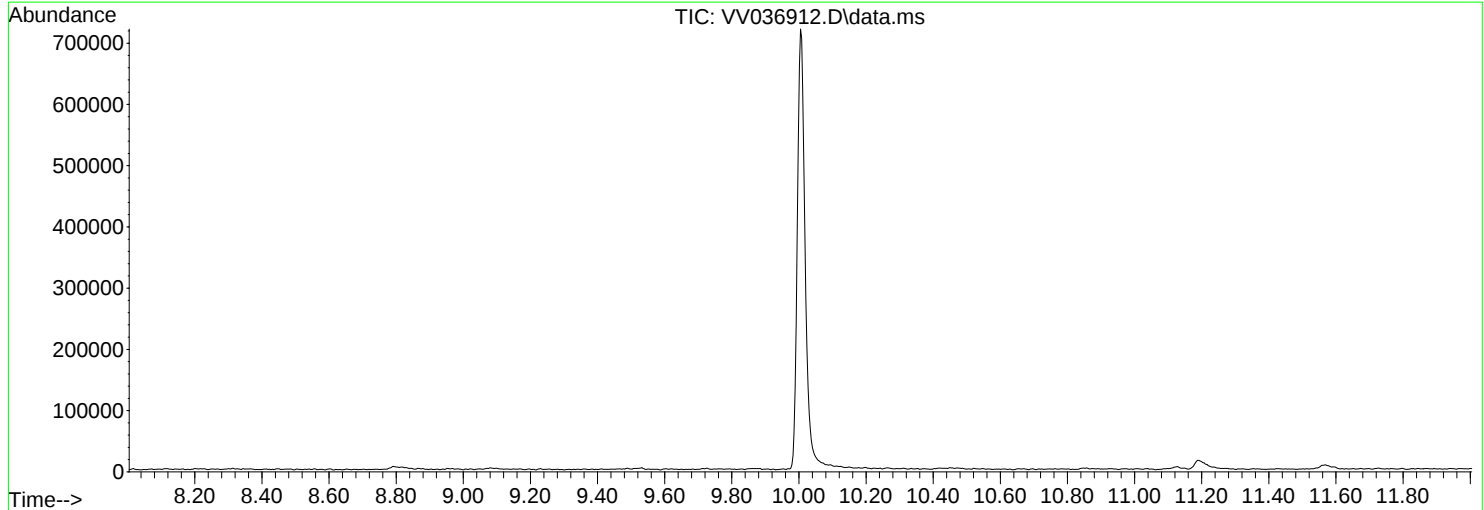

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	28632	PASS
75	95	30	80	52.5	77011	PASS
95	95	100	100	100.0	146816	PASS
96	95	5	9	6.9	10144	PASS
173	174	0.00	2	0.4	386	PASS
174	95	50	120	70.3	103160	PASS
175	174	5	9	7.7	7935	PASS
176	174	95	105	98.4	101467	PASS
177	176	5	10	6.4	6498	PASS

m/z	Abundance
35.90	132.0
36.40	159.0
36.90	108.0
38.40	115.0
39.00	206.0
39.80	409.0
41.00	200.0
42.20	167.0
43.10	180.0
43.90	1299.0
44.90	133.0
47.00	115.0
51.00	162.0
51.90	132.0
54.80	167.0
55.10	140.0
58.20	106.0
60.00	115.0
62.80	121.0
69.20	133.0
78.00	135.0
79.00	125.0
81.00	103.0
90.40	102.0
105.20	123.0
106.50	136.0
148.80	103.0
164.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	1302.0
37.00	7010.0
38.00	6406.0
39.00	2242.0
40.00	464.0
41.00	248.0
42.00	163.0
42.80	271.0
44.00	2033.0
45.00	1367.0
46.10	224.0
47.00	2108.0
47.90	903.0
49.00	6238.0
50.00	27488.0
51.00	8633.0
52.00	379.0
53.30	112.0
53.90	121.0
55.00	529.0
56.00	2286.0
57.00	4181.0
58.00	279.0
60.00	1464.0
61.00	6328.0
62.00	6757.0
63.00	5700.0
64.00	626.0
65.10	258.0
66.00	107.0
66.90	394.0
68.00	14485.0
69.00	14666.0
70.00	1157.0
71.00	119.0
71.90	975.0
73.00	7209.0
74.00	24488.0
75.00	74336.0
76.00	6202.0
76.90	1062.0
77.90	704.0
78.90	4827.0
80.00	1450.0
80.90	5294.0
81.80	996.0
82.80	140.0
83.10	142.0
84.20	104.0
85.80	281.0
86.90	5625.0
88.00	5878.0
89.40	132.0
90.90	651.0
92.00	4607.0
93.00	6645.0
94.00	16183.0
95.00	141184.0
96.00	10160.0
97.00	403.0
103.90	635.0
104.80	279.0
105.80	787.0
107.00	187.0
109.70	157.0
111.00	186.0
112.80	215.0
114.60	124.0
115.80	570.0
116.80	873.0
117.90	465.0
118.80	859.0
120.20	118.0
125.80	123.0
127.70	376.0
128.90	225.0
129.80	530.0
130.90	222.0
134.80	224.0
136.90	255.0
139.80	151.0
140.90	1243.0
142.00	301.0
142.90	1416.0
145.00	270.0
145.80	159.0
146.80	130.0
147.80	492.0
148.80	120.0
149.80	205.0
151.90	100.0
152.80	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

154.90	392.0
155.90	115.0
157.00	220.0
158.80	155.0
161.00	146.0
172.00	551.0
173.90	95128.0
174.90	7515.0
175.90	93776.0
177.00	6040.0
177.90	311.0
207.30	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	1424.0
37.00	7234.0
38.00	6518.0
39.00	2466.0
40.00	459.0
41.00	251.0
42.00	185.0
42.90	251.0
44.00	1833.0
45.00	1570.0
46.10	189.0
47.00	2318.0
47.90	981.0
49.00	6952.0
50.00	29688.0
51.00	9205.0
52.00	488.0
53.20	151.0
53.90	128.0
55.00	541.0
56.00	2412.0
57.00	4487.0
57.90	264.0
59.20	120.0
60.00	1384.0
61.00	7143.0
62.00	7330.0
63.00	6348.0
64.00	707.0
65.10	299.0
66.00	115.0
66.90	443.0
68.00	15781.0
69.00	15916.0
70.00	1344.0
71.00	119.0
71.90	933.0
73.00	7888.0
74.00	25968.0
75.00	79888.0
76.00	6622.0
76.90	1024.0
77.90	736.0
78.90	5131.0
79.90	1466.0
80.90	5675.0
81.90	1186.0
82.90	184.0
83.90	118.0
85.80	308.0
86.90	6311.0
87.90	6809.0
89.40	134.0
90.90	669.0
92.00	5133.0
93.00	6888.0
94.00	16792.0
95.00	152576.0
96.00	10534.0
97.00	384.0
102.30	101.0
103.90	693.0
104.80	320.0
105.80	739.0
107.00	240.0
109.70	169.0
111.00	226.0
112.80	205.0
114.80	132.0
115.80	628.0
116.80	1054.0
117.90	477.0
118.80	861.0
120.20	111.0
126.10	114.0
127.80	563.0
129.10	274.0
129.80	623.0
130.90	246.0
134.80	286.0
136.90	278.0
139.80	175.0
140.90	1494.0
142.00	267.0
142.90	1569.0
144.20	130.0
144.60	111.0
145.10	199.0
146.00	199.0
146.80	126.0
147.90	454.0
148.70	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

149.80	196.0
152.80	101.0
153.80	111.0
154.90	479.0
157.00	205.0
158.90	183.0
161.10	134.0
170.90	103.0
172.00	616.0
173.90	106544.0
174.90	8288.0
175.90	105416.0
177.00	6712.0
177.90	297.0
207.20	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	1464.0
37.00	6902.0
38.00	5966.0
39.00	2502.0
40.00	410.0
41.00	265.0
42.00	190.0
42.90	282.0
44.00	1727.0
45.00	1548.0
45.90	140.0
47.00	2175.0
48.00	827.0
49.00	6902.0
50.00	28720.0
51.00	8706.0
52.00	540.0
53.30	155.0
53.90	148.0
55.00	482.0
55.90	2301.0
57.00	4345.0
57.90	243.0
59.10	114.0
60.00	1165.0
61.00	7138.0
62.00	6992.0
63.00	6132.0
64.00	683.0
65.00	284.0
66.90	465.0
68.00	15614.0
69.00	15513.0
70.00	1338.0
71.00	106.0
72.00	853.0
73.00	7626.0
74.00	25264.0
75.00	76808.0
76.00	6118.0
77.00	886.0
77.90	605.0
78.90	4950.0
79.90	1318.0
80.90	5303.0
81.90	1138.0
82.90	199.0
83.90	125.0
85.80	253.0
86.90	6438.0
87.90	7074.0
89.40	118.0
90.80	654.0
92.00	4896.0
93.00	6241.0
94.00	16712.0
95.00	146688.0
96.00	9738.0
97.10	332.0
103.90	779.0
104.80	293.0
106.00	666.0
107.00	280.0
109.00	102.0
109.80	145.0
111.00	172.0
112.80	197.0
114.90	187.0
115.80	610.0
116.90	1071.0
117.90	524.0
118.90	817.0
120.10	115.0
124.80	107.0
126.20	129.0
127.80	639.0
129.10	314.0
129.80	679.0
130.90	224.0
134.90	329.0
136.90	277.0
139.80	161.0
140.90	1553.0
141.90	208.0
142.90	1669.0
144.20	153.0
144.60	139.0
145.10	175.0
146.00	238.0
146.80	110.0
147.80	381.0
149.70	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

152.10	114.0
153.90	121.0
154.90	485.0
156.90	176.0
158.90	200.0
160.60	115.0
172.10	578.0
172.90	1159.0
173.90	107808.0
174.90	8001.0
175.90	105208.0
177.00	6741.0
177.80	262.0
207.10	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360