

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036937.D
 Acq On : 15 Aug 2024 09:20
 Operator : SY/MD
 Sample : VV0815MBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 16 02:15:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 16 02:14:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	707396	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	668243	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	324569	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	271415	48.038	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	96.080%		
7) Chloroethane-d5	1.532	69	219902	49.353	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.700%		
11) 1,1-Dichloroethene-d2	2.060	65	117335	48.549	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.100%		
21) 2-Butanone-d5	3.796	46	238195	79.568	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.570%		
24) Chloroform-d	4.243	84	480917	47.431	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.860%		
26) 1,2-Dichloroethane-d4	4.937	65	305638	46.884	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.760%		
32) Benzene-d6	4.953	84	1001098	49.600	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.200%		
36) 1,2-Dichloropropane-d6	5.985	67	318506	48.915	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.820%		
41) Toluene-d8	7.239	98	891334	48.143	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.280%		
43) trans-1,3-Dichloroprop...	7.551	79	137198	40.486	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.980%		
47) 2-Hexanone-d5	8.024	63	131103	70.025	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.030%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	329308	44.046	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.100%		
66) 1,2-Dichlorobenzene-d4	11.554	152	319698	48.338	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.680%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3665	0.783	ug/L	# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036937.D
Acq On : 15 Aug 2024 09:20
Operator : SY/MD
Sample : VV0815MBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 16 02:15:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 16 02:14:55 2024
Response via : Initial Calibration

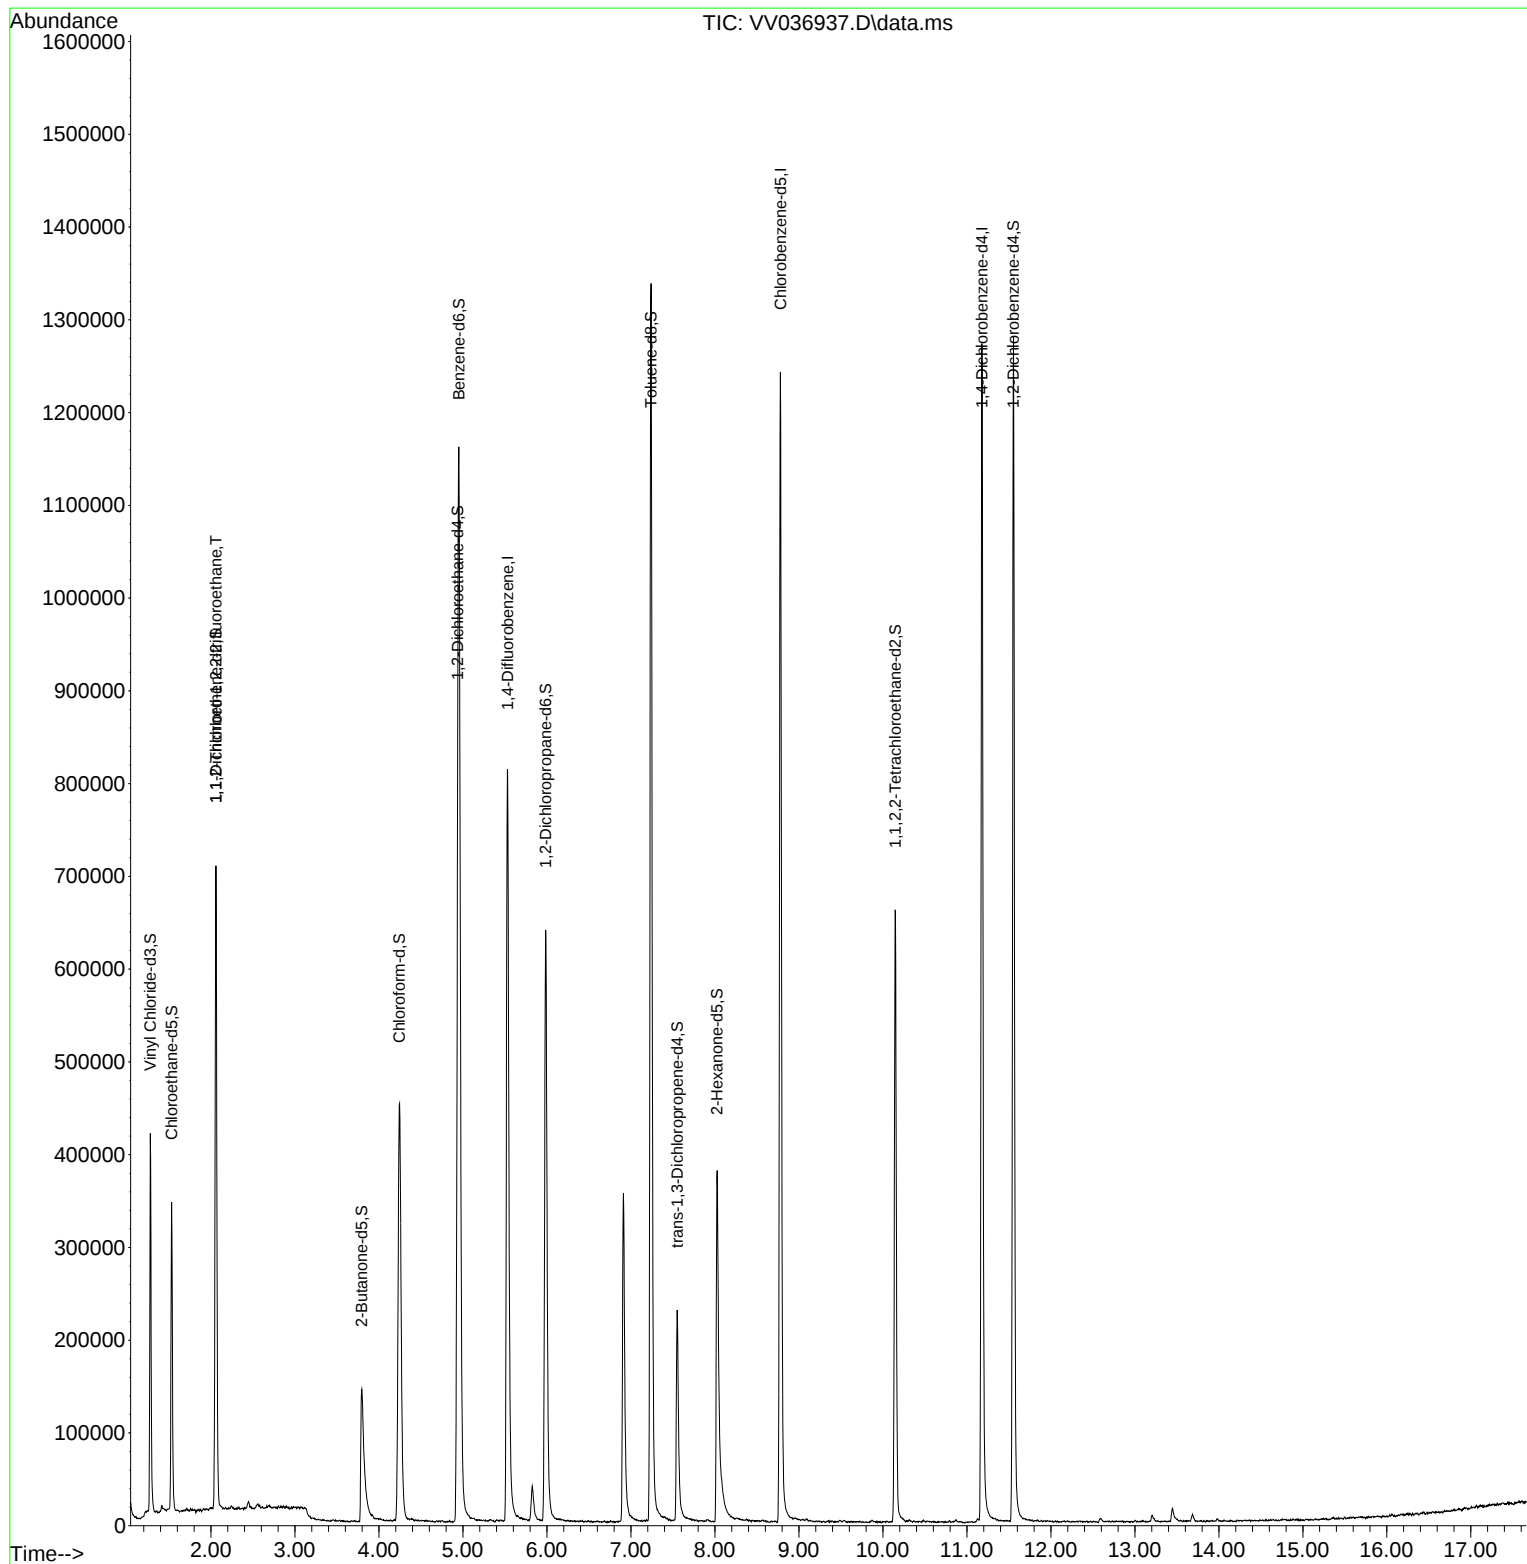

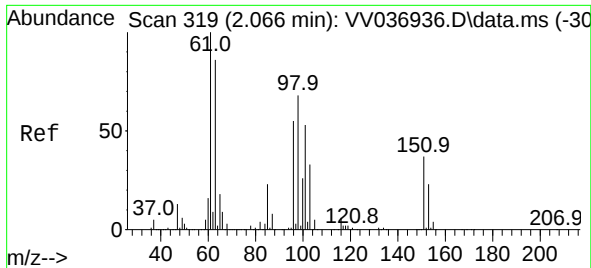

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.783 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV036937.D
 Acq: 15 Aug 2024 09:20

Instrument :
 MSVOA_V
 ClientSampleId :

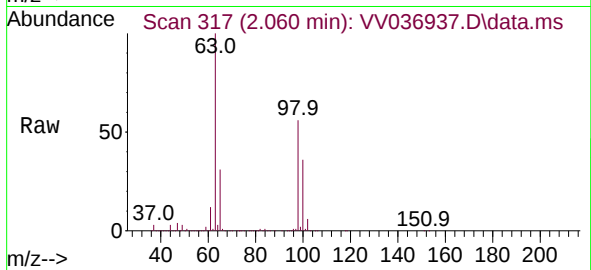

Tgt Ion:	101	Resp:	3665
Ion Ratio	Lower	Upper	
101	100		
85	3.3	34.6	51.8#
151	1.8	55.9	83.9#

