

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036939.D
 Acq On : 15 Aug 2024 14:58
 Operator : SY/MD
 Sample : P3589-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	91	rVB	413060	450747	15.71%	2.165%
2	1.532	145	153	165	rBV	333522	384011	13.39%	1.845%
3	2.056	306	316	331	rBV	698170	1010410	35.22%	4.854%
4	3.368	722	724	727	rBV4	1628	989	0.03%	0.005%
5	3.461	746	753	755	rBV7	1632	1936	0.07%	0.009%
6	3.551	775	781	782	rBV4	1369	1209	0.04%	0.006%
7	3.590	790	793	795	rBV3	1399	874	0.03%	0.004%
8	3.706	825	829	831	rVB4	1157	771	0.03%	0.004%
9	3.793	844	856	891	rBV	149931	426174	14.86%	2.047%
10	4.239	978	995	1029	rBV2	478951	1450822	50.57%	6.970%
11	4.526	1081	1084	1086	rBV3	1157	978	0.03%	0.005%
12	4.596	1102	1106	1109	rBV6	993	801	0.03%	0.004%
13	4.638	1115	1119	1121	rBV4	1127	801	0.03%	0.004%
14	4.773	1156	1161	1163	rBV5	1731	1056	0.04%	0.005%
15	4.873	1189	1192	1196	rVB4	1220	1120	0.04%	0.005%
16	4.944	1196	1214	1250	rBV2	1131900	2868714	100.00%	13.782%
17	5.294	1319	1323	1325	rBV4	1469	980	0.03%	0.005%
18	5.313	1325	1329	1332	rBV4	1474	1322	0.05%	0.006%
19	5.439	1364	1368	1371	rBV6	1179	897	0.03%	0.004%
20	5.526	1384	1395	1429	rBV	747842	1527730	53.25%	7.340%
21	5.818	1475	1486	1510	rVB3	43195	100680	3.51%	0.484%
22	5.982	1523	1537	1564	rBV	622313	1289793	44.96%	6.196%
23	6.339	1643	1648	1651	rBV6	1176	1147	0.04%	0.006%
24	6.355	1651	1653	1657	rBV5	1281	931	0.03%	0.004%
25	6.432	1665	1677	1695	rBV	29154	62698	2.19%	0.301%
26	6.735	1768	1771	1775	rBV5	1505	1266	0.04%	0.006%
27	6.844	1802	1805	1808	rBV4	1736	1430	0.05%	0.007%
28	6.908	1812	1825	1850	rBV	353323	669250	23.33%	3.215%
29	7.162	1901	1904	1905	rBV3	1279	739	0.03%	0.004%
30	7.236	1915	1927	1952	rBV	1276557	2277097	79.38%	10.940%
31	7.548	2014	2024	2055	rBV	231328	426287	14.86%	2.048%
32	7.760	2085	2090	2091	rBV5	1263	1172	0.04%	0.006%
33	7.873	2123	2125	2127	rVB3	1692	780	0.03%	0.004%
34	8.024	2161	2172	2210	rBV2	396996	885128	30.85%	4.252%
35	8.532	2328	2330	2333	rVV4	2209	1280	0.04%	0.006%
36	8.551	2333	2336	2341	rVB6	1914	1792	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036939.D
 Acq On : 15 Aug 2024 14:58
 Operator : SY/MD
 Sample : P3589-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.625	2355	2359	2362	rBV5	1090	689	0.02%	0.003%
38	8.725	2384	2390	2391	rBV5	1075	897	0.03%	0.004%
39	8.779	2395	2407	2435	rBV	1119395	1872411	65.27%	8.995%
40	8.950	2457	2460	2462	rBV3	2387	1607	0.06%	0.008%
41	9.204	2534	2539	2541	rBV5	1171	967	0.03%	0.005%
42	9.239	2546	2550	2555	rVB7	1376	1232	0.04%	0.006%
43	9.320	2573	2575	2579	rVV5	1087	848	0.03%	0.004%
44	9.480	2613	2625	2628	rBV5	6332	9195	0.32%	0.044%
45	9.522	2633	2638	2641	rVV5	2356	2811	0.10%	0.014%
46	9.603	2658	2663	2665	rBV6	1389	1207	0.04%	0.006%
47	9.815	2725	2729	2731	rBV5	928	738	0.03%	0.004%
48	9.863	2741	2744	2747	rBV5	1330	1102	0.04%	0.005%
49	9.924	2759	2763	2767	rVB6	2048	1759	0.06%	0.008%
50	9.950	2767	2771	2774	rBV6	1453	1083	0.04%	0.005%
51	10.011	2789	2790	2797	rVB7	1862	1410	0.05%	0.007%
52	10.043	2797	2800	2804	rBV5	1721	1501	0.05%	0.007%
53	10.146	2819	2832	2853	rBV	652763	1046801	36.49%	5.029%
54	10.384	2903	2906	2907	rBV3	1480	860	0.03%	0.004%
55	10.403	2909	2912	2915	rVV5	1709	1250	0.04%	0.006%
56	10.422	2915	2918	2922	rVB6	1396	1054	0.04%	0.005%
57	10.467	2929	2932	2934	rBV3	1903	1178	0.04%	0.006%
58	10.522	2946	2949	2954	rVB6	1575	1415	0.05%	0.007%
59	10.548	2954	2957	2959	rBV4	1023	785	0.03%	0.004%
60	10.567	2961	2963	2966	rVB4	2064	1280	0.04%	0.006%
61	10.603	2972	2974	2979	rBV6	1141	710	0.02%	0.003%
62	10.664	2991	2993	2994	rBV2	1599	750	0.03%	0.004%
63	10.722	3009	3011	3014	rVB3	1437	748	0.03%	0.004%
64	10.866	3046	3056	3063	rBV3	4052	8628	0.30%	0.041%
65	11.062	3113	3117	3119	rBV4	1184	910	0.03%	0.004%
66	11.098	3124	3128	3131	rBV5	1256	840	0.03%	0.004%
67	11.123	3131	3136	3138	rBV5	2897	2962	0.10%	0.014%
68	11.178	3143	3153	3186	rBV	1184210	1875615	65.38%	9.011%
69	11.394	3218	3220	3223	rBV4	1221	851	0.03%	0.004%
70	11.474	3243	3245	3248	rVB3	1460	709	0.02%	0.003%
71	11.554	3257	3270	3298	rBV	1237590	2002805	69.82%	9.622%
72	11.950	3390	3393	3397	rBV3	1623	1482	0.05%	0.007%
73	11.992	3401	3406	3413	rBV8	1586	2140	0.07%	0.010%
74	12.191	3466	3468	3471	rBV4	1226	777	0.03%	0.004%
75	12.313	3501	3506	3507	rBV3	1163	988	0.03%	0.005%
76	12.525	3568	3572	3574	rBV6	1209	772	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036939.D
 Acq On : 15 Aug 2024 14:58
 Operator : SY/MD
 Sample : P3589-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	12.596	3586	3594	3599	rBV10	2423	3628	0.13%	0.017%
78	12.683	3618	3621	3623	rBV4	1147	722	0.03%	0.003%
79	12.721	3631	3633	3637	rVB5	1809	1052	0.04%	0.005%
80	12.757	3642	3644	3648	rVB5	1464	1032	0.04%	0.005%
81	12.783	3648	3652	3655	rBV5	1449	1120	0.04%	0.005%
82	12.811	3658	3661	3665	rBV4	1245	1300	0.05%	0.006%
83	13.149	3764	3766	3769	rBV3	1250	937	0.03%	0.005%
84	13.207	3774	3784	3795	rBV6	14419	27850	0.97%	0.134%
85	13.300	3810	3813	3815	rBV4	1307	761	0.03%	0.004%
86	13.374	3832	3836	3847	rVB8	6531	8717	0.30%	0.042%
87	13.448	3847	3859	3869	rBV2	19433	39310	1.37%	0.189%
88	13.538	3885	3887	3889	rVB3	1684	722	0.03%	0.003%
89	13.622	3911	3913	3916	rVV4	1011	676	0.02%	0.003%
90	13.686	3925	3933	3939	rBV4	4182	6308	0.22%	0.030%
91	13.943	4010	4013	4014	rBV2	1451	702	0.02%	0.003%
92	13.969	4018	4021	4022	rBV3	1486	854	0.03%	0.004%
93	14.175	4082	4085	4089	rBV6	1211	918	0.03%	0.004%
94	14.374	4144	4147	4150	rBV4	1576	868	0.03%	0.004%
95	14.413	4157	4159	4161	rBV3	1230	773	0.03%	0.004%
96	14.451	4168	4171	4173	rBV4	1110	880	0.03%	0.004%
97	14.721	4248	4255	4259	rBV9	2031	2808	0.10%	0.013%
98	14.834	4288	4290	4293	rBV4	1293	902	0.03%	0.004%
99	15.123	4376	4380	4384	rBV7	1414	1682	0.06%	0.008%
100	15.454	4481	4483	4484	rBV2	2043	921	0.03%	0.004%




Sum of corrected areas: 20815022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036939.D
Acq On : 15 Aug 2024 14:58
Operator : SY/MD
Sample : P3589-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

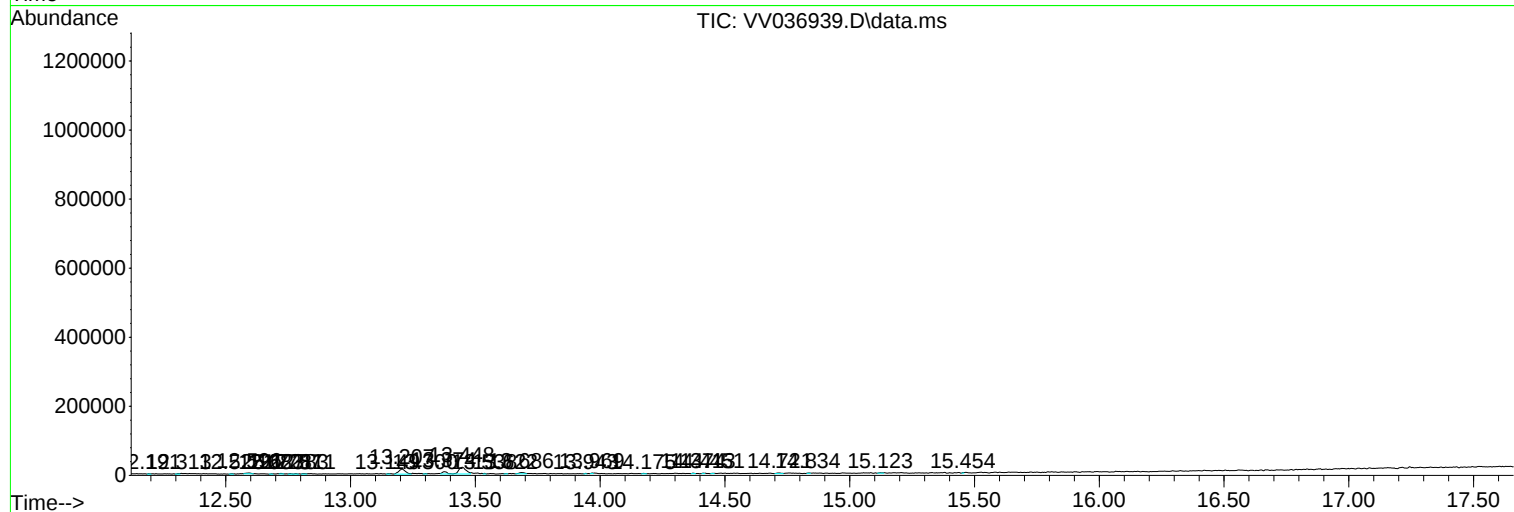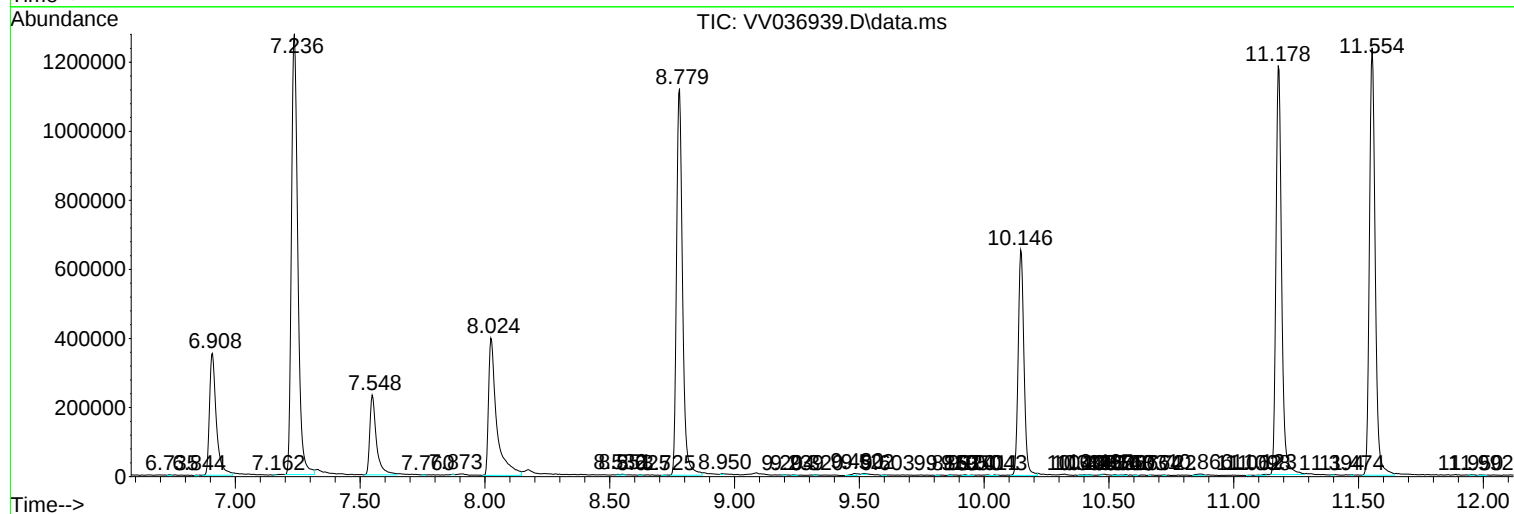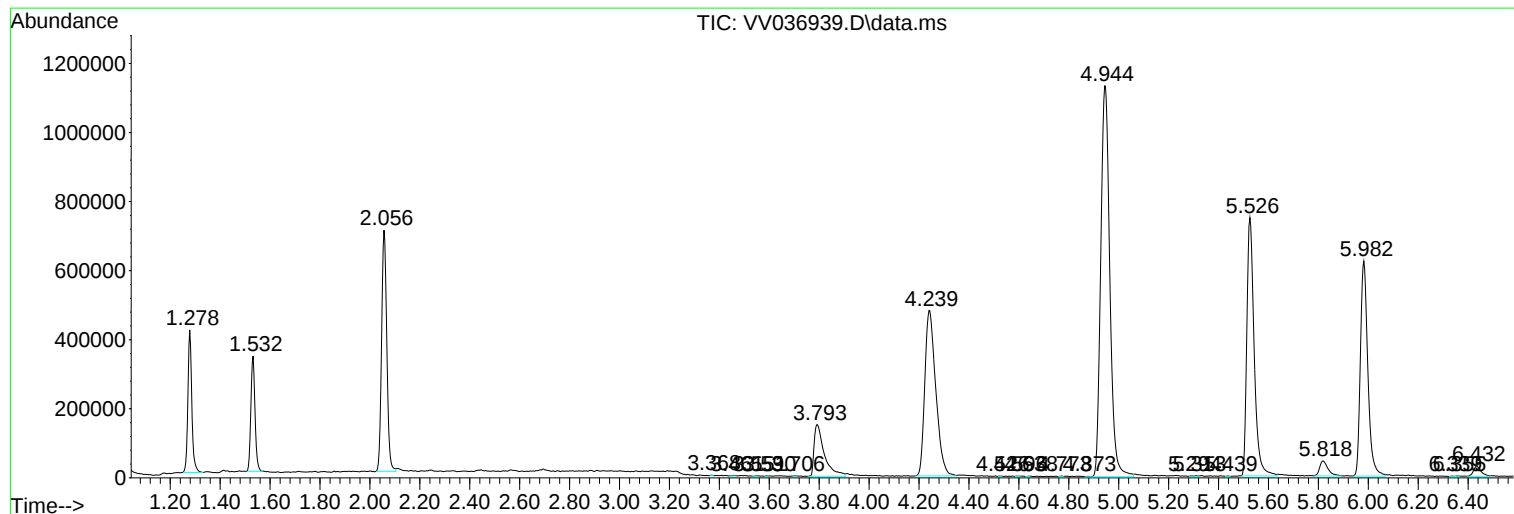

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036939.D
Acq On : 15 Aug 2024 14:58
Operator : SY/MD
Sample : P3589-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036939.D
Acq On : 15 Aug 2024 14:58
Operator : SY/MD
Sample : P3589-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc