

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036940.D
 Acq On : 15 Aug 2024 15:20
 Operator : SY/MD
 Sample : P3603-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rVB	388646	412986	15.29%	2.086%
2	1.532	145	153	167	rVB	304701	366778	13.57%	1.852%
3	2.060	307	317	332	rBV	634343	909266	33.65%	4.592%
4	3.458	748	752	754	rBV4	1545	1235	0.05%	0.006%
5	3.616	798	801	805	rVB5	1450	998	0.04%	0.005%
6	3.799	849	858	890	rBV	151032	418938	15.51%	2.116%
7	4.243	979	996	1032	rBV	422225	1075834	39.82%	5.433%
8	4.449	1056	1060	1065	rVB6	1857	2089	0.08%	0.011%
9	4.474	1065	1068	1069	rBV3	1999	1088	0.04%	0.005%
10	4.645	1118	1121	1123	rBV4	1306	996	0.04%	0.005%
11	4.683	1129	1133	1138	rVB6	1258	1384	0.05%	0.007%
12	4.712	1138	1142	1143	rBV4	1995	1268	0.05%	0.006%
13	4.732	1146	1148	1152	rVV4	1088	778	0.03%	0.004%
14	4.863	1185	1189	1193	rBV6	1565	1589	0.06%	0.008%
15	4.950	1199	1216	1245	rBV2	1083980	2701872	100.00%	13.645%
16	5.381	1346	1350	1351	rBV4	1178	885	0.03%	0.004%
17	5.423	1360	1363	1368	rBV8	1275	1249	0.05%	0.006%
18	5.529	1385	1396	1431	rBV	742321	1533388	56.75%	7.744%
19	5.825	1476	1488	1512	rBV6	31683	79020	2.92%	0.399%
20	5.986	1524	1538	1564	rBV	592464	1226187	45.38%	6.192%
21	6.281	1628	1630	1633	rVB4	1354	751	0.03%	0.004%
22	6.317	1636	1641	1646	rBV8	940	937	0.03%	0.005%
23	6.365	1654	1656	1661	rVB6	1653	894	0.03%	0.005%
24	6.449	1673	1682	1698	rVB6	6408	13536	0.50%	0.068%
25	6.635	1737	1740	1744	rVB5	1404	868	0.03%	0.004%
26	6.690	1753	1757	1759	rBV3	1508	1049	0.04%	0.005%
27	6.728	1767	1769	1771	rVV3	1799	811	0.03%	0.004%
28	6.741	1771	1773	1777	rVB4	1483	864	0.03%	0.004%
29	6.912	1814	1826	1854	rBV	327085	627591	23.23%	3.169%
30	7.159	1898	1903	1906	rBV5	1845	1798	0.07%	0.009%
31	7.182	1906	1910	1911	rBV3	1428	1089	0.04%	0.005%
32	7.239	1916	1928	1954	rBV	1234216	2174308	80.47%	10.980%
33	7.551	2015	2025	2049	rBV	215424	396209	14.66%	2.001%
34	7.767	2089	2092	2095	rBV5	1356	891	0.03%	0.004%
35	7.863	2118	2122	2124	rBV6	1493	1168	0.04%	0.006%
36	7.905	2124	2135	2155	rVV2	72099	133568	4.94%	0.675%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036940.D
 Acq On : 15 Aug 2024 15:20
 Operator : SY/MD
 Sample : P3603-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	8.027	2164	2173	2212	rBV2	402860	881555	32.63%	4.452%
38	8.545	2328	2334	2336	rBV6	1947	1751	0.06%	0.009%
39	8.609	2351	2354	2360	rVB8	1687	1880	0.07%	0.009%
40	8.641	2362	2364	2371	rVB9	1943	1473	0.05%	0.007%
41	8.699	2380	2382	2387	rVB5	1246	818	0.03%	0.004%
42	8.728	2387	2391	2395	rBV6	1653	1945	0.07%	0.010%
43	8.780	2395	2407	2438	rBV	1141130	1878811	69.54%	9.488%
44	9.024	2480	2483	2485	rBV4	1657	1036	0.04%	0.005%
45	9.317	2572	2574	2579	rVB5	1869	1075	0.04%	0.005%
46	9.387	2590	2596	2598	rBV6	1695	1442	0.05%	0.007%
47	9.436	2607	2611	2614	rVB5	908	826	0.03%	0.004%
48	9.484	2619	2626	2629	rBV6	3301	4056	0.15%	0.020%
49	9.535	2640	2642	2646	rVB4	1409	821	0.03%	0.004%
50	9.612	2664	2666	2667	rBV2	1767	751	0.03%	0.004%
51	9.670	2673	2684	2693	rBV2	6537	12938	0.48%	0.065%
52	9.728	2698	2702	2703	rBV3	1328	898	0.03%	0.005%
53	9.805	2723	2726	2728	rVB3	1813	935	0.03%	0.005%
54	9.837	2732	2736	2738	rBV4	1374	829	0.03%	0.004%
55	9.870	2741	2746	2749	rBV5	1146	1076	0.04%	0.005%
56	9.950	2766	2771	2772	rBV5	1493	1063	0.04%	0.005%
57	10.027	2791	2795	2797	rBV4	1166	1058	0.04%	0.005%
58	10.149	2820	2833	2853	rBV	663480	1072288	39.69%	5.415%
59	10.320	2882	2886	2892	rVB6	2513	2684	0.10%	0.014%
60	10.397	2905	2910	2912	rBV5	1523	994	0.04%	0.005%
61	10.452	2923	2927	2931	rBV6	1164	1028	0.04%	0.005%
62	10.484	2932	2937	2941	rBV5	1803	1879	0.07%	0.009%
63	10.526	2947	2950	2952	rBV4	1231	846	0.03%	0.004%
64	10.609	2973	2976	2981	rVB7	968	767	0.03%	0.004%
65	10.651	2986	2989	2995	rVB7	1544	1506	0.06%	0.008%
66	10.683	2995	2999	3001	rBV3	1161	832	0.03%	0.004%
67	11.130	3135	3138	3141	rVB5	1136	806	0.03%	0.004%
68	11.181	3143	3154	3186	rBV	1184583	1871349	69.26%	9.450%
69	11.554	3258	3270	3294	rBV	1192466	1905272	70.52%	9.622%
70	11.873	3367	3369	3373	rVB4	1146	787	0.03%	0.004%
71	11.988	3399	3405	3406	rBV5	1297	1216	0.05%	0.006%
72	12.101	3434	3440	3441	rBV5	997	864	0.03%	0.004%
73	12.226	3477	3479	3483	rVB5	1349	827	0.03%	0.004%
74	12.249	3483	3486	3488	rBV3	1307	1056	0.04%	0.005%
75	12.310	3501	3505	3506	rBV3	1680	1036	0.04%	0.005%
76	12.468	3549	3554	3557	rVB4	1588	1581	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036940.D
 Acq On : 15 Aug 2024 15:20
 Operator : SY/MD
 Sample : P3603-01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.490	3557	3561	3563	rBV3	2225	1696	0.06%	0.009%
78	12.532	3569	3574	3577	rBV7	823	877	0.03%	0.004%
79	12.644	3605	3609	3611	rBV5	926	856	0.03%	0.004%
80	12.709	3627	3629	3632	rBV3	916	740	0.03%	0.004%
81	12.805	3656	3659	3662	rBV4	1081	884	0.03%	0.004%
82	12.905	3686	3690	3693	rVB4	780	759	0.03%	0.004%
83	12.947	3697	3703	3707	rBV6	1976	2238	0.08%	0.011%
84	13.207	3778	3784	3785	rBV6	3676	3224	0.12%	0.016%
85	13.246	3794	3796	3801	rVB5	1245	807	0.03%	0.004%
86	13.345	3825	3827	3831	rVB4	997	728	0.03%	0.004%
87	13.455	3852	3861	3871	rVV4	7517	14830	0.55%	0.075%
88	13.529	3881	3884	3887	rBV4	1356	756	0.03%	0.004%
89	13.683	3928	3932	3934	rBV4	1762	1771	0.07%	0.009%
90	13.747	3948	3952	3954	rVV5	1882	1165	0.04%	0.006%
91	13.760	3954	3956	3959	rVV3	1179	798	0.03%	0.004%
92	13.982	4020	4025	4027	rBV4	2337	1943	0.07%	0.010%
93	14.140	4071	4074	4078	rVB6	1773	1138	0.04%	0.006%
94	14.590	4211	4214	4219	rVB7	1439	1193	0.04%	0.006%
95	14.673	4236	4240	4243	rVB6	1739	1324	0.05%	0.007%
96	14.750	4261	4264	4269	rVV6	1735	1641	0.06%	0.008%
97	14.834	4286	4290	4293	rBV5	973	790	0.03%	0.004%
98	14.930	4318	4320	4323	rBV3	1392	1145	0.04%	0.006%
99	15.014	4344	4346	4351	rVB6	1482	842	0.03%	0.004%
100	15.082	4365	4367	4369	rBV3	1474	728	0.03%	0.004%




Sum of corrected areas: 19801688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036940.D
Acq On : 15 Aug 2024 15:20
Operator : SY/MD
Sample : P3603-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

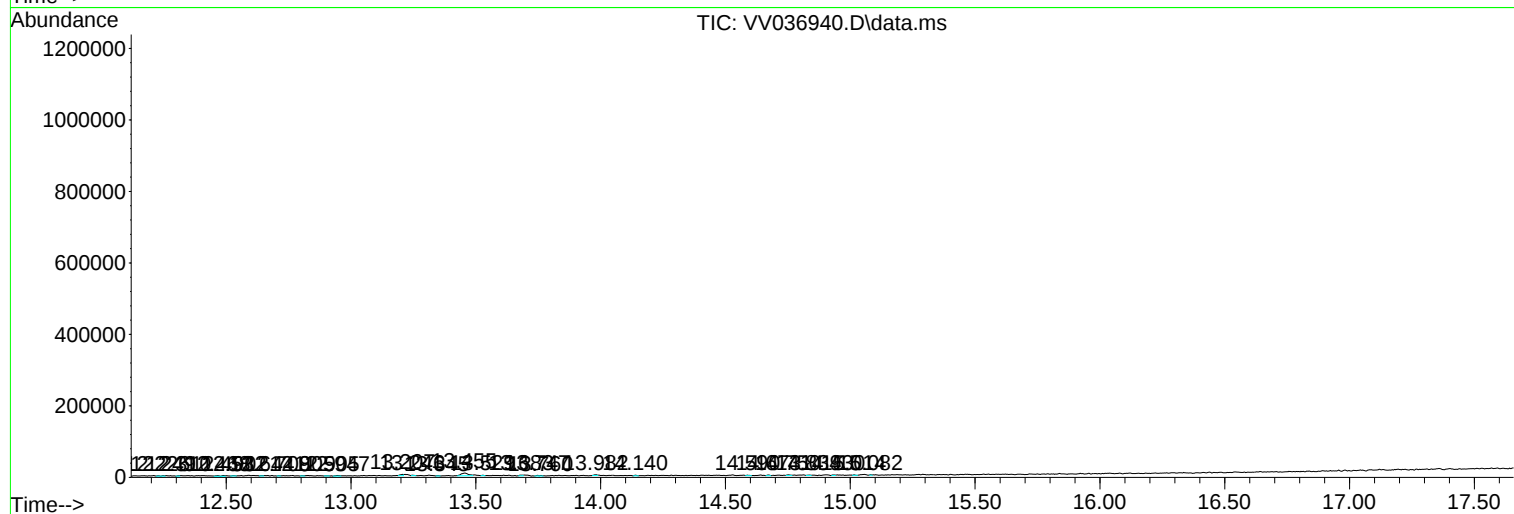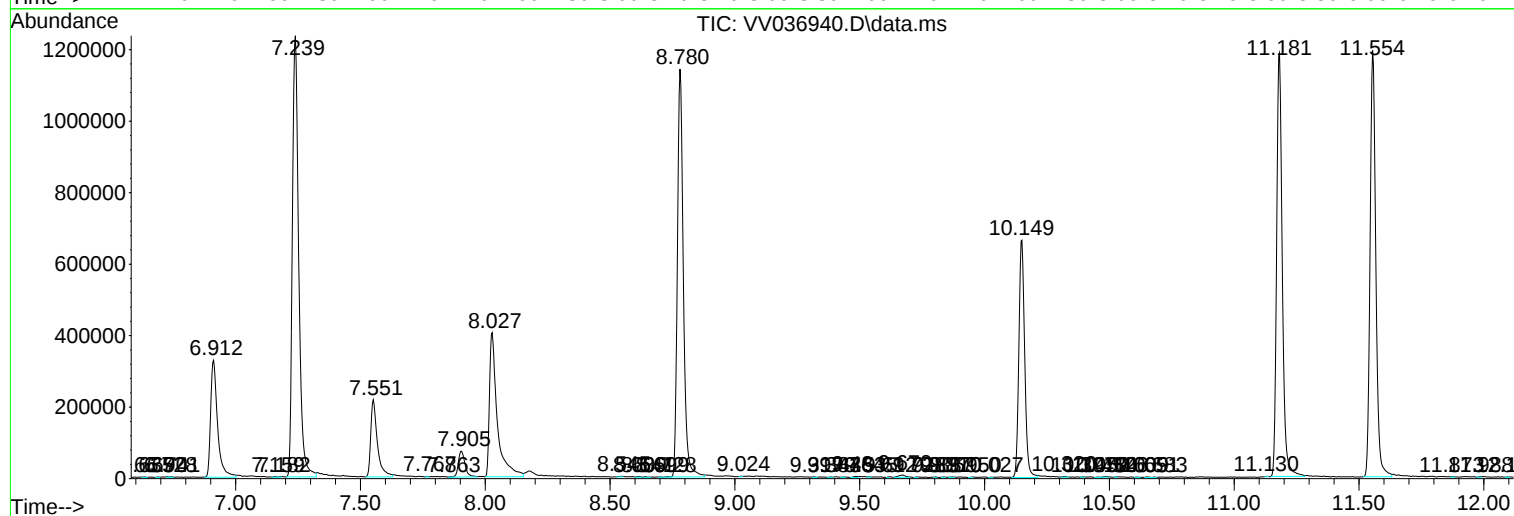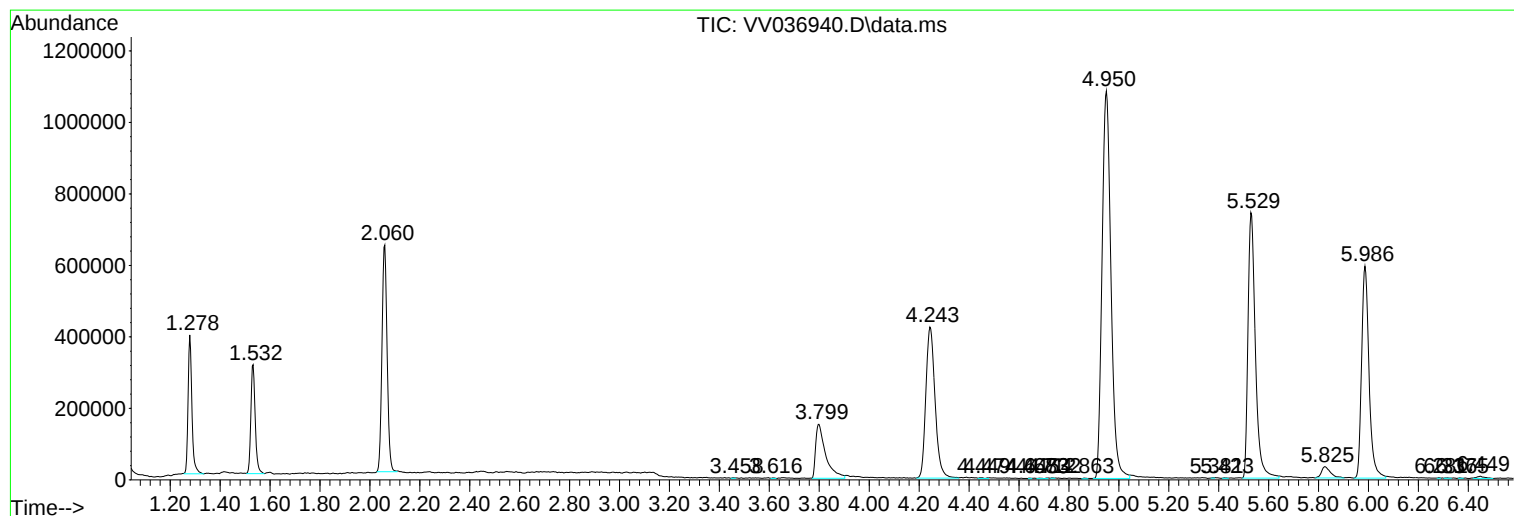

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036940.D
Acq On : 15 Aug 2024 15:20
Operator : SY/MD
Sample : P3603-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036940.D
Acq On : 15 Aug 2024 15:20
Operator : SY/MD
Sample : P3603-01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------