

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036942.D
 Acq On : 15 Aug 2024 16:26
 Operator : SY/MD
 Sample : P3603-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	378052	397993	14.71%	2.052%
2	1.532	146	153	168	rVB	304859	358071	13.24%	1.847%
3	2.059	308	317	333	rVB	634005	907793	33.55%	4.681%
4	3.632	803	806	808	rVB4	1888	1059	0.04%	0.005%
5	3.799	849	858	888	rBV	152032	414257	15.31%	2.136%
6	4.243	981	996	1022	rBV	418126	1056272	39.04%	5.447%
7	4.699	1136	1138	1140	rBV3	1642	891	0.03%	0.005%
8	4.815	1173	1174	1176	rBV2	756	317	0.01%	0.002%
9	4.828	1176	1178	1180	rVV2	503	211	0.01%	0.001%
10	4.838	1180	1181	1182	rVV	810	231	0.01%	0.001%
11	4.847	1182	1184	1186	rVV3	1512	791	0.03%	0.004%
12	4.950	1201	1216	1253	rBV2	1090753	2705437	100.00%	13.952%
13	5.381	1348	1350	1352	rBV3	1146	546	0.02%	0.003%
14	5.529	1386	1396	1426	rBV	728885	1487040	54.96%	7.669%
15	5.985	1526	1538	1568	rBV	592487	1220260	45.10%	6.293%
16	6.365	1653	1656	1659	rBV6	1273	779	0.03%	0.004%
17	6.381	1659	1661	1664	rBV4	1135	639	0.02%	0.003%
18	6.641	1741	1742	1744	rVB2	598	197	0.01%	0.001%
19	6.651	1744	1745	1746	rBV	895	324	0.01%	0.002%
20	6.799	1788	1791	1792	rBV2	933	608	0.02%	0.003%
21	6.831	1799	1801	1803	rBV2	673	367	0.01%	0.002%
22	6.863	1808	1811	1813	rBV3	880	634	0.02%	0.003%
23	6.911	1816	1826	1854	rBV	324649	611613	22.61%	3.154%
24	7.198	1913	1915	1917	rBV3	1852	845	0.03%	0.004%
25	7.239	1917	1928	1958	rBV	1237307	2176288	80.44%	11.223%
26	7.509	2010	2012	2014	rBV3	1180	694	0.03%	0.004%
27	7.551	2017	2025	2051	rVV	211850	389308	14.39%	2.008%
28	7.976	2154	2157	2161	rBV5	1834	1655	0.06%	0.009%
29	7.998	2161	2164	2165	rBV3	1135	750	0.03%	0.004%
30	8.027	2165	2173	2207	rBV2	412856	887451	32.80%	4.577%
31	8.484	2313	2315	2317	rBV3	1285	736	0.03%	0.004%
32	8.522	2325	2327	2329	rBV3	1029	550	0.02%	0.003%
33	8.728	2390	2391	2392	rBV	730	225	0.01%	0.001%
34	8.779	2393	2407	2445	rVV	1129896	1881613	69.55%	9.703%
35	9.188	2532	2534	2538	rBV5	1231	836	0.03%	0.004%
36	9.223	2543	2545	2549	rBV5	1352	1089	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036942.D
 Acq On : 15 Aug 2024 16:26
 Operator : SY/MD
 Sample : P3603-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.291	2564	2566	2567	rBV2	757	333	0.01%	0.002%
38	9.336	2578	2580	2584	rBV5	1102	674	0.02%	0.003%
39	9.371	2587	2591	2593	rBV3	1334	1090	0.04%	0.006%
40	9.406	2598	2602	2606	rBV6	1514	1286	0.05%	0.007%
41	9.445	2611	2614	2616	rBV3	816	455	0.02%	0.002%
42	9.477	2622	2624	2629	rBV6	1000	1003	0.04%	0.005%
43	9.500	2629	2631	2636	rVB6	1849	1051	0.04%	0.005%
44	9.583	2654	2657	2661	rBV5	1203	765	0.03%	0.004%
45	9.606	2661	2664	2668	rBV5	719	543	0.02%	0.003%
46	9.632	2670	2672	2675	rBV2	1284	784	0.03%	0.004%
47	9.686	2685	2689	2690	rBV4	1436	879	0.03%	0.005%
48	9.715	2696	2698	2700	rBV2	934	481	0.02%	0.002%
49	9.763	2710	2713	2714	rBV3	968	432	0.02%	0.002%
50	9.815	2726	2729	2730	rBV2	1120	584	0.02%	0.003%
51	9.844	2736	2738	2740	rBV3	990	511	0.02%	0.003%
52	9.988	2780	2783	2784	rVB2	834	356	0.01%	0.002%
53	10.001	2784	2787	2789	rBV3	822	445	0.02%	0.002%
54	10.024	2791	2794	2796	rBV3	1572	970	0.04%	0.005%
55	10.107	2818	2820	2821	rBV2	1377	611	0.02%	0.003%
56	10.149	2821	2833	2851	rVV	665685	1059603	39.17%	5.464%
57	10.423	2916	2918	2921	rBV3	1170	825	0.03%	0.004%
58	10.496	2931	2941	2948	rBV10	2299	3621	0.13%	0.019%
59	10.545	2954	2956	2960	rVB5	934	576	0.02%	0.003%
60	10.583	2966	2968	2971	rBV3	1083	615	0.02%	0.003%
61	10.612	2971	2977	2980	rBV9	926	1168	0.04%	0.006%
62	10.654	2987	2990	2992	rBV4	1434	769	0.03%	0.004%
63	10.715	3006	3009	3013	rVB5	1452	810	0.03%	0.004%
64	10.738	3013	3016	3022	rVB5	768	507	0.02%	0.003%
65	10.773	3025	3027	3029	rBV3	685	397	0.01%	0.002%
66	10.815	3038	3040	3043	rBV4	706	406	0.02%	0.002%
67	10.831	3043	3045	3048	rVB4	864	497	0.02%	0.003%
68	10.886	3061	3062	3063	rBV	725	230	0.01%	0.001%
69	10.908	3067	3069	3071	rBV3	765	345	0.01%	0.002%
70	10.924	3072	3074	3077	rVB3	869	417	0.02%	0.002%
71	10.940	3077	3079	3081	rBV3	682	355	0.01%	0.002%
72	11.004	3097	3099	3101	rBV4	1154	626	0.02%	0.003%
73	11.046	3109	3112	3114	rBV4	1064	763	0.03%	0.004%
74	11.082	3120	3123	3128	rVB5	1485	957	0.04%	0.005%
75	11.111	3128	3132	3133	rBV4	1494	1023	0.04%	0.005%
76	11.181	3143	3154	3186	rBV	1172214	1849348	68.36%	9.537%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
 Data File : VV036942.D
 Acq On : 15 Aug 2024 16:26
 Operator : SY/MD
 Sample : P3603-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	11.458	3237	3240	3241	rBV2	1374	771	0.03%	0.004%
78	11.554	3259	3270	3297	rBV	1193191	1921003	71.01%	9.906%
79	11.908	3375	3380	3381	rBV5	2202	1659	0.06%	0.009%
80	11.979	3399	3402	3405	rBV4	1511	1184	0.04%	0.006%
81	12.406	3530	3535	3536	rBV4	1129	909	0.03%	0.005%
82	12.445	3545	3547	3550	rVB5	1324	607	0.02%	0.003%
83	12.467	3552	3554	3556	rVB3	1380	693	0.03%	0.004%
84	12.541	3575	3577	3580	rBV3	1106	651	0.02%	0.003%
85	12.577	3586	3588	3589	rBV2	979	464	0.02%	0.002%
86	12.828	3663	3666	3668	rBV3	1466	933	0.03%	0.005%
87	12.853	3672	3674	3679	rVB3	1316	951	0.04%	0.005%
88	12.879	3679	3682	3683	rBV2	978	437	0.02%	0.002%
89	12.914	3690	3693	3694	rBV3	916	538	0.02%	0.003%
90	13.004	3718	3721	3722	rBV2	962	593	0.02%	0.003%
91	13.075	3740	3743	3747	rBV5	970	712	0.03%	0.004%
92	13.123	3756	3758	3762	rVB4	1590	831	0.03%	0.004%
93	13.281	3805	3807	3812	rVB6	1186	739	0.03%	0.004%
94	13.303	3812	3814	3815	rBV2	994	424	0.02%	0.002%
95	13.381	3836	3838	3841	rBV3	1287	699	0.03%	0.004%
96	13.413	3845	3848	3850	rBV4	1008	693	0.03%	0.004%
97	13.458	3854	3862	3868	rBV6	4948	7664	0.28%	0.040%
98	13.609	3907	3909	3911	rBV3	1380	642	0.02%	0.003%
99	13.873	3988	3991	3994	rVB4	1358	685	0.03%	0.004%
100	13.972	4020	4022	4025	rBV4	2085	1442	0.05%	0.007%




Sum of corrected areas: 19391405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036942.D
Acq On : 15 Aug 2024 16:26
Operator : SY/MD
Sample : P3603-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

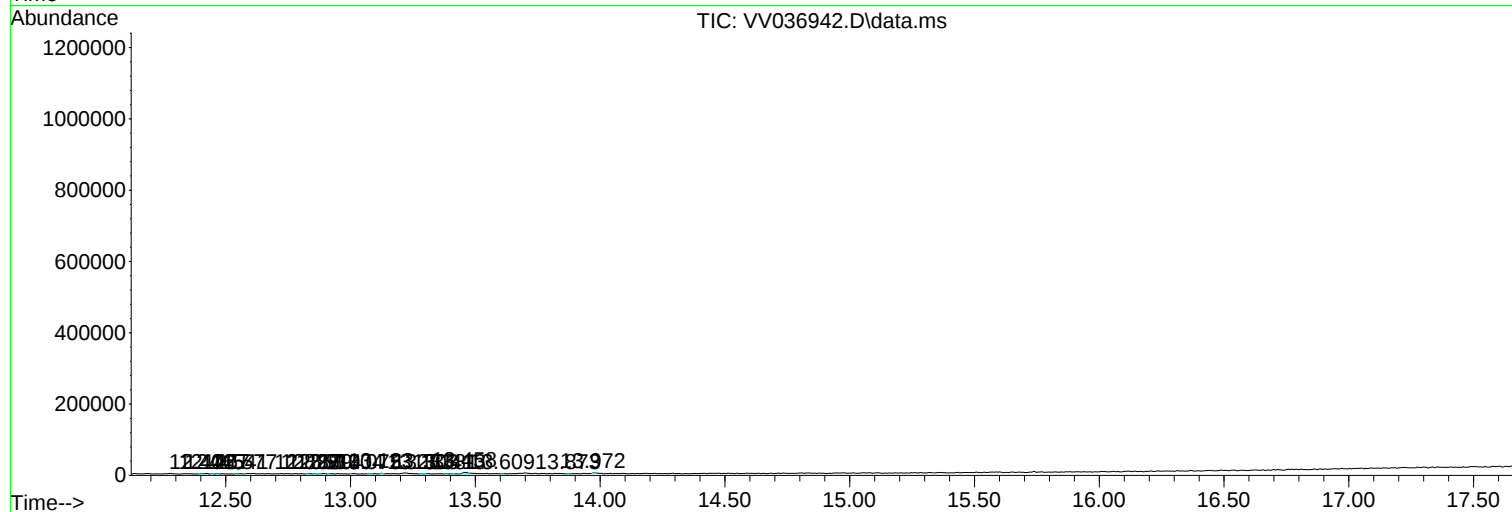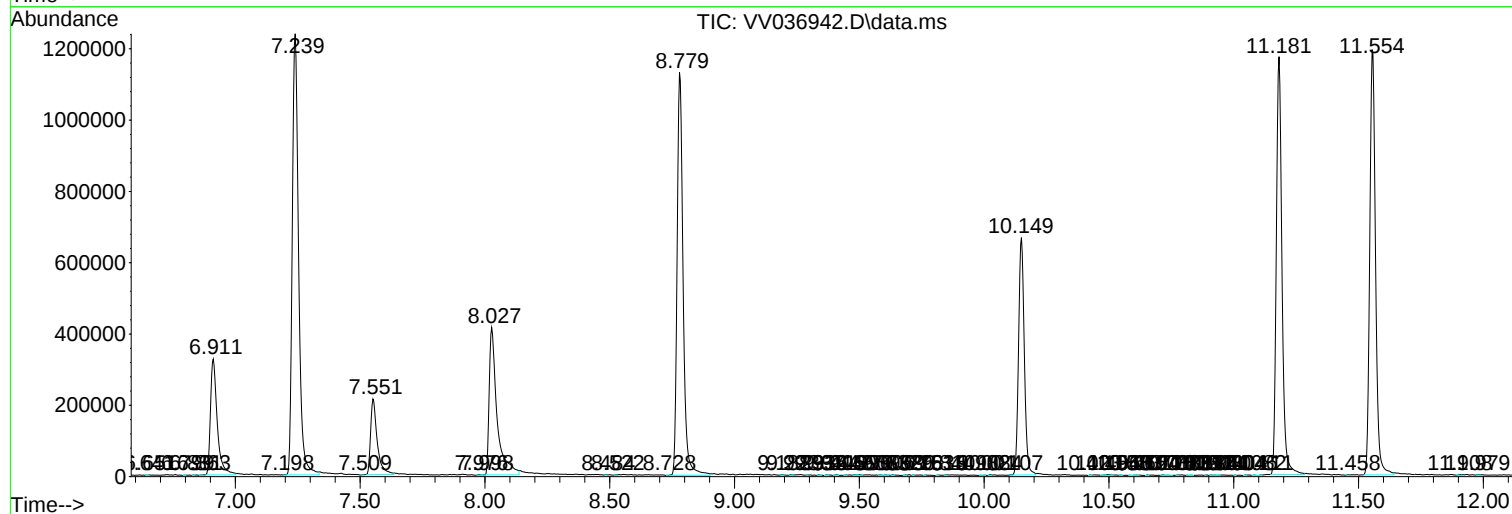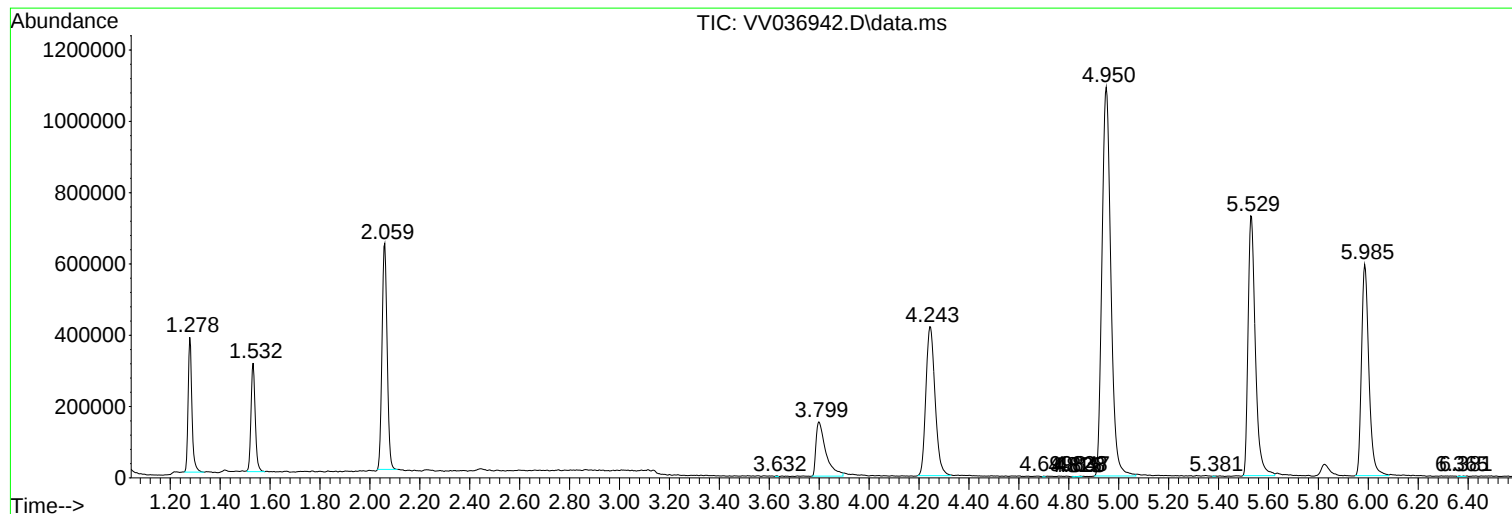

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036942.D
Acq On : 15 Aug 2024 16:26
Operator : SY/MD
Sample : P3603-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036942.D
Acq On : 15 Aug 2024 16:26
Operator : SY/MD
Sample : P3603-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc