
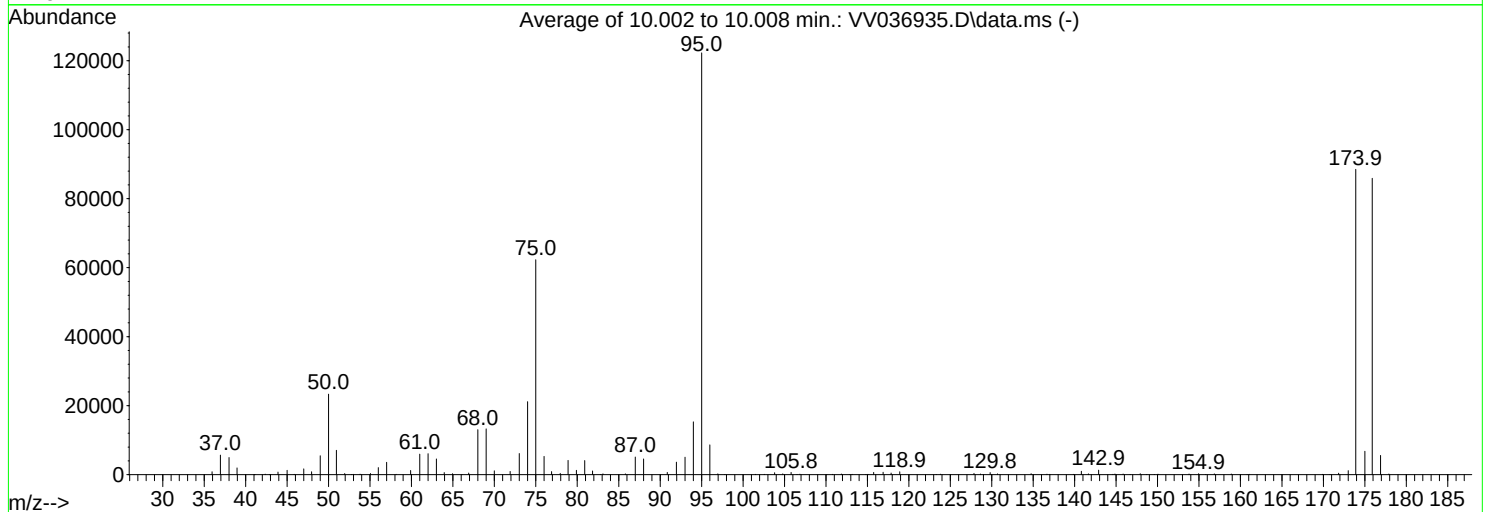


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081524\
Data File : VV036935.D
Acq On : 15 Aug 2024 08:03
Operator : SY/MD
Sample : BFB362
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB362

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Fri Aug 16 02:14:55 2024

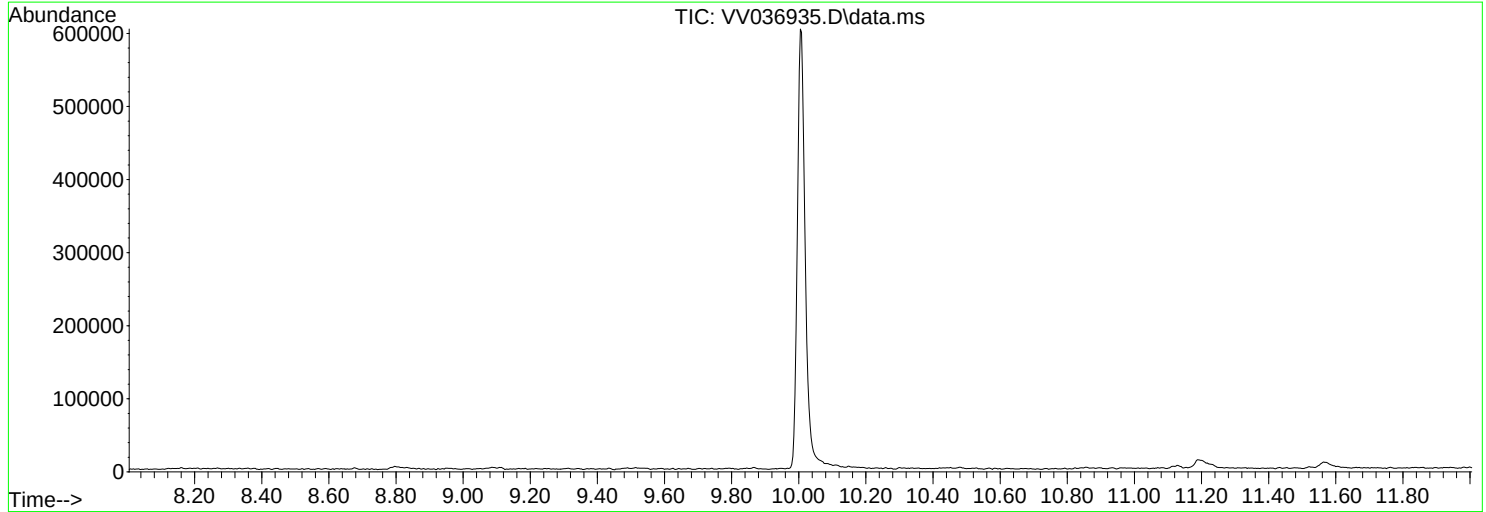

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	23344	PASS
75	95	30	80	51.0	62315	PASS
95	95	100	100	100.0	122272	PASS
96	95	5	9	7.1	8621	PASS
173	174	0.00	2	1.3	1171	PASS
174	95	50	120	72.4	88493	PASS
175	174	5	9	7.6	6764	PASS
176	174	95	105	97.1	85920	PASS
177	176	5	10	6.5	5581	PASS

m/z	Abundance
35.90	104.0
36.80	135.0
38.20	157.0
38.90	210.0
39.90	684.0
40.70	139.0
41.10	160.0
41.90	195.0
42.80	188.0
43.90	1244.0
46.00	129.0
47.60	102.0
48.20	124.0
50.90	124.0
54.70	126.0
57.00	130.0
58.30	120.0
66.20	105.0
70.40	104.0
76.90	195.0
78.10	191.0
96.20	102.0
127.90	105.0
207.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.10	1002.0
37.00	5518.0
38.00	4966.0
39.00	1987.0
40.00	611.0
41.00	158.0
42.40	175.0
43.00	199.0
44.00	2070.0
45.00	1110.0
45.80	181.0
47.00	1660.0
47.90	903.0
49.00	5184.0
50.00	21912.0
51.00	7137.0
52.00	383.0
52.80	126.0
54.00	107.0
55.10	336.0
56.00	2006.0
57.00	3604.0
58.10	221.0
59.90	1141.0
61.00	5447.0
62.00	5728.0
63.00	4164.0
63.90	602.0
64.90	241.0
66.10	131.0
67.00	451.0
68.00	12368.0
69.00	13207.0
70.00	1003.0
71.90	888.0
73.00	5961.0
74.00	20416.0
75.00	59216.0
76.00	5336.0
77.00	978.0
78.00	492.0
78.90	3927.0
79.90	1101.0
80.90	3909.0
81.80	1030.0
82.80	165.0
83.10	137.0
85.80	182.0
87.00	4759.0
88.00	4190.0
90.80	585.0
92.00	3130.0
93.00	4866.0
94.00	14188.0
95.00	115336.0
96.00	8245.0
97.00	187.0
102.50	104.0
103.80	481.0
104.80	232.0
105.80	619.0
106.90	132.0
110.80	120.0
111.90	154.0
113.20	134.0
114.80	137.0
115.80	702.0
116.90	700.0
117.90	359.0
118.90	798.0
123.80	193.0
127.90	395.0
128.60	193.0
129.80	595.0
130.70	219.0
134.80	213.0
136.60	133.0
137.00	125.0
140.80	923.0
141.60	171.0
142.90	1272.0
144.90	251.0
145.80	185.0
147.90	244.0
150.00	128.0
153.80	201.0
155.00	229.0
155.80	104.0
156.90	240.0
158.90	219.0
161.10	134.0
171.80	377.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

173.00	1070.0
173.90	79848.0
175.00	6326.0
175.90	78976.0
176.90	5516.0
177.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.00	919.0
37.00	5975.0
38.00	5315.0
39.00	2270.0
40.10	524.0
41.00	183.0
42.30	147.0
43.00	198.0
44.00	2040.0
45.00	1323.0
45.80	234.0
47.00	1785.0
47.90	854.0
49.00	5765.0
50.00	24104.0
51.00	7498.0
51.90	361.0
53.00	124.0
53.80	112.0
55.10	357.0
56.00	2167.0
57.00	3885.0
58.10	191.0
59.90	1250.0
61.00	6054.0
62.00	6300.0
63.00	4717.0
63.90	633.0
64.90	298.0
66.10	175.0
66.90	472.0
68.00	13619.0
69.00	13763.0
70.00	1155.0
71.90	953.0
73.00	6342.0
74.00	21816.0
75.00	64400.0
76.00	5420.0
76.90	1154.0
77.90	572.0
78.90	4322.0
79.90	1298.0
80.90	4231.0
81.80	1091.0
83.10	250.0
85.80	267.0
87.00	5389.0
88.00	4708.0
90.80	636.0
92.00	3760.0
93.00	5186.0
94.00	15810.0
95.00	126536.0
96.00	9174.0
97.00	225.0
101.50	104.0
102.50	119.0
103.80	580.0
104.80	214.0
105.80	665.0
106.50	147.0
106.90	145.0
110.80	108.0
111.80	178.0
113.10	103.0
115.10	175.0
115.80	651.0
116.90	662.0
117.80	464.0
118.90	859.0
123.30	105.0
123.80	156.0
127.90	481.0
128.70	210.0
129.80	641.0
130.70	261.0
134.70	300.0
136.70	156.0
137.00	144.0
139.90	122.0
140.80	965.0
141.70	261.0
142.90	1360.0
144.80	245.0
145.90	225.0
147.90	270.0
148.70	101.0
149.60	120.0
150.00	148.0
153.80	166.0
155.00	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

156.80	259.0
158.90	185.0
161.00	132.0
169.90	123.0
170.80	110.0
171.80	454.0
173.00	1197.0
173.90	91616.0
175.00	7060.0
175.90	88640.0
176.90	5751.0
177.90	162.0
207.20	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
35.90	873.0
37.00	5881.0
38.00	5070.0
39.00	2198.0
40.10	444.0
41.00	206.0
42.30	166.0
43.00	192.0
43.90	1854.0
45.00	1387.0
45.80	250.0
47.00	1620.0
48.00	803.0
49.00	5513.0
50.00	24016.0
51.00	6865.0
51.90	300.0
53.00	168.0
53.70	156.0
55.00	346.0
56.00	1998.0
57.00	3580.0
58.10	168.0
59.90	1268.0
61.00	6332.0
62.00	6145.0
63.00	4709.0
64.00	595.0
65.00	356.0
66.10	150.0
66.80	486.0
68.00	13066.0
69.00	12826.0
70.00	1196.0
71.90	938.0
73.00	6011.0
74.00	21216.0
75.00	63328.0
76.00	5108.0
76.90	1136.0
77.90	588.0
78.90	4197.0
79.90	1344.0
80.90	4179.0
81.90	1077.0
83.10	326.0
85.80	239.0
87.00	5148.0
88.00	4699.0
90.90	673.0
91.90	3938.0
93.00	5141.0
94.00	15907.0
95.00	124944.0
96.00	8750.0
96.90	237.0
97.80	109.0
101.50	126.0
102.60	112.0
103.80	570.0
104.80	209.0
105.80	643.0
106.70	144.0
110.10	104.0
111.80	173.0
112.90	106.0
115.00	182.0
115.70	547.0
116.90	677.0
117.80	572.0
118.90	822.0
123.90	116.0
127.80	552.0
128.70	172.0
129.00	180.0
129.80	607.0
130.70	244.0
134.70	348.0
136.70	169.0
139.80	137.0
140.80	1038.0
141.70	267.0
142.90	1333.0
144.60	247.0
145.90	219.0
146.70	147.0
147.90	276.0
148.70	109.0
150.10	130.0
153.80	143.0
154.90	353.0
156.90	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

158.90	134.0
160.80	134.0
169.90	113.0
171.90	498.0
173.00	1246.0
173.90	94016.0
175.00	6906.0
175.90	90144.0
176.90	5475.0
177.90	173.0
207.20	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362