

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036953.D
 Acq On : 16 Aug 2024 14:30
 Operator : SY/MD
 Sample : P3648-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 16 23:08:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 16 23:06:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	586994	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	559148	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	261810	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	233775	49.862	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 99.720%			
7) Chloroethane-d5	1.532	69	190613	51.555	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 103.100%			
11) 1,1-Dichloroethene-d2	2.059	65	103324	51.521	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 103.040%			
21) 2-Butanone-d5	3.796	46	251332	101.178	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 101.180%			
24) Chloroform-d	4.246	84	432001	51.346	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.700%			
26) 1,2-Dichloroethane-d4	4.937	65	278121	51.414	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.820%			
32) Benzene-d6	4.953	84	884697	52.385	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.780%			
36) 1,2-Dichloropropane-d6	5.985	67	284409	52.200	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 104.400%			
41) Toluene-d8	7.239	98	797171	51.458	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 102.920%			
43) trans-1,3-Dichloroprop...	7.551	79	124304	43.838	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 87.680%			
47) 2-Hexanone-d5	8.027	63	141997	90.642	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 90.640%			
56) 1,1,2,2-Tetrachloroeth...	10.149	84	326324	52.163	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 104.320%			
66) 1,2-Dichlorobenzene-d4	11.558	152	289766	54.314	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.620%			
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	3059	0.788	ug/L	# 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036953.D
Acq On : 16 Aug 2024 14:30
Operator : SY/MD
Sample : P3648-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 16 23:08:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 16 23:06:03 2024
Response via : Initial Calibration

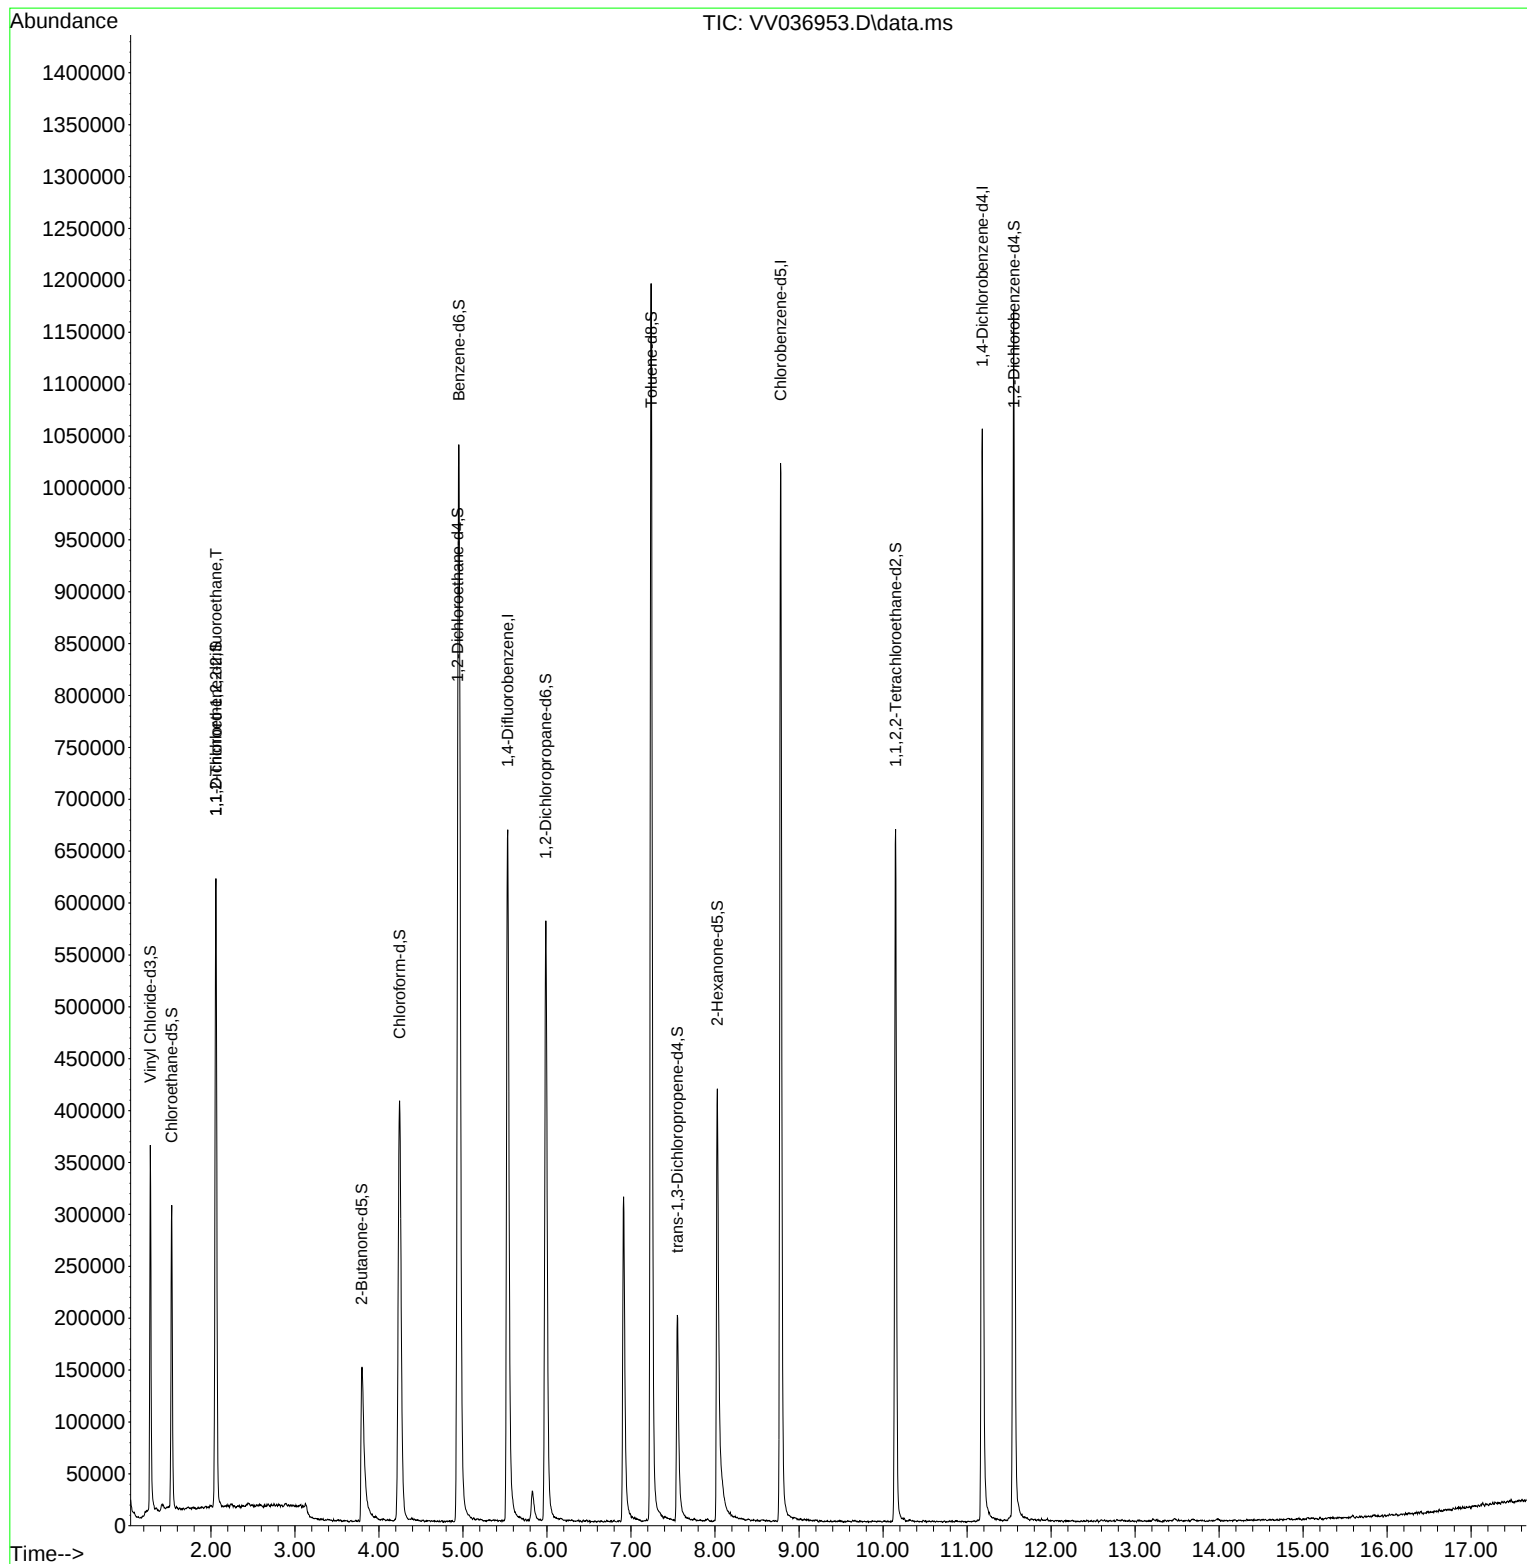

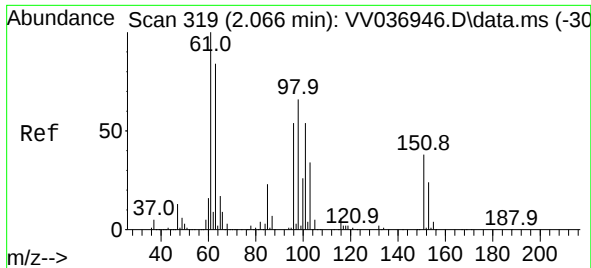

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.788 ug/L
 RT: 2.059 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV036953.D
 Acq: 16 Aug 2024 14:30

Instrument :
 MSVOA_V
 ClientSampleId :

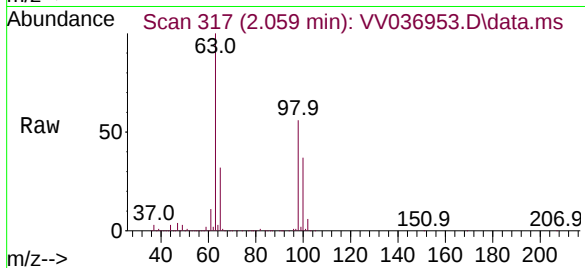

Tgt Ion:101 Resp: 3059
 Ion Ratio Lower Upper
 101 100
 85 11.6 34.6 51.8#
 151 5.8 55.9 83.9#

