

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036956.D
 Acq On : 16 Aug 2024 15:35
 Operator : SY/MD
 Sample : P3648-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 16 23:08:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 16 23:06:03 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	607106	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	579916	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	279593	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	229738	47.378	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	94.760%	
7) Chloroethane-d5	1.532	69	184630	48.282	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	96.560%	
11) 1,1-Dichloroethene-d2	2.056	65	102162	49.254	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	98.500%	
21) 2-Butanone-d5	3.799	46	244987	95.356	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	95.360%	
24) Chloroform-d	4.246	84	426333	48.994	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.980%	
26) 1,2-Dichloroethane-d4	4.937	65	278474	49.773	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.540%	
32) Benzene-d6	4.953	84	872120	49.791	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.580%	
36) 1,2-Dichloropropane-d6	5.985	67	280648	49.665	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.340%	
41) Toluene-d8	7.239	98	770774	47.972	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.940%	
43) trans-1,3-Dichloroprop...	7.551	79	117607	39.991	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.980%	
47) 2-Hexanone-d5	8.027	63	141592	87.146	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	87.150%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	320477	49.393	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.780%	
66) 1,2-Dichlorobenzene-d4	11.558	152	281167	49.350	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.700%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	2947	0.734	ug/L	Qvalue # 26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036956.D
Acq On : 16 Aug 2024 15:35
Operator : SY/MD
Sample : P3648-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 16 23:08:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 16 23:06:03 2024
Response via : Initial Calibration

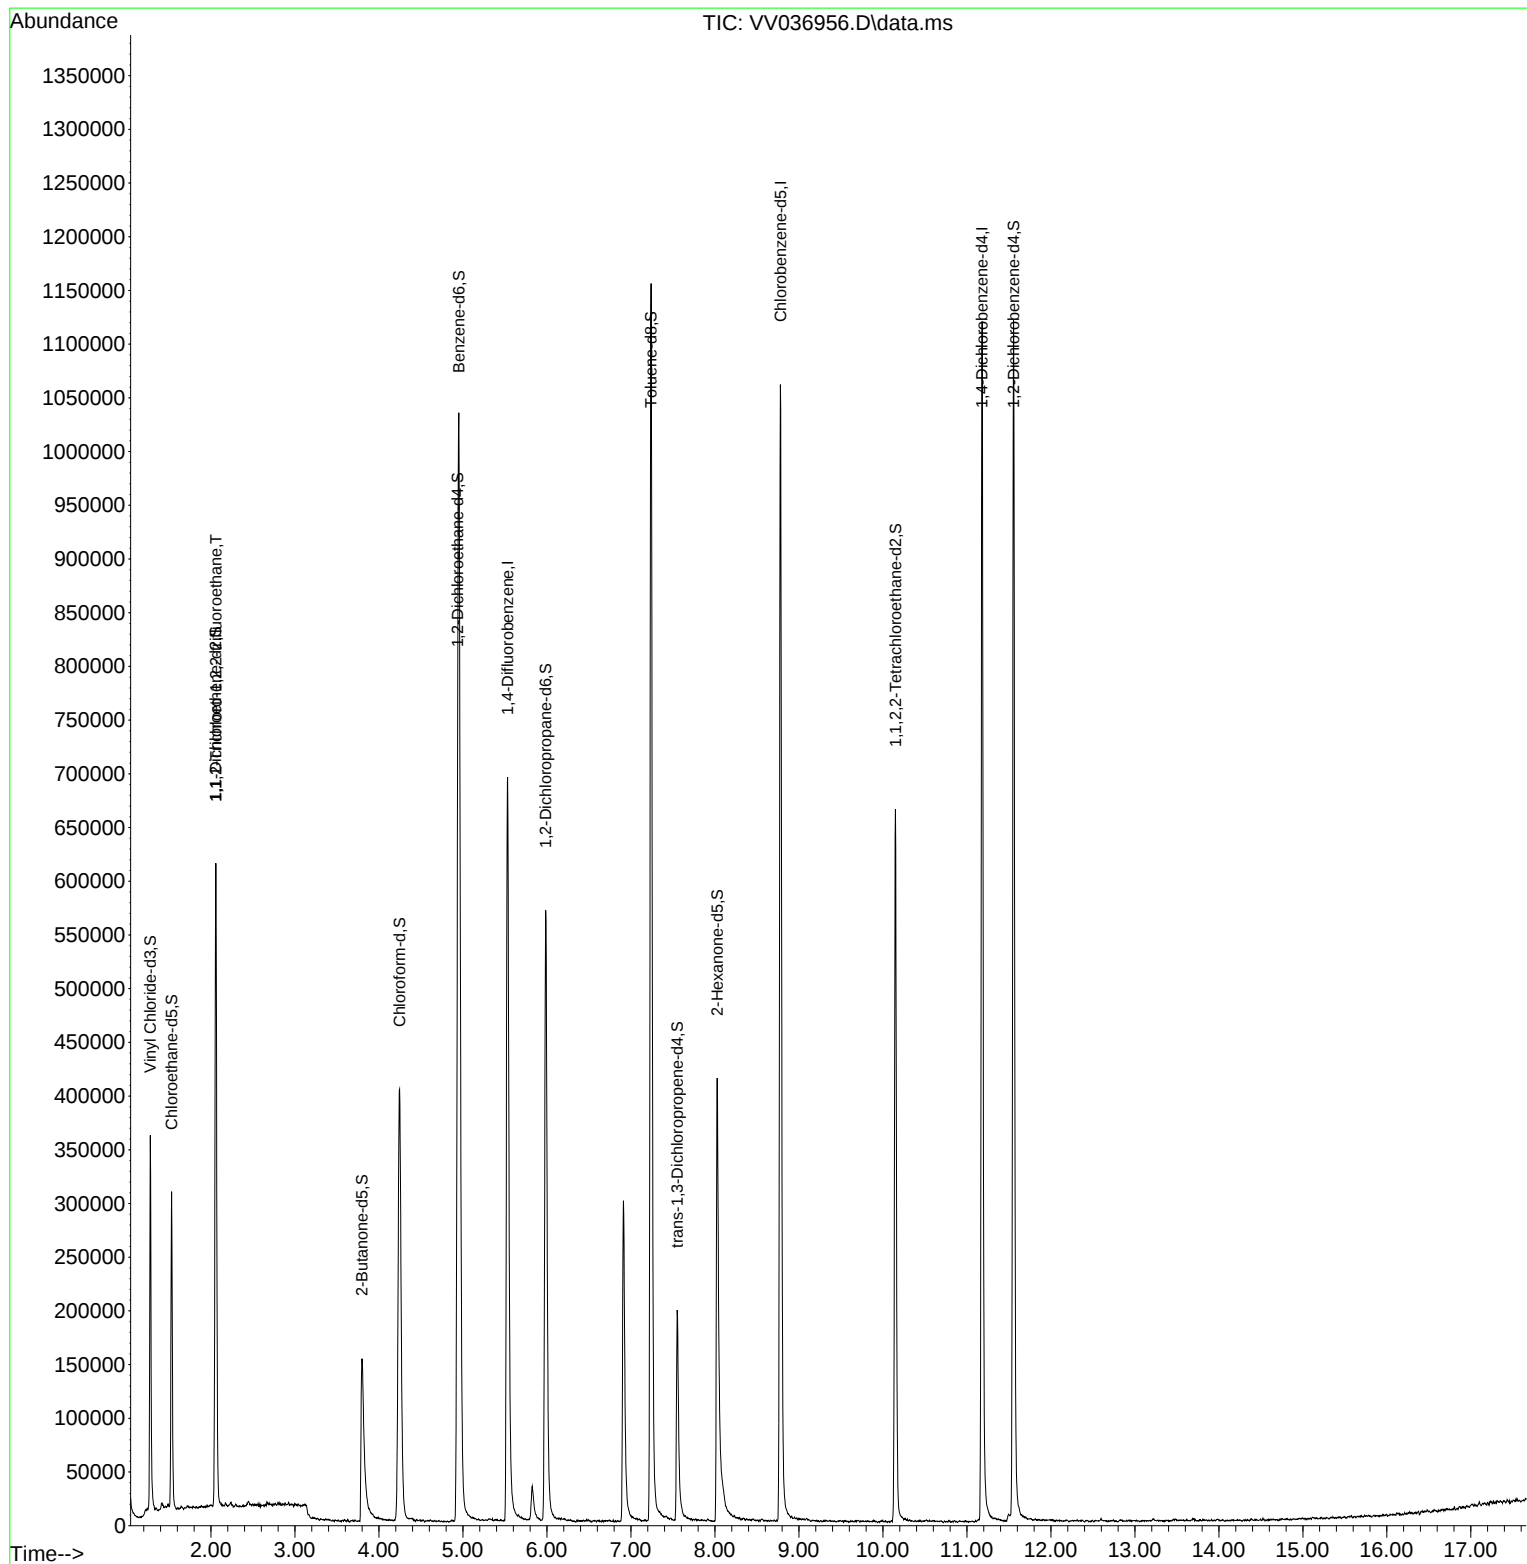

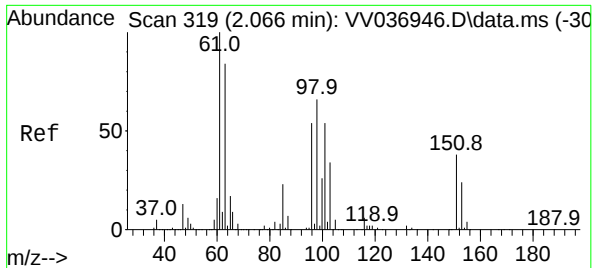

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.734 ug/L
 RT: 2.059 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV036956.D
 Acq: 16 Aug 2024 15:35

Instrument :
 MSVOA_V
 ClientSampleId :

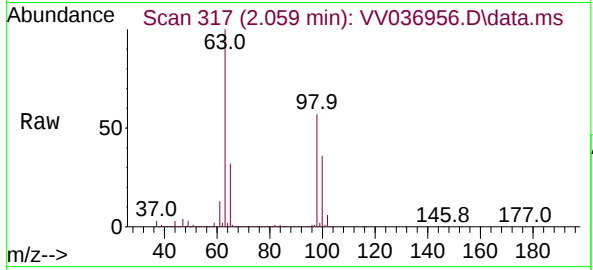

Tgt Ion:	101	Resp:	2947
Ion Ratio	Lower	Upper	
101	100		
85	5.8	34.6	51.8#
151	1.5	55.9	83.9#

