

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036952.D
 Acq On : 16 Aug 2024 14:08
 Operator : SY/MD
 Sample : P3648-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	93	rVB	544734	589967	14.24%	2.198%
2	1.532	146	153	166	rVB	467757	542148	13.09%	2.020%
3	2.059	308	317	333	rVB	961824	1367938	33.02%	5.097%
4	3.413	735	738	740	rBV4	1551	851	0.02%	0.003%
5	3.751	840	843	845	rBV4	1190	749	0.02%	0.003%
6	3.796	848	857	898	rBV	246755	675807	16.31%	2.518%
7	4.246	982	997	1029	rBV	646031	1614649	38.98%	6.017%
8	4.567	1094	1097	1099	rBV3	1541	1177	0.03%	0.004%
9	4.812	1171	1173	1174	rBV2	1012	470	0.01%	0.002%
10	4.844	1180	1183	1188	rVB4	1531	1424	0.03%	0.005%
11	4.873	1188	1192	1193	rBV4	1668	1153	0.03%	0.004%
12	4.950	1200	1216	1246	rBV2	1660026	4142262	100.00%	15.435%
13	5.532	1386	1397	1436	rBV	683530	1418870	34.25%	5.287%
14	5.825	1478	1488	1507	rBV3	36695	86873	2.10%	0.324%
15	5.985	1522	1538	1567	rBV	922384	1879705	45.38%	7.004%
16	6.577	1717	1722	1727	rVB8	2029	1949	0.05%	0.007%
17	6.603	1727	1730	1734	rBV5	934	873	0.02%	0.003%
18	6.628	1734	1738	1739	rBV3	1859	880	0.02%	0.003%
19	6.815	1793	1796	1798	rBV3	1093	508	0.01%	0.002%
20	6.908	1814	1825	1864	rBV	516334	983402	23.74%	3.664%
21	7.239	1917	1928	1957	rBV	1912096	3317015	80.08%	12.360%
22	7.548	2015	2024	2051	rBV2	332652	611927	14.77%	2.280%
23	8.024	2163	2172	2214	rBV2	704397	1431002	34.55%	5.332%
24	8.680	2374	2376	2377	rBV2	597	225	0.01%	0.001%
25	8.696	2379	2381	2385	rVV5	1248	745	0.02%	0.003%
26	8.741	2393	2395	2396	rBV	1307	645	0.02%	0.002%
27	8.780	2397	2407	2440	rVV	1070811	1757787	42.44%	6.550%
28	9.149	2519	2522	2525	rBV5	1366	996	0.02%	0.004%
29	9.181	2530	2532	2537	rVB6	1392	775	0.02%	0.003%
30	9.223	2543	2545	2548	rBV4	1137	522	0.01%	0.002%
31	9.278	2560	2562	2563	rBV2	1038	512	0.01%	0.002%
32	9.484	2622	2626	2628	rVB5	811	433	0.01%	0.002%
33	9.548	2643	2646	2649	rBV4	1820	1446	0.03%	0.005%
34	9.587	2653	2658	2662	rVB7	1699	1525	0.04%	0.006%
35	9.609	2662	2665	2666	rBV2	750	406	0.01%	0.002%
36	9.664	2680	2682	2683	rBV2	756	355	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036952.D
 Acq On : 16 Aug 2024 14:08
 Operator : SY/MD
 Sample : P3648-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.728	2700	2702	2703	rBV2	1011	231	0.01%	0.001%
38	9.770	2712	2715	2719	rBV6	1231	744	0.02%	0.003%
39	9.792	2719	2722	2726	rBV6	1446	1284	0.03%	0.005%
40	9.812	2726	2728	2732	rVB3	1200	744	0.02%	0.003%
41	9.831	2732	2734	2738	rVB3	950	508	0.01%	0.002%
42	9.850	2738	2740	2744	rBV4	1379	1170	0.03%	0.004%
43	9.876	2744	2748	2749	rBV3	1053	566	0.01%	0.002%
44	9.915	2758	2760	2763	rVB3	848	400	0.01%	0.001%
45	9.937	2765	2767	2769	rVV3	500	230	0.01%	0.001%
46	9.960	2772	2774	2775	rVB2	795	268	0.01%	0.001%
47	10.017	2787	2792	2797	rVB8	1255	1258	0.03%	0.005%
48	10.046	2797	2801	2802	rBV3	1106	519	0.01%	0.002%
49	10.066	2806	2807	2810	rVB4	676	253	0.01%	0.001%
50	10.085	2810	2813	2814	rBV2	457	231	0.01%	0.001%
51	10.149	2820	2833	2854	rBV	1072501	1701990	41.09%	6.342%
52	10.361	2898	2899	2901	rBV2	939	424	0.01%	0.002%
53	10.432	2917	2921	2925	rBV6	1107	782	0.02%	0.003%
54	10.464	2929	2931	2932	rBV2	1112	408	0.01%	0.002%
55	10.612	2975	2977	2979	rBV2	608	201	0.00%	0.001%
56	10.638	2979	2985	2991	rVB9	1071	1488	0.04%	0.006%
57	10.660	2991	2992	2993	rBV	357	119	0.00%	0.000%
58	10.693	3001	3002	3006	rBV4	617	340	0.01%	0.001%
59	10.754	3018	3021	3022	rBV2	1165	519	0.01%	0.002%
60	10.792	3030	3033	3036	rVB5	1810	1062	0.03%	0.004%
61	10.857	3048	3053	3054	rBV3	1228	883	0.02%	0.003%
62	10.918	3071	3072	3075	rBV2	730	379	0.01%	0.001%
63	10.943	3075	3080	3082	rVV5	1055	944	0.02%	0.004%
64	10.972	3085	3089	3092	rBV5	1222	968	0.02%	0.004%
65	11.008	3098	3100	3105	rVB6	1378	1154	0.03%	0.004%
66	11.033	3105	3108	3109	rBV3	1630	709	0.02%	0.003%
67	11.181	3143	3154	3182	rBV	1077726	1736296	41.92%	6.470%
68	11.513	3248	3257	3258	rBV7	4223	5541	0.13%	0.021%
69	11.554	3259	3270	3299	rVV	1841244	2910618	70.27%	10.846%
70	12.053	3423	3425	3428	rBV4	1235	746	0.02%	0.003%
71	12.094	3436	3438	3441	rVB4	1382	662	0.02%	0.002%
72	12.146	3452	3454	3457	rBV4	621	456	0.01%	0.002%
73	12.226	3477	3479	3480	rBV2	877	426	0.01%	0.002%
74	12.397	3529	3532	3535	rBV4	1617	1147	0.03%	0.004%
75	12.432	3540	3543	3545	rVV4	1353	789	0.02%	0.003%
76	12.448	3545	3548	3550	rVV3	1021	554	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036952.D
 Acq On : 16 Aug 2024 14:08
 Operator : SY/MD
 Sample : P3648-04
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	12.586	3587	3591	3594	rBV5	2311	1866	0.05%	0.007%
78	12.734	3634	3637	3639	rBV4	870	567	0.01%	0.002%
79	12.792	3653	3655	3656	rBV3	694	243	0.01%	0.001%
80	12.828	3663	3666	3668	rBV4	1793	1134	0.03%	0.004%
81	12.876	3677	3681	3683	rBV3	1603	1057	0.03%	0.004%
82	13.008	3720	3722	3725	rBV4	1398	920	0.02%	0.003%
83	13.082	3743	3745	3749	rBV4	1164	819	0.02%	0.003%
84	13.458	3853	3862	3866	rBV6	4071	5230	0.13%	0.019%
85	13.548	3888	3890	3893	rBV3	889	485	0.01%	0.002%
86	13.686	3928	3933	3939	rBV8	3074	4427	0.11%	0.016%
87	13.750	3951	3953	3957	rVB5	1275	736	0.02%	0.003%
88	13.773	3957	3960	3964	rBV4	1114	986	0.02%	0.004%
89	13.808	3969	3971	3975	rVV4	1288	822	0.02%	0.003%
90	14.438	4164	4167	4172	rBV7	1684	1259	0.03%	0.005%




Sum of corrected areas: 26836533

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036952.D
Acq On : 16 Aug 2024 14:08
Operator : SY/MD
Sample : P3648-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

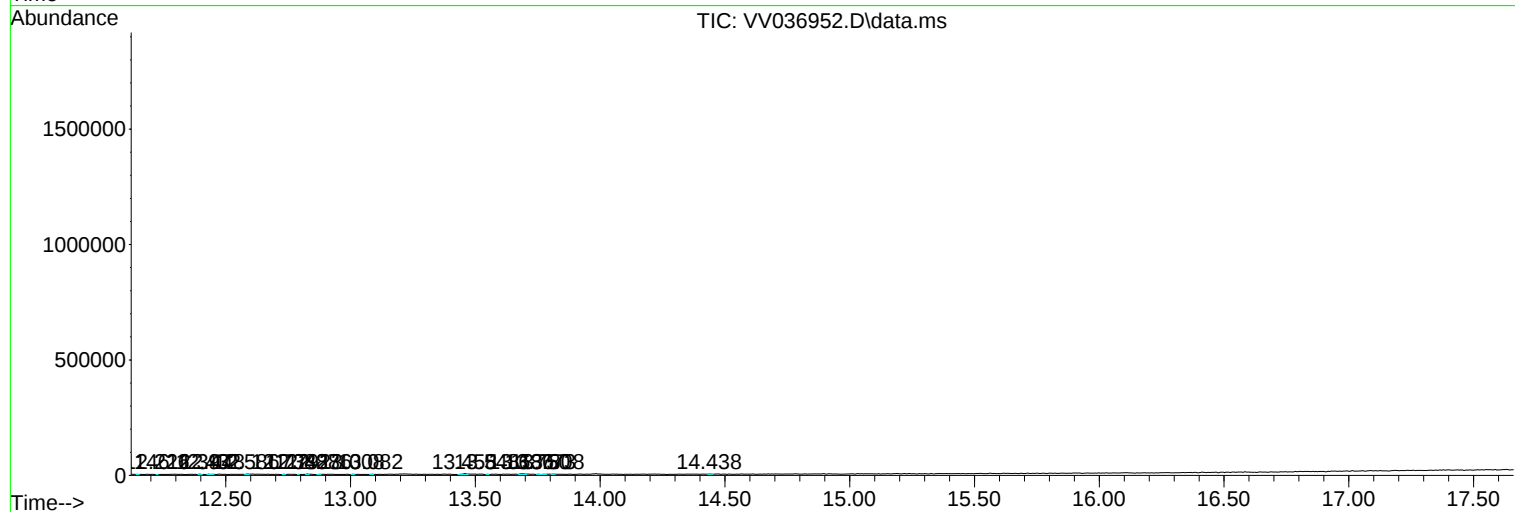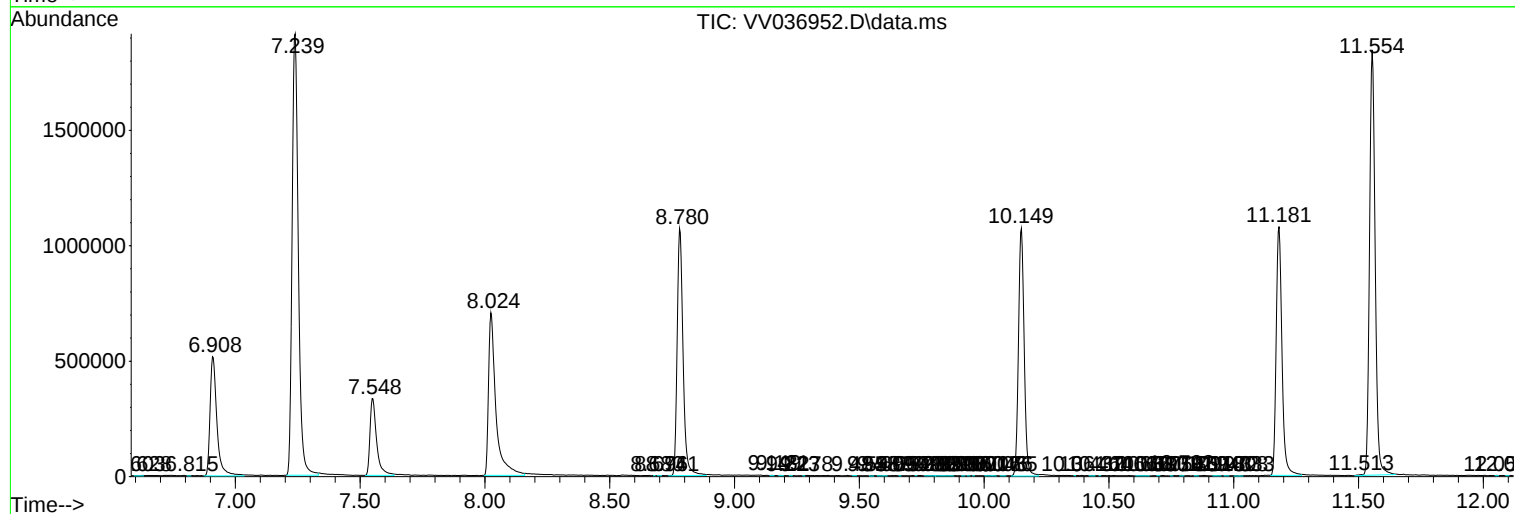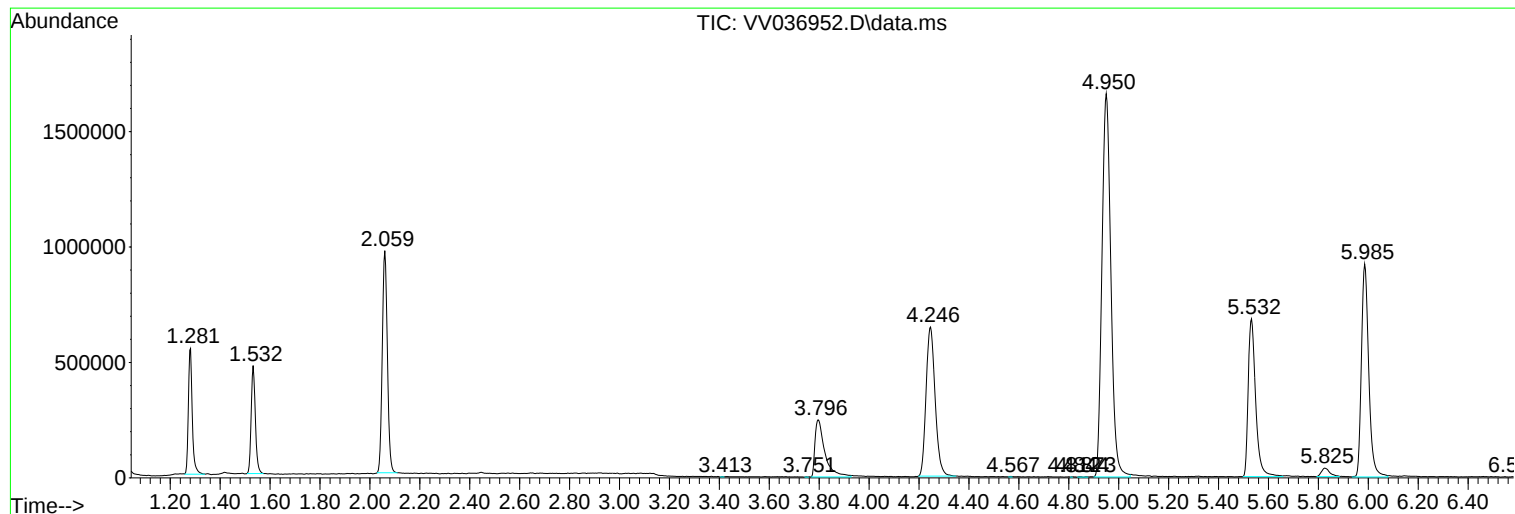

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036952.D
Acq On : 16 Aug 2024 14:08
Operator : SY/MD
Sample : P3648-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036952.D
Acq On : 16 Aug 2024 14:08
Operator : SY/MD
Sample : P3648-04
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc