

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036954.D
 Acq On : 16 Aug 2024 14:51
 Operator : SY/MD
 Sample : P3648-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	342820	367745	14.25%	1.968%
2	1.532	146	153	166	rVB	294767	337290	13.07%	1.805%
3	2.060	308	317	331	rVB	595843	853722	33.08%	4.570%
4	3.799	849	858	884	rBV	149456	399345	15.47%	2.137%
5	4.243	982	996	1026	rVB	402817	1006048	38.98%	5.385%
6	4.548	1088	1091	1095	rBV5	1286	1022	0.04%	0.005%
7	4.600	1105	1107	1110	rBV4	1076	740	0.03%	0.004%
8	4.641	1116	1120	1121	rBV4	1027	736	0.03%	0.004%
9	4.748	1152	1153	1154	rBV	633	226	0.01%	0.001%
10	4.757	1154	1156	1159	rVV3	878	472	0.02%	0.003%
11	4.950	1200	1216	1247	rBV2	1043011	2580926	100.00%	13.814%
12	5.400	1353	1356	1358	rBV4	1688	792	0.03%	0.004%
13	5.529	1385	1396	1432	rBV	707180	1462229	56.66%	7.827%
14	5.825	1481	1488	1505	rVB3	30070	62219	2.41%	0.333%
15	5.985	1526	1538	1569	rBV	571381	1167624	45.24%	6.250%
16	6.301	1634	1636	1640	rVB5	1523	1117	0.04%	0.006%
17	6.339	1640	1648	1650	rBV6	1873	2079	0.08%	0.011%
18	6.506	1696	1700	1703	rBV5	1151	992	0.04%	0.005%
19	6.542	1709	1711	1715	rVB5	1103	642	0.02%	0.003%
20	6.590	1724	1726	1727	rBV	546	276	0.01%	0.001%
21	6.619	1732	1735	1737	rBV4	917	652	0.03%	0.003%
22	6.706	1758	1762	1765	rBV4	1748	1013	0.04%	0.005%
23	6.741	1771	1773	1780	rBV7	1327	789	0.03%	0.004%
24	6.821	1795	1798	1800	rBV3	1300	567	0.02%	0.003%
25	6.837	1802	1803	1806	rBV3	901	499	0.02%	0.003%
26	6.873	1812	1814	1816	rBV3	537	377	0.01%	0.002%
27	6.911	1816	1826	1858	rVV	304116	588984	22.82%	3.153%
28	7.239	1917	1928	1961	rBV	1165052	2057423	79.72%	11.012%
29	7.509	2010	2012	2014	rBV2	1444	642	0.02%	0.003%
30	7.551	2016	2025	2055	rVV	197209	373741	14.48%	2.000%
31	7.863	2120	2122	2126	rBV4	1329	823	0.03%	0.004%
32	8.027	2164	2173	2217	rBV2	406799	891903	34.56%	4.774%
33	8.545	2331	2334	2336	rBV4	2020	1445	0.06%	0.008%
34	8.780	2396	2407	2437	rBV	1084602	1819973	70.52%	9.741%
35	9.191	2532	2535	2537	rBV4	1220	753	0.03%	0.004%
36	9.284	2561	2564	2565	rBV3	1166	698	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036954.D
 Acq On : 16 Aug 2024 14:51
 Operator : SY/MD
 Sample : P3648-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.307	2569	2571	2572	rBV2	1017	479	0.02%	0.003%
38	9.345	2581	2583	2585	rBV3	930	491	0.02%	0.003%
39	9.381	2593	2594	2595	rBV2	867	293	0.01%	0.002%
40	9.474	2617	2623	2625	rBV6	1979	1669	0.06%	0.009%
41	9.612	2663	2666	2669	rBV5	1343	888	0.03%	0.005%
42	9.625	2669	2670	2672	rVV2	1083	295	0.01%	0.002%
43	9.651	2676	2678	2681	rVB4	607	348	0.01%	0.002%
44	9.706	2693	2695	2697	rVB3	1016	394	0.02%	0.002%
45	9.725	2699	2701	2703	rBV3	894	406	0.02%	0.002%
46	9.776	2714	2717	2723	rBV4	1718	1710	0.07%	0.009%
47	9.815	2727	2729	2731	rVB3	754	223	0.01%	0.001%
48	9.850	2738	2740	2744	rBV4	1406	835	0.03%	0.004%
49	9.915	2758	2760	2765	rBV5	1454	1203	0.05%	0.006%
50	9.934	2765	2766	2768	rBV2	775	267	0.01%	0.001%
51	9.969	2774	2777	2779	rBV4	963	560	0.02%	0.003%
52	10.046	2799	2801	2803	rBV3	684	340	0.01%	0.002%
53	10.149	2821	2833	2858	rBV	653717	1050934	40.72%	5.625%
54	10.281	2872	2874	2877	rBV4	1219	817	0.03%	0.004%
55	10.352	2892	2896	2901	rVB8	1767	1959	0.08%	0.010%
56	10.374	2901	2903	2905	rBV3	1097	478	0.02%	0.003%
57	10.426	2917	2919	2922	rBV3	908	551	0.02%	0.003%
58	10.480	2933	2936	2937	rBV3	942	569	0.02%	0.003%
59	10.567	2960	2963	2966	rBV4	984	619	0.02%	0.003%
60	10.587	2966	2969	2972	rVB4	998	494	0.02%	0.003%
61	10.609	2975	2976	2978	rVB2	353	108	0.00%	0.001%
62	10.625	2978	2981	2983	rBV3	413	229	0.01%	0.001%
63	10.648	2983	2988	2989	rBV4	1058	743	0.03%	0.004%
64	10.738	3013	3016	3017	rBV3	1042	578	0.02%	0.003%
65	10.747	3017	3019	3025	rVV6	1531	1346	0.05%	0.007%
66	10.834	3044	3046	3048	rVB3	739	293	0.01%	0.002%
67	10.847	3048	3050	3051	rBV2	995	468	0.02%	0.003%
68	10.934	3075	3077	3080	rVB4	1191	512	0.02%	0.003%
69	10.950	3080	3082	3084	rBV3	1165	609	0.02%	0.003%
70	10.966	3085	3087	3089	rVV3	704	245	0.01%	0.001%
71	10.988	3091	3094	3099	rBV7	1175	1382	0.05%	0.007%
72	11.088	3123	3125	3128	rBV3	1026	640	0.02%	0.003%
73	11.181	3143	3154	3187	rBV	1105303	1782764	69.07%	9.542%
74	11.503	3246	3254	3259	rBV10	5722	10143	0.39%	0.054%
75	11.554	3260	3270	3300	rVB	1138953	1818107	70.44%	9.731%
76	12.242	3482	3484	3486	rBV3	677	428	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036954.D
 Acq On : 16 Aug 2024 14:51
 Operator : SY/MD
 Sample : P3648-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

77	12.300	3501	3502	3504	rBV2	1012	512	0.02%	0.003%
78	12.381	3522	3527	3528	rBV6	1716	1083	0.04%	0.006%
79	12.506	3562	3566	3568	rVB5	1103	692	0.03%	0.004%
80	12.525	3568	3572	3573	rBV3	1465	1000	0.04%	0.005%
81	12.622	3600	3602	3603	rBV2	933	331	0.01%	0.002%
82	12.728	3632	3635	3637	rBV3	943	571	0.02%	0.003%
83	12.876	3679	3681	3683	rBV3	1197	612	0.02%	0.003%
84	12.930	3694	3698	3700	rBV4	1338	1000	0.04%	0.005%
85	13.094	3745	3749	3751	rBV4	1152	1036	0.04%	0.006%
86	13.139	3760	3763	3765	rBV2	1395	864	0.03%	0.005%
87	13.255	3797	3799	3800	rBV2	1129	596	0.02%	0.003%
88	13.345	3824	3827	3829	rBV3	794	544	0.02%	0.003%
89	13.455	3857	3861	3863	rBV5	2245	1622	0.06%	0.009%
90	14.117	4064	4067	4068	rBV3	1164	632	0.02%	0.003%




Sum of corrected areas: 18683036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036954.D
Acq On : 16 Aug 2024 14:51
Operator : SY/MD
Sample : P3648-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

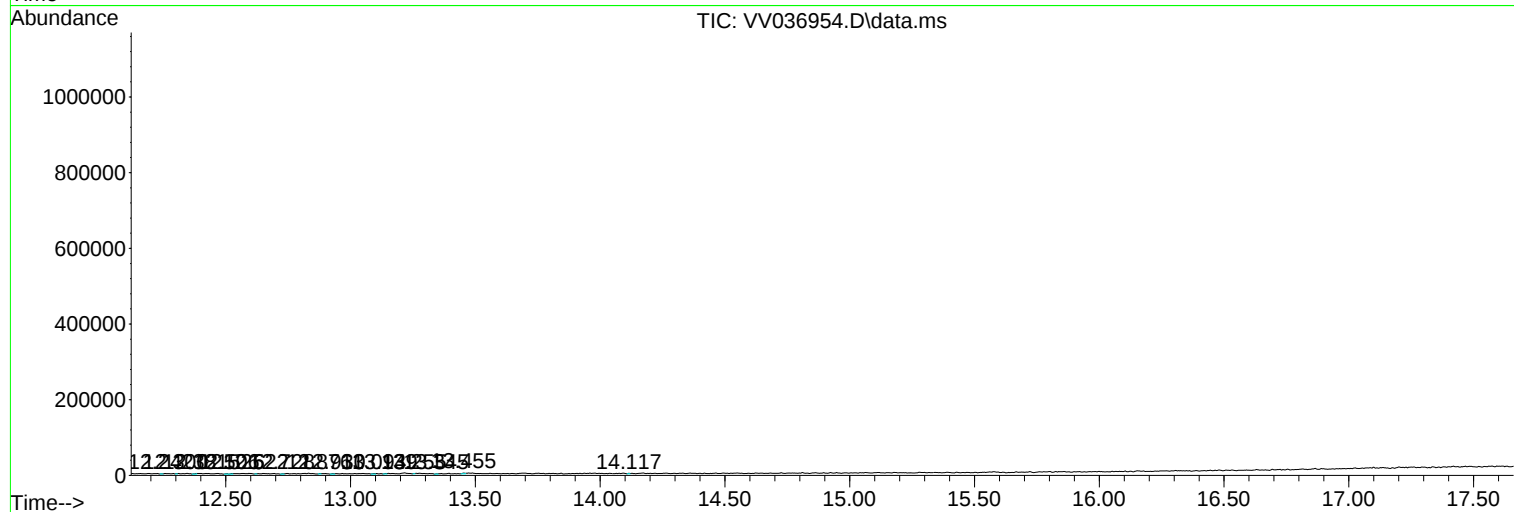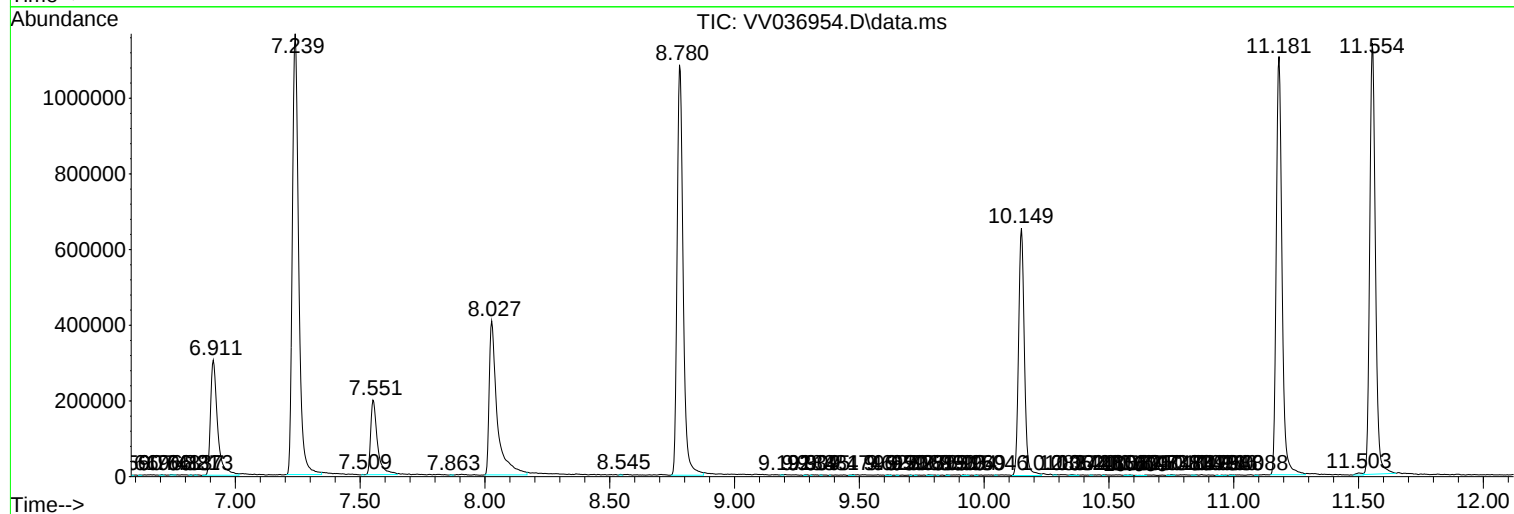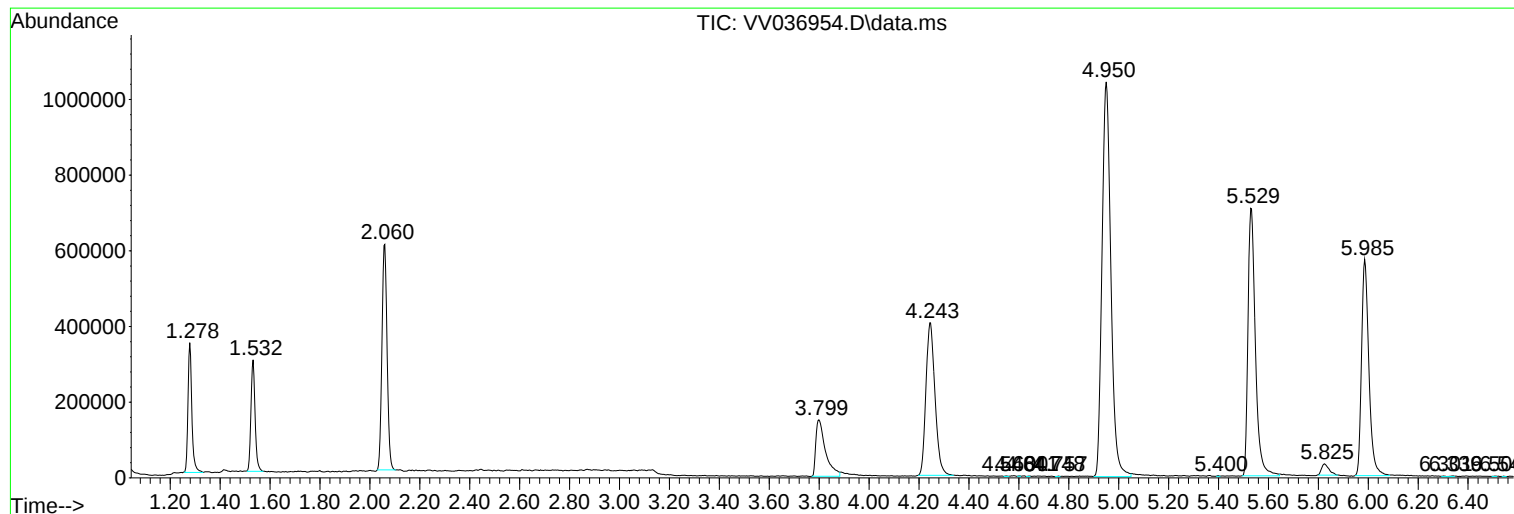

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036954.D
Acq On : 16 Aug 2024 14:51
Operator : SY/MD
Sample : P3648-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036954.D
Acq On : 16 Aug 2024 14:51
Operator : SY/MD
Sample : P3648-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc