

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036955.D
 Acq On : 16 Aug 2024 15:13
 Operator : SY/MD
 Sample : P3648-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

Signal : TIC: VV036955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	334115	354482	14.15%	1.963%
2	1.532	146	153	168	rVB	279018	334380	13.35%	1.852%
3	2.060	308	317	330	rVB	578799	831058	33.17%	4.602%
4	3.757	841	845	849	rBV7	1614	1334	0.05%	0.007%
5	3.799	849	858	885	rBV	145569	390927	15.60%	2.165%
6	4.246	982	997	1026	rVB	389512	985899	39.35%	5.459%
7	4.693	1133	1136	1138	rBV4	1048	674	0.03%	0.004%
8	4.751	1152	1154	1157	rBV5	742	467	0.02%	0.003%
9	4.783	1162	1164	1165	rBV2	755	235	0.01%	0.001%
10	4.847	1179	1184	1186	rBV6	1370	1194	0.05%	0.007%
11	4.863	1186	1189	1195	rVV7	1354	1158	0.05%	0.006%
12	4.950	1201	1216	1243	rBV2	1011903	2505235	100.00%	13.872%
13	5.532	1386	1397	1427	rBV	691792	1427932	57.00%	7.907%
14	5.985	1526	1538	1563	rBV	556000	1138040	45.43%	6.302%
15	6.339	1646	1648	1650	rBV3	1286	570	0.02%	0.003%
16	6.513	1698	1702	1705	rBV4	1057	953	0.04%	0.005%
17	6.600	1728	1729	1733	rVB4	1272	593	0.02%	0.003%
18	6.619	1733	1735	1738	rVB4	1198	597	0.02%	0.003%
19	6.638	1738	1741	1745	rVB6	1957	1414	0.06%	0.008%
20	6.657	1745	1747	1748	rBV2	1361	537	0.02%	0.003%
21	6.670	1748	1751	1753	rBV3	1550	973	0.04%	0.005%
22	6.754	1774	1777	1780	rVB3	1599	1123	0.04%	0.006%
23	6.854	1805	1808	1811	rBV5	1063	875	0.03%	0.005%
24	6.911	1814	1826	1850	rBV	297713	570326	22.77%	3.158%
25	7.239	1917	1928	1959	rBV	1147078	2009550	80.21%	11.128%
26	7.551	2017	2025	2055	rBV	185747	347329	13.86%	1.923%
27	8.027	2165	2173	2214	rBV2	392469	853374	34.06%	4.725%
28	8.706	2382	2384	2385	rBV3	749	276	0.01%	0.002%
29	8.780	2396	2407	2433	rBV	1064183	1757287	70.14%	9.731%
30	9.333	2576	2579	2581	rBV4	1732	1074	0.04%	0.006%
31	9.387	2593	2596	2599	rBV5	2135	1340	0.05%	0.007%
32	9.403	2599	2601	2604	rVV3	950	430	0.02%	0.002%
33	9.448	2612	2615	2617	rBV3	890	629	0.03%	0.003%
34	9.603	2661	2663	2665	rVB3	900	395	0.02%	0.002%
35	9.654	2676	2679	2680	rBV4	1060	555	0.02%	0.003%
36	9.712	2694	2697	2701	rBV5	1931	1056	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036955.D
 Acq On : 16 Aug 2024 15:13
 Operator : SY/MD
 Sample : P3648-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAAS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.808	2725	2727	2732	rVB6	995	617	0.02%	0.003%
38	9.831	2732	2734	2737	rVB4	824	416	0.02%	0.002%
39	9.850	2737	2740	2744	rBV4	1266	965	0.04%	0.005%
40	9.995	2782	2785	2786	rBV3	1016	595	0.02%	0.003%
41	10.034	2795	2797	2798	rBV2	788	441	0.02%	0.002%
42	10.098	2813	2817	2820	rBV5	1340	1105	0.04%	0.006%
43	10.149	2821	2833	2854	rVV	642077	1015558	40.54%	5.623%
44	10.435	2916	2922	2923	rBV5	1057	962	0.04%	0.005%
45	10.474	2931	2934	2936	rBV3	2022	1210	0.05%	0.007%
46	10.551	2957	2958	2960	rBV2	995	372	0.01%	0.002%
47	10.577	2964	2966	2967	rBV2	977	326	0.01%	0.002%
48	10.635	2981	2984	2985	rBV3	755	368	0.01%	0.002%
49	10.689	2999	3001	3006	rVB5	1453	1382	0.06%	0.008%
50	10.715	3006	3009	3010	rBV2	1795	909	0.04%	0.005%
51	10.780	3025	3029	3032	rBV5	1411	1182	0.05%	0.007%
52	10.850	3048	3051	3053	rBV3	757	509	0.02%	0.003%
53	10.943	3079	3080	3081	rVB	644	124	0.00%	0.001%
54	10.953	3081	3083	3087	rBV4	934	732	0.03%	0.004%
55	10.979	3090	3091	3092	rBV4	373	118	0.00%	0.001%
56	11.017	3100	3103	3108	rBV6	1229	1008	0.04%	0.006%
57	11.050	3110	3113	3114	rBV3	760	334	0.01%	0.002%
58	11.088	3123	3125	3129	rBV5	861	505	0.02%	0.003%
59	11.181	3143	3154	3185	rBV	1094631	1740963	69.49%	9.640%
60	11.554	3260	3270	3298	rBV	1114987	1760661	70.28%	9.749%
61	11.927	3384	3386	3388	rBV2	1259	659	0.03%	0.004%
62	12.287	3494	3498	3501	rBV4	1696	1394	0.06%	0.008%
63	12.648	3608	3610	3618	rVB6	1013	1039	0.04%	0.006%
64	12.689	3621	3623	3625	rBV2	1000	511	0.02%	0.003%




Sum of corrected areas: 18059236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036955.D
Acq On : 16 Aug 2024 15:13
Operator : SY/MD
Sample : P3648-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

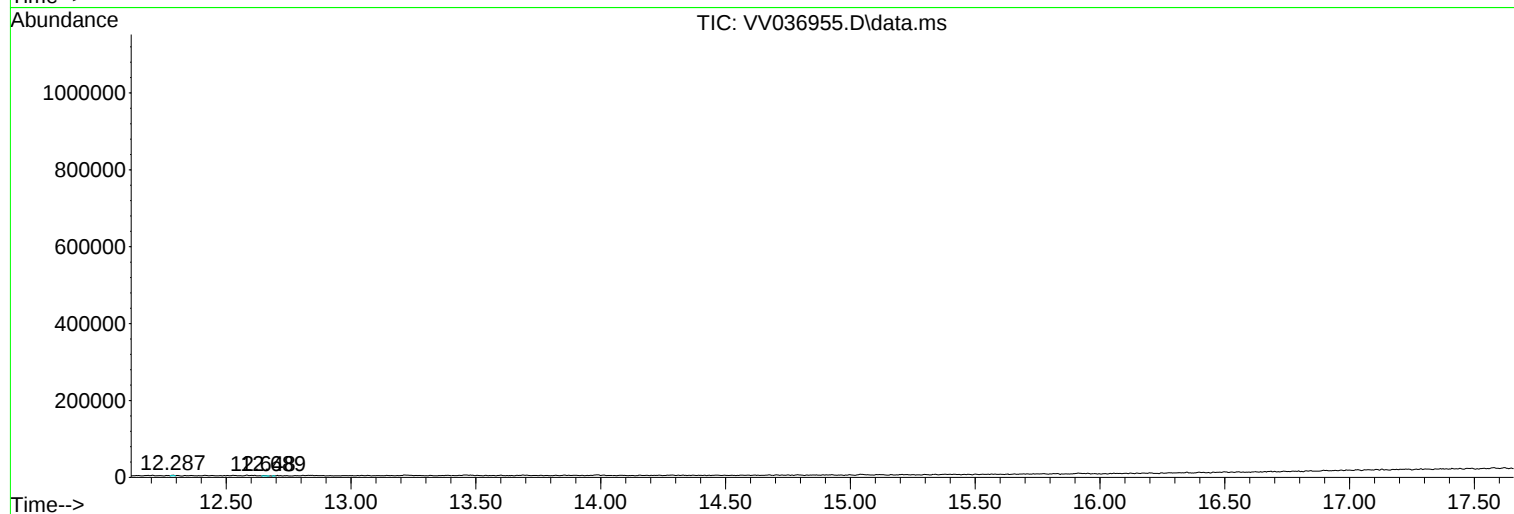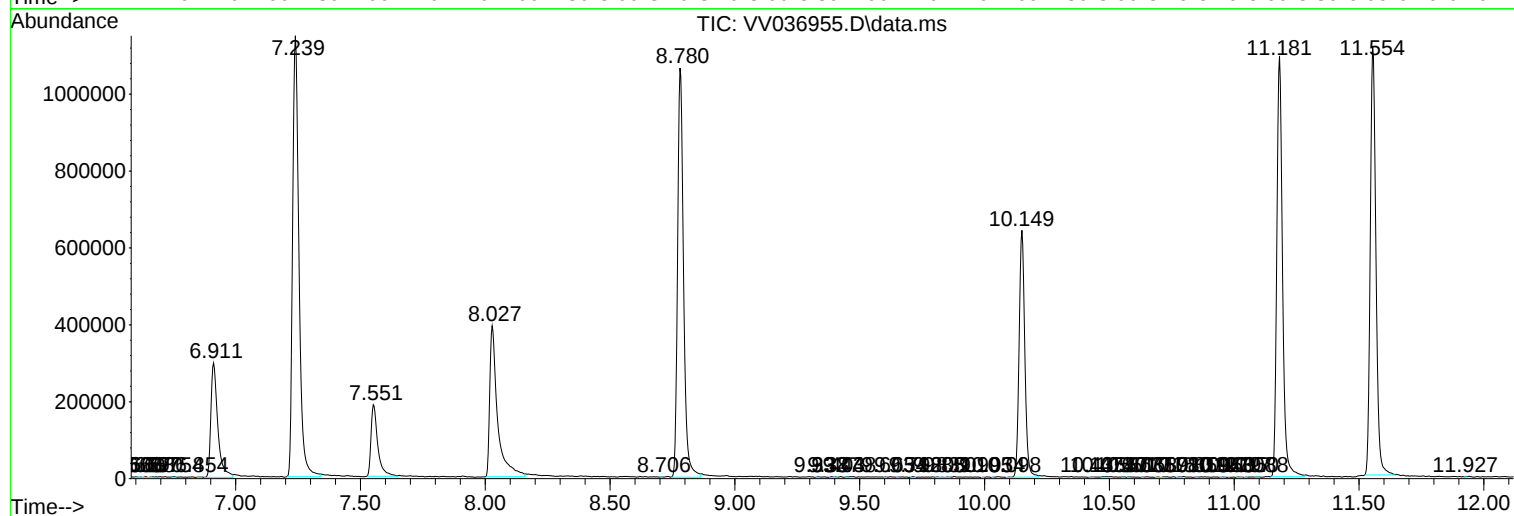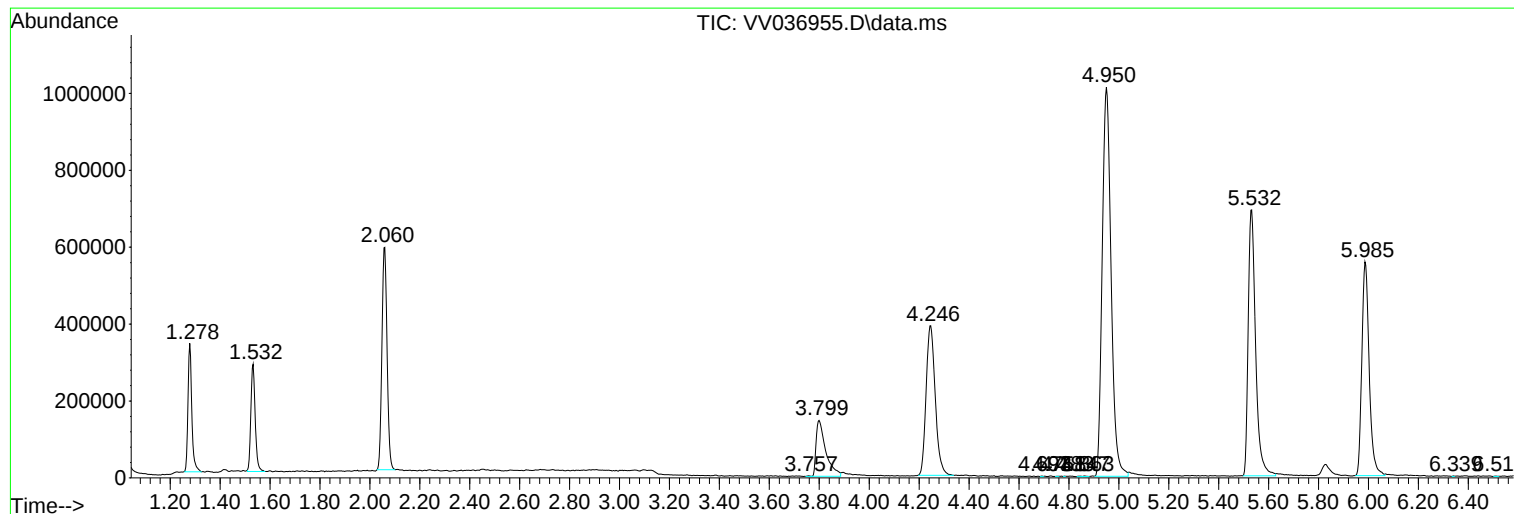

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036955.D
Acq On : 16 Aug 2024 15:13
Operator : SY/MD
Sample : P3648-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036955.D
Acq On : 16 Aug 2024 15:13
Operator : SY/MD
Sample : P3648-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAAS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
