

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036959.D
 Acq On : 16 Aug 2024 16:41
 Operator : SY/MD
 Sample : P3648-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

Signal : TIC: VV036959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	350589	361842	13.05%	1.788%
2	1.529	146	152	169	rVB	280242	345376	12.46%	1.707%
3	2.056	307	316	331	rBV	599127	859668	31.00%	4.249%
4	3.580	787	790	791	rBV3	1516	799	0.03%	0.004%
5	3.799	849	858	889	rBV	156524	426296	15.37%	2.107%
6	4.265	981	1003	1034	rBV4	841002	2772752	100.00%	13.703%
7	4.680	1130	1132	1137	rBV6	1229	930	0.03%	0.005%
8	4.760	1155	1157	1160	rBV4	901	352	0.01%	0.002%
9	4.812	1171	1173	1177	rBV5	945	401	0.01%	0.002%
10	4.873	1187	1192	1194	rBV5	2094	1765	0.06%	0.009%
11	4.950	1198	1216	1248	rBV2	1040363	2570271	92.70%	12.702%
12	5.432	1364	1366	1368	rVB3	1548	580	0.02%	0.003%
13	5.448	1368	1371	1372	rBV3	929	480	0.02%	0.002%
14	5.529	1386	1396	1433	rBV	684234	1407399	50.76%	6.955%
15	5.985	1526	1538	1564	rBV	565941	1155031	41.66%	5.708%
16	6.435	1668	1678	1697	rBV	64256	131424	4.74%	0.650%
17	6.657	1744	1747	1752	rBV7	1903	1456	0.05%	0.007%
18	6.731	1764	1770	1772	rBV5	1424	1480	0.05%	0.007%
19	6.815	1793	1796	1800	rBV4	1153	782	0.03%	0.004%
20	6.841	1801	1804	1808	rVV6	1514	989	0.04%	0.005%
21	6.911	1816	1826	1848	rBV	302579	576703	20.80%	2.850%
22	7.239	1917	1928	1955	rBV	1149372	2030023	73.21%	10.032%
23	7.551	2017	2025	2054	rBV	191037	352990	12.73%	1.744%
24	8.027	2164	2173	2203	rBV2	428634	897033	32.35%	4.433%
25	8.609	2351	2354	2356	rVB4	1349	708	0.03%	0.003%
26	8.686	2376	2378	2380	rBV2	1181	601	0.02%	0.003%
27	8.779	2395	2407	2441	rBV	1044901	1755674	63.32%	8.677%
28	9.226	2544	2546	2548	rBV3	968	561	0.02%	0.003%
29	9.255	2553	2555	2560	rVB5	1706	1222	0.04%	0.006%
30	9.336	2576	2580	2581	rBV4	1208	806	0.03%	0.004%
31	9.451	2613	2616	2618	rVB3	1329	619	0.02%	0.003%
32	9.464	2618	2620	2622	rBV2	943	448	0.02%	0.002%
33	9.525	2635	2639	2642	rBV4	1528	1047	0.04%	0.005%
34	9.545	2642	2645	2649	rBV5	1076	939	0.03%	0.005%
35	9.677	2682	2686	2689	rBV6	861	794	0.03%	0.004%
36	9.725	2696	2701	2703	rBV5	1557	1115	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
 Data File : VV036959.D
 Acq On : 16 Aug 2024 16:41
 Operator : SY/MD
 Sample : P3648-14
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JAATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
 Title : VOC Analysis

37	9.760	2710	2712	2713	rBV2	724	233	0.01%	0.001%
38	9.779	2715	2718	2721	rVB3	1676	1162	0.04%	0.006%
39	9.799	2723	2724	2726	rBV2	564	258	0.01%	0.001%
40	9.812	2726	2728	2730	rVB3	1184	444	0.02%	0.002%
41	9.828	2730	2733	2735	rBV2	1170	821	0.03%	0.004%
42	9.876	2746	2748	2752	rVB5	1671	887	0.03%	0.004%
43	9.905	2755	2757	2760	rVB3	1152	584	0.02%	0.003%
44	9.985	2781	2782	2785	rVB3	486	200	0.01%	0.001%
45	10.004	2785	2788	2790	rBV3	878	479	0.02%	0.002%
46	10.040	2797	2799	2803	rVB4	1174	615	0.02%	0.003%
47	10.066	2803	2807	2808	rBV2	1415	913	0.03%	0.005%
48	10.149	2820	2833	2856	rBV	653015	1047722	37.79%	5.178%
49	10.358	2896	2898	2901	rBV5	824	556	0.02%	0.003%
50	10.374	2901	2903	2905	rBV3	895	451	0.02%	0.002%
51	10.455	2926	2928	2929	rBV2	873	416	0.02%	0.002%
52	10.570	2962	2964	2966	rBV3	857	412	0.01%	0.002%
53	10.586	2966	2969	2971	rVB3	1453	650	0.02%	0.003%
54	10.603	2973	2974	2977	rVB3	1350	627	0.02%	0.003%
55	10.619	2977	2979	2980	rBV	1429	453	0.02%	0.002%
56	10.664	2991	2993	2995	rBV3	951	479	0.02%	0.002%
57	10.680	2995	2998	2999	rVV3	819	450	0.02%	0.002%
58	10.705	3003	3006	3008	rVV3	1386	934	0.03%	0.005%
59	10.738	3011	3016	3019	rBV4	1663	1276	0.05%	0.006%
60	10.754	3019	3021	3023	rBV2	593	272	0.01%	0.001%
61	10.767	3023	3025	3029	rBV5	1120	664	0.02%	0.003%
62	10.789	3029	3032	3037	rBV7	2115	1654	0.06%	0.008%
63	10.937	3074	3078	3079	rBV3	1178	744	0.03%	0.004%
64	10.950	3081	3082	3085	rVB3	829	356	0.01%	0.002%
65	10.969	3085	3088	3091	rBV4	816	412	0.01%	0.002%
66	10.988	3091	3094	3095	rBV3	375	261	0.01%	0.001%
67	11.017	3099	3103	3107	rBV4	1412	1127	0.04%	0.006%
68	11.049	3110	3113	3117	rBV5	1833	1381	0.05%	0.007%
69	11.117	3127	3134	3136	rBV7	1892	2205	0.08%	0.011%
70	11.181	3144	3154	3187	rBV	1071280	1706964	61.56%	8.436%
71	11.554	3260	3270	3295	rBV	1118878	1786910	64.45%	8.831%
72	12.249	3484	3486	3488	rBV3	1115	439	0.02%	0.002%
73	12.400	3529	3533	3534	rBV2	1301	940	0.03%	0.005%
74	12.506	3565	3566	3568	rBV2	1191	477	0.02%	0.002%
75	12.564	3582	3584	3585	rBV2	963	317	0.01%	0.002%
76	12.683	3619	3621	3626	rBV6	1485	1380	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036959.D
Acq On : 16 Aug 2024 16:41
Operator : SY/MD
Sample : P3648-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAATO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M

Title : VOC Analysis

77	12.782	3650	3652	3653	rBV2	1026	356	0.01%	0.002%
78	13.017	3720	3725	3727	rBV5	1396	1054	0.04%	0.005%
79	13.146	3760	3765	3767	rBV5	1479	1330	0.05%	0.007%
80	13.258	3798	3800	3803	rBV4	1198	727	0.03%	0.004%
81	13.818	3970	3974	3979	rBV7	1294	1454	0.05%	0.007%
82	13.924	4005	4007	4009	rBV3	1154	703	0.03%	0.003%




Sum of corrected areas: 20234505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036959.D
Acq On : 16 Aug 2024 16:41
Operator : SY/MD
Sample : P3648-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAATO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

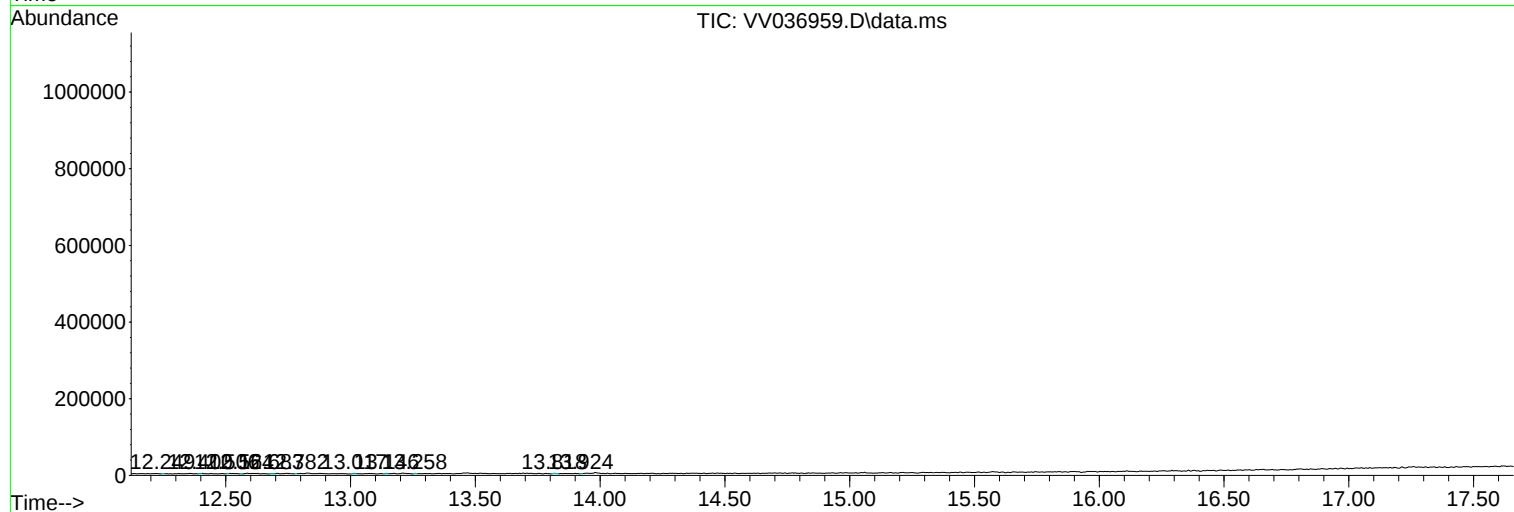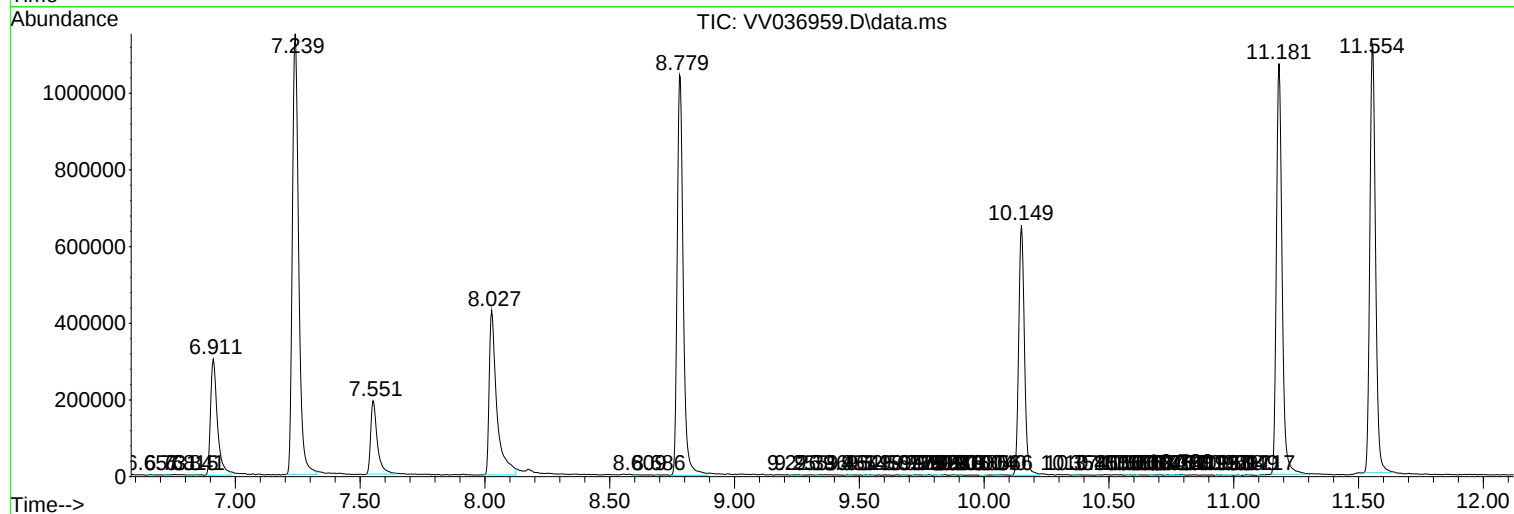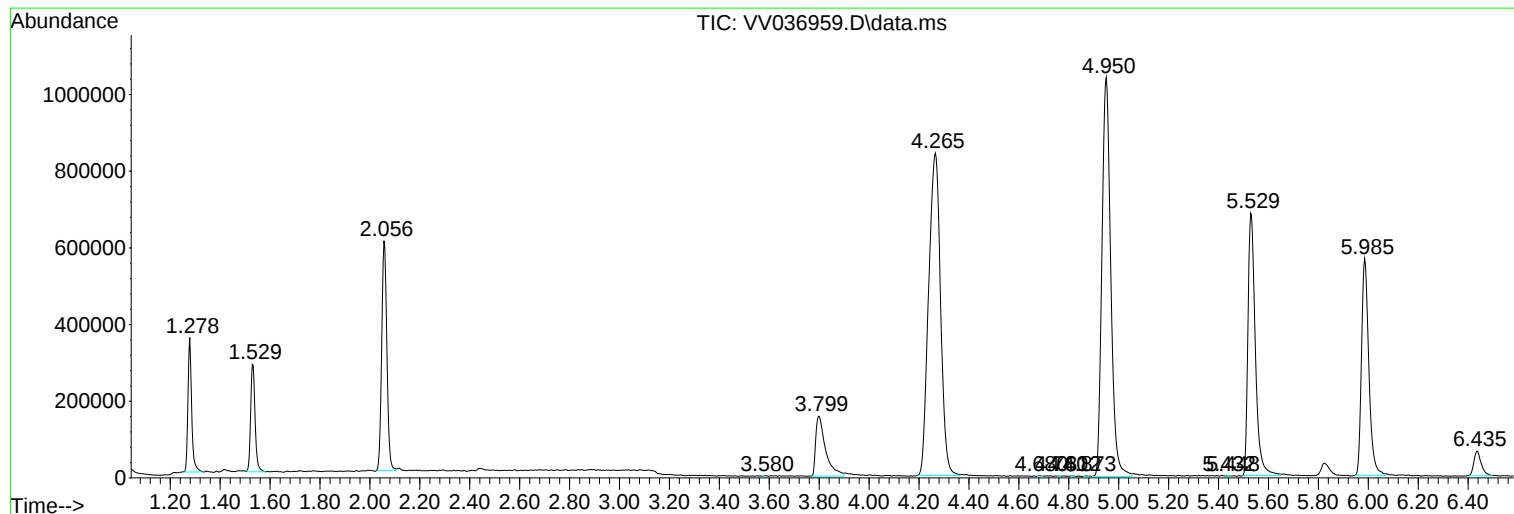

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036959.D
Acq On : 16 Aug 2024 16:41
Operator : SY/MD
Sample : P3648-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAATO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036959.D
Acq On : 16 Aug 2024 16:41
Operator : SY/MD
Sample : P3648-14
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JAATO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
