
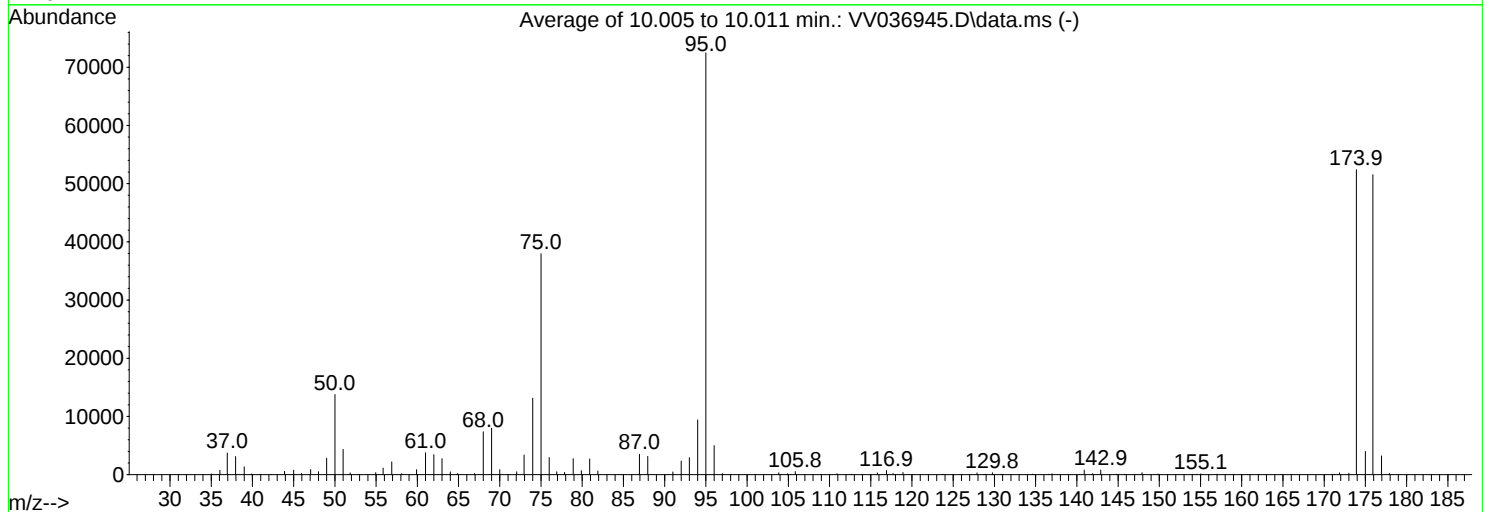


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081624\
Data File : VV036945.D
Acq On : 16 Aug 2024 07:53
Operator : SY/MD
Sample : BFB363
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB363

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080224WMA.M
Title : VOC Analysis
Last Update : Fri Aug 16 23:06:03 2024

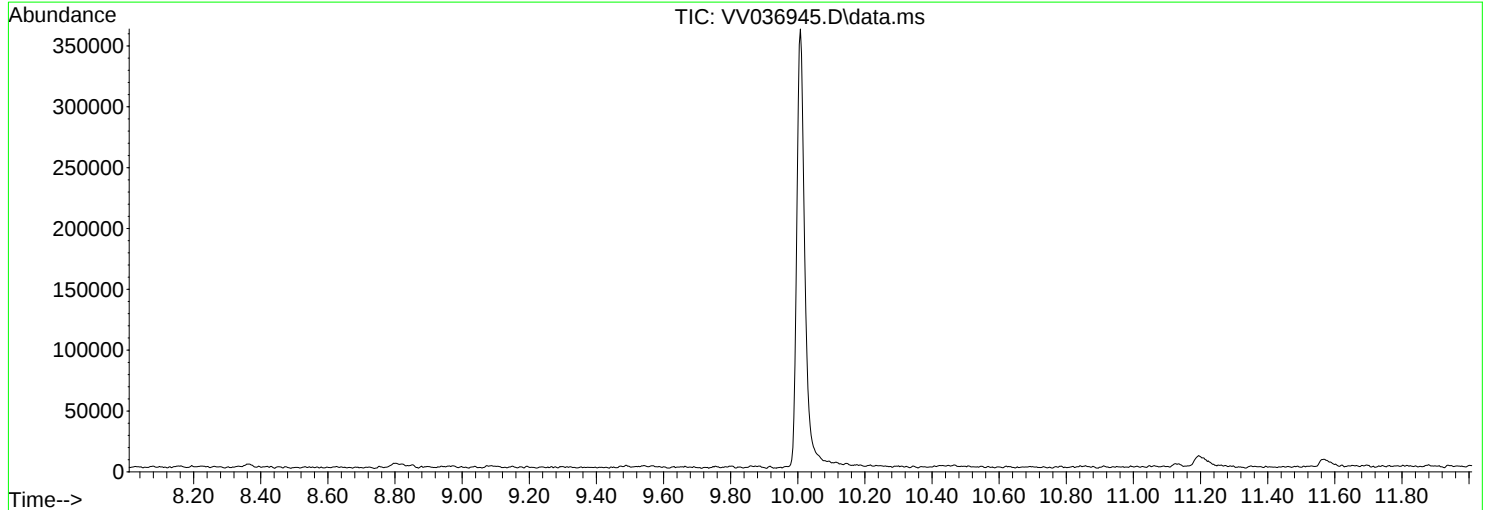

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	13776	PASS
75	95	30	80	52.4	37968	PASS
95	95	100	100	100.0	72483	PASS
96	95	5	9	6.9	5019	PASS
173	174	0.00	2	0.5	262	PASS
174	95	50	120	72.3	52392	PASS
175	174	5	9	7.6	3983	PASS
176	174	95	105	98.4	51549	PASS
177	176	5	10	6.3	3230	PASS

m/z	Abundance
35.80	222.0
36.90	109.0
37.80	135.0
38.40	131.0
39.00	276.0
39.90	494.0
40.90	161.0
41.70	174.0
43.10	238.0
43.90	1091.0
54.80	113.0
55.70	190.0
64.80	138.0
66.10	119.0
66.90	113.0
69.00	102.0
69.80	126.0
72.90	103.0
76.90	191.0
207.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.10	115.0
36.00	768.0
37.00	3792.0
38.00	3368.0
39.00	1615.0
39.90	626.0
41.00	168.0
41.80	115.0
42.30	103.0
42.90	133.0
43.90	1660.0
45.00	772.0
46.00	173.0
47.10	949.0
48.00	456.0
49.00	2915.0
50.00	14112.0
51.00	4087.0
51.90	290.0
55.00	435.0
55.90	1270.0
56.90	2187.0
58.10	216.0
59.90	841.0
61.00	3899.0
62.00	3585.0
63.00	2556.0
64.00	420.0
64.90	270.0
67.00	356.0
68.00	7202.0
69.00	8089.0
70.00	768.0
71.10	105.0
72.10	500.0
73.00	3475.0
74.00	13375.0
75.00	37944.0
76.00	3038.0
76.90	618.0
77.90	327.0
78.90	2832.0
79.90	656.0
80.90	2658.0
81.90	676.0
86.90	3779.0
88.00	2875.0
91.00	483.0
92.00	2238.0
93.00	2925.0
94.00	9507.0
95.00	73216.0
96.00	5268.0
97.00	174.0
103.90	354.0
104.90	157.0
105.90	594.0
110.90	104.0
112.70	119.0
115.90	354.0
116.90	757.0
117.70	215.0
118.90	398.0
123.80	114.0
127.90	230.0
128.70	127.0
129.70	310.0
134.60	120.0
136.60	144.0
137.00	164.0
140.90	712.0
141.90	159.0
142.90	844.0
145.70	120.0
147.90	400.0
149.80	107.0
155.10	126.0
171.20	158.0
171.80	296.0
173.90	51040.0
175.00	4058.0
175.90	50296.0
176.90	3304.0
177.90	157.0
207.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.00	105.0
36.00	769.0
37.00	3987.0
38.00	3293.0
39.00	1688.0
39.90	612.0
41.00	198.0
41.70	150.0
42.90	161.0
43.90	1706.0
45.00	806.0
46.00	196.0
47.10	930.0
48.00	550.0
49.00	2849.0
50.00	14194.0
51.00	4483.0
51.90	303.0
55.00	501.0
55.90	1376.0
56.90	2258.0
58.10	177.0
59.90	886.0
61.00	3916.0
62.00	3462.0
63.00	2770.0
64.00	483.0
65.00	302.0
67.00	306.0
68.00	7598.0
69.00	8348.0
70.00	918.0
72.00	501.0
73.00	3669.0
74.00	13532.0
75.00	39192.0
76.00	3057.0
76.90	714.0
77.90	406.0
78.90	2907.0
79.90	702.0
80.90	2812.0
81.90	671.0
86.90	3622.0
87.90	3239.0
91.00	471.0
92.00	2436.0
93.00	2924.0
94.00	9644.0
95.00	74584.0
96.00	5147.0
97.00	183.0
103.90	330.0
104.90	162.0
105.90	532.0
110.90	177.0
112.70	120.0
115.80	302.0
116.90	716.0
117.70	231.0
118.90	420.0
123.70	115.0
127.90	302.0
128.90	134.0
129.80	347.0
130.80	107.0
134.60	117.0
136.60	119.0
137.00	148.0
140.90	841.0
141.90	196.0
142.90	811.0
144.80	127.0
145.80	105.0
147.90	351.0
149.90	130.0
152.00	102.0
154.50	132.0
155.10	144.0
157.00	122.0
160.70	101.0
171.20	134.0
171.90	317.0
173.90	54184.0
175.00	4038.0
175.90	53512.0
177.00	3298.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363

m/z	Abundance
35.00	110.0
36.10	709.0
37.00	3713.0
38.00	3055.0
39.00	1541.0
39.90	572.0
41.00	195.0
41.60	186.0
42.90	196.0
44.00	1611.0
45.00	749.0
45.90	201.0
47.00	783.0
48.00	527.0
49.00	2756.0
50.00	13023.0
51.00	4425.0
51.80	301.0
52.80	122.0
55.00	505.0
55.90	1295.0
56.90	2162.0
58.00	113.0
59.90	808.0
61.00	3478.0
62.00	3307.0
63.00	2963.0
64.00	475.0
65.00	382.0
67.00	242.0
68.00	7296.0
69.00	7789.0
70.00	878.0
72.00	489.0
73.00	3339.0
74.00	12538.0
75.00	36768.0
76.00	2727.0
77.00	717.0
77.80	430.0
78.90	2562.0
79.90	724.0
80.90	2602.0
81.90	584.0
87.00	3086.0
87.90	3319.0
91.00	470.0
92.00	2372.0
93.00	2892.0
94.00	9030.0
95.00	69648.0
96.00	4641.0
97.00	150.0
103.80	312.0
104.90	156.0
105.80	425.0
107.00	106.0
110.90	187.0
115.70	247.0
116.90	595.0
117.70	206.0
118.90	360.0
127.90	422.0
128.90	154.0
129.80	352.0
130.80	184.0
134.80	112.0
137.00	115.0
140.90	827.0
141.90	139.0
142.90	753.0
144.80	128.0
146.00	127.0
147.90	258.0
149.90	141.0
154.60	165.0
155.00	149.0
157.00	147.0
171.90	306.0
173.00	786.0
173.90	51952.0
175.00	3854.0
175.90	50840.0
176.90	3087.0
177.90	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB363