

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027422.D
 Acq On : 17 Aug 2022 16:59
 Operator : SY/MD
 Sample : VV0818WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 18 02:24:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 02:23:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	266474	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	269651	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	120380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	90801	49.980	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	99.960%
7) Chloroethane-d5	1.561	69	72817	54.826	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.660%
11) 1,1-Dichloroethene-d2	2.105	63	146323	44.032	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.060%
21) 2-Butanone-d5	3.876	46	138158	85.433	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.430%
24) Chloroform-d	4.342	84	175219	47.084	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.160%
26) 1,2-Dichloroethane-d4	5.027	65	120457	52.134	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.260%
32) Benzene-d6	5.047	84	353256	54.629	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.260%
36) 1,2-Dichloropropane-d6	6.066	67	118859	51.673	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.340%
41) Toluene-d8	7.313	98	284681	51.649	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.300%
43) trans-1,3-Dichloroprop...	7.622	79	48351	48.225	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.460%
47) 2-Hexanone-d5	8.088	63	86283	77.882	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.880%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	156776	41.823	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.640%
66) 1,2-Dichlorobenzene-d4	11.622	152	104182	50.115	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.240%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.105	101	1350	0.703	ug/L	# 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027422.D
Acq On : 17 Aug 2022 16:59
Operator : SY/MD
Sample : VV0818WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 18 02:24:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 02:23:52 2022
Response via : Initial Calibration

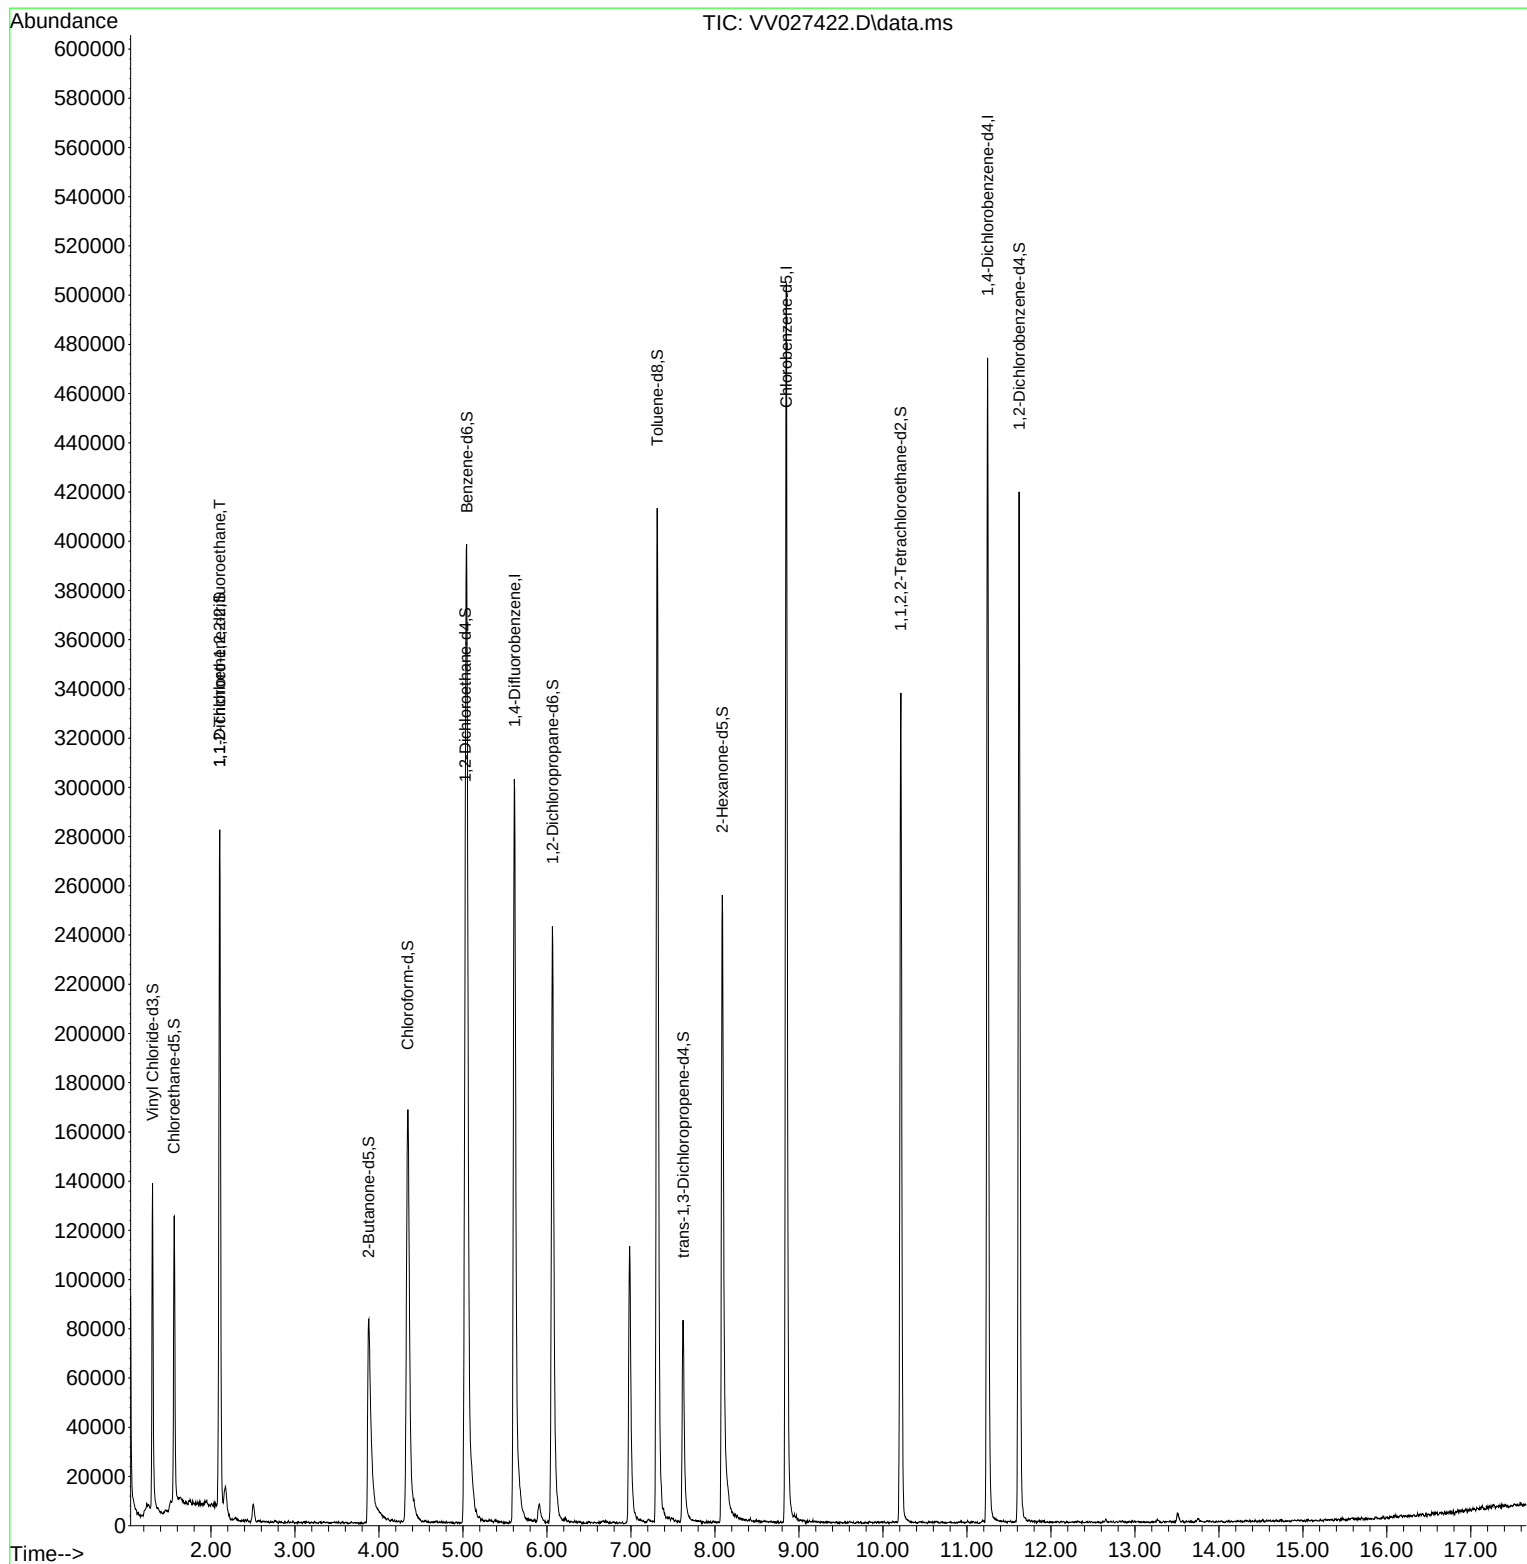

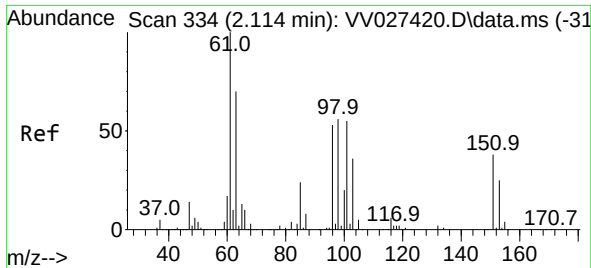

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.703 ug/L
 RT: 2.105 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV027422.D
 Acq: 17 Aug 2022 16:59

Instrument :
 MSVOA_V
 ClientSampleId :

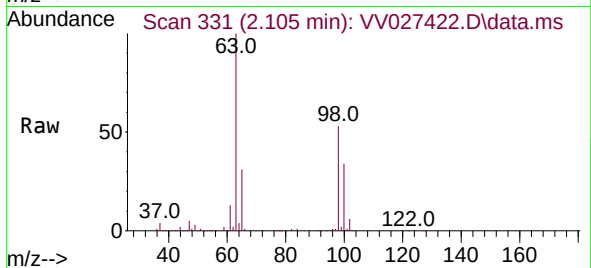

Tgt Ion:101 Resp: 1350
 Ion Ratio Lower Upper
 101 100
 85 3.2 34.1 51.1#
 151 0.0 57.8 86.8#

