

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027429.D
 Acq On : 18 Aug 2022 11:01
 Operator : SY/MD
 Sample : VV0818WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Aug 18 20:48:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 02:23:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	279534	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	284542	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	129166	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	90789	47.638	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.280%
7) Chloroethane-d5	1.564	69	64353	46.189	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.380%
11) 1,1-Dichloroethene-d2	2.105	63	150996	43.315	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.640%
21) 2-Butanone-d5	3.879	46	133625	78.770	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.770%
24) Chloroform-d	4.346	84	180709	46.290	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.580%
26) 1,2-Dichloroethane-d4	5.027	65	122209	50.421	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.840%
32) Benzene-d6	5.047	84	344817	50.534	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.060%
36) 1,2-Dichloropropane-d6	6.066	67	115143	47.438	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.880%
41) Toluene-d8	7.313	98	278529	47.889	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.780%
43) trans-1,3-Dichloroprop...	7.622	79	46912	44.341	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.680%
47) 2-Hexanone-d5	8.088	63	80858	69.165	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	69.170%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	151458	38.290	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.580%
66) 1,2-Dichlorobenzene-d4	11.622	152	101565	45.533	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.060%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.108	101	1414	0.702	ug/L	Qvalue # 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027429.D
Acq On : 18 Aug 2022 11:01
Operator : SY/MD
Sample : VV0818WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Aug 18 20:48:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 02:23:52 2022
Response via : Initial Calibration

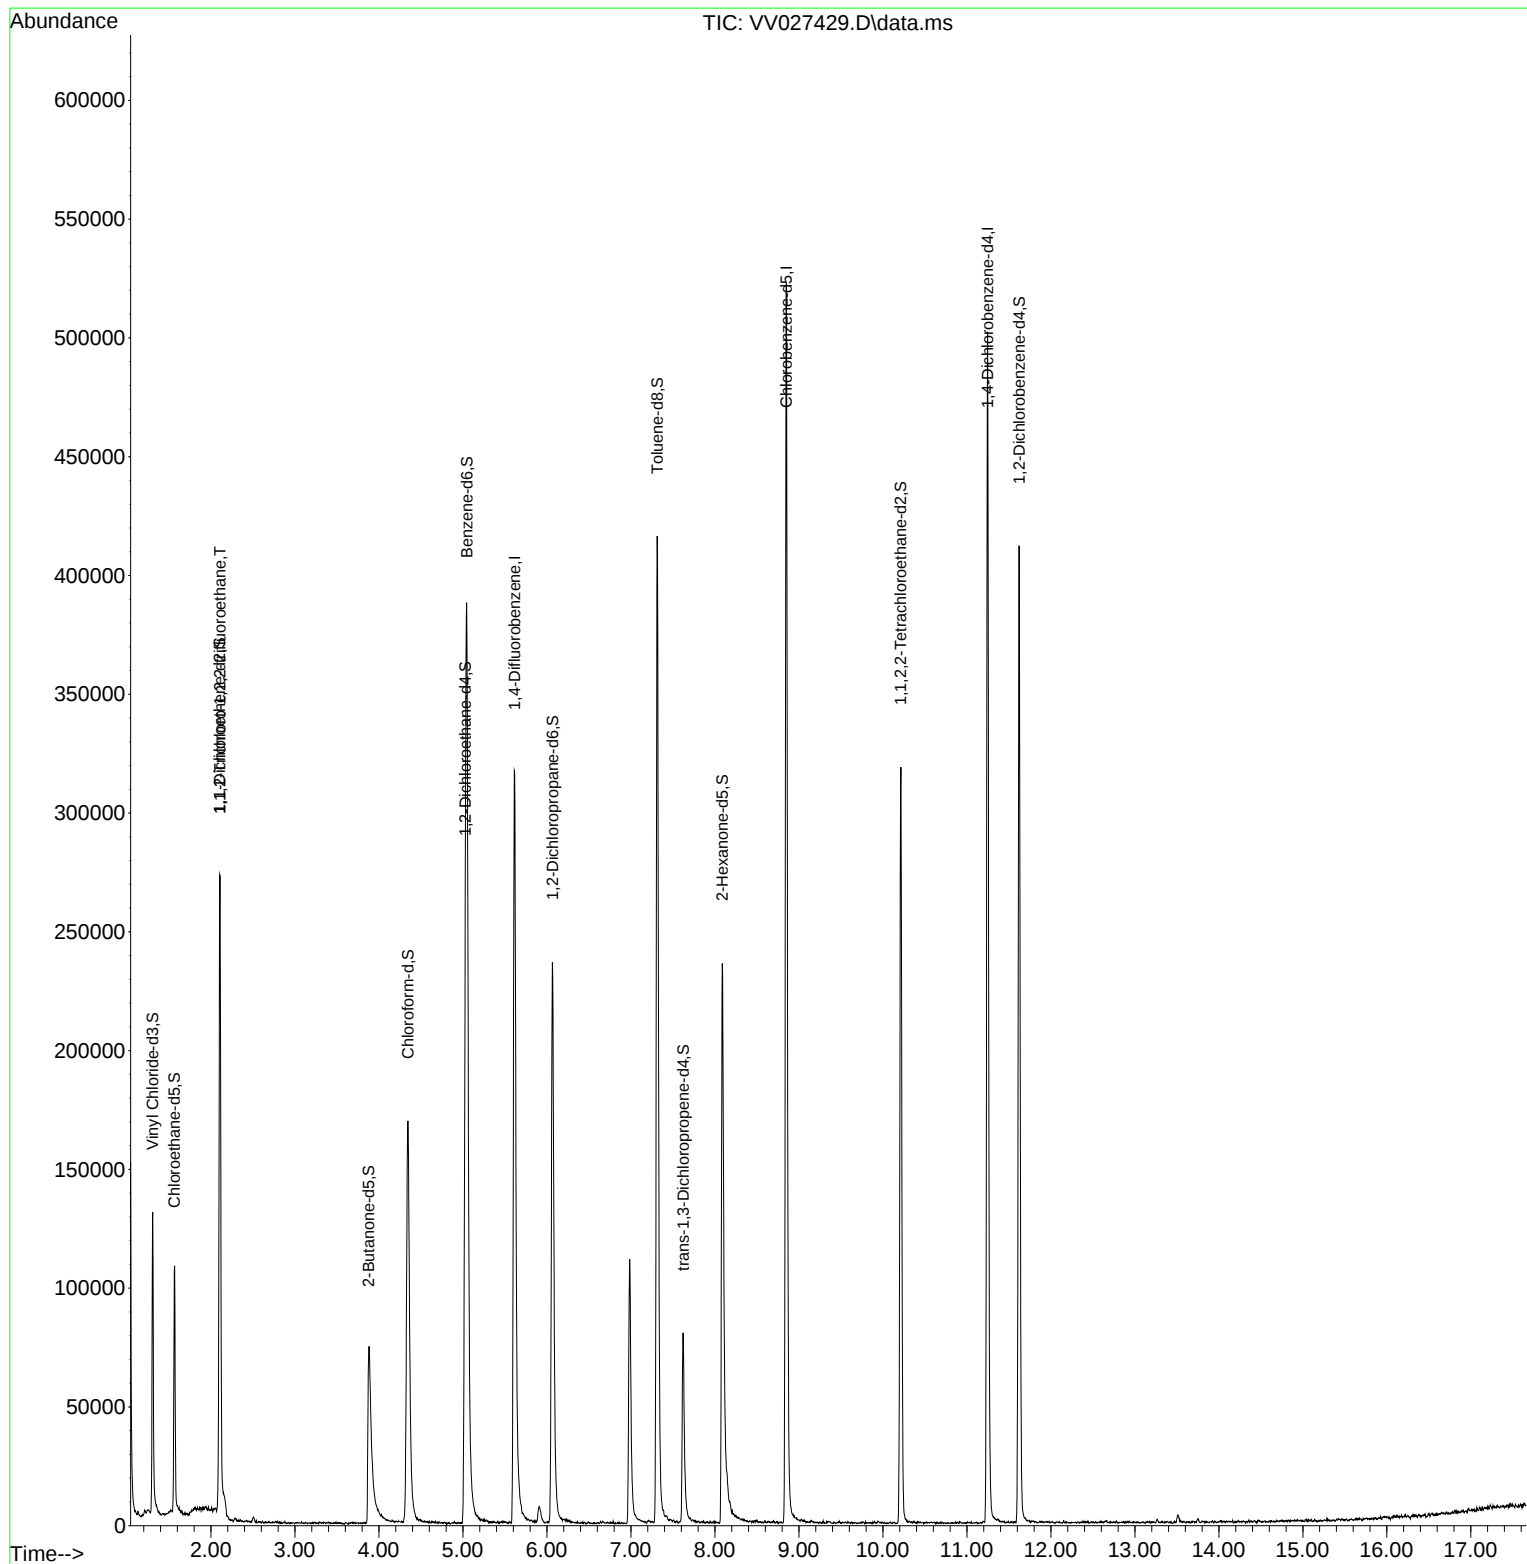

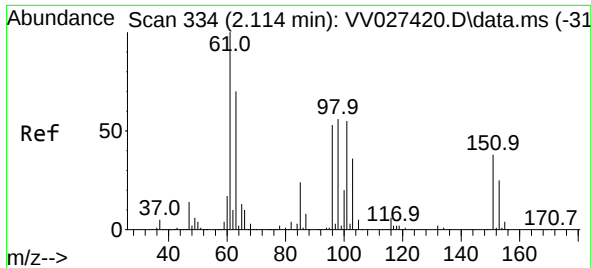

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.702 ug/L
 RT: 2.108 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: VV027429.D
 Acq: 18 Aug 2022 11:01

Instrument :
 MSVOA_V
 ClientSampleId :

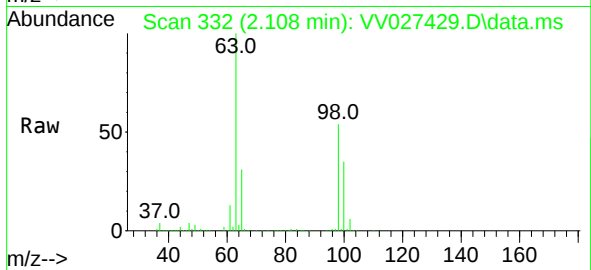

Tgt Ion:	101	Resp:	1414
Ion	Ratio	Lower	Upper
101	100		
85	4.5	34.1	51.1#
151	0.0	57.8	86.8#

