

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027421.D
 Acq On : 17 Aug 2022 16:34
 Operator : SY/MD
 Sample : VV0818MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M

Title : VOC Analysis

Signal : TIC: VV027421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	143155	151413	13.09%	1.771%
2	1.564	157	163	175	rVB	113248	129907	11.23%	1.519%
3	2.105	322	331	344	rBV	298794	419746	36.28%	4.909%
4	2.506	447	456	466	rBV5	8416	13741	1.19%	0.161%
5	2.600	482	485	487	rBV2	714	509	0.04%	0.006%
6	2.629	492	494	497	rBV3	548	298	0.03%	0.003%
7	2.728	523	525	528	rVB3	612	334	0.03%	0.004%
8	2.802	546	548	550	rBV2	399	244	0.02%	0.003%
9	2.892	573	576	581	rBV4	559	445	0.04%	0.005%
10	3.037	619	621	624	rBV2	689	407	0.04%	0.005%
11	3.050	624	625	628	rVB	843	324	0.03%	0.004%
12	3.069	628	631	633	rBV2	729	513	0.04%	0.006%
13	3.127	646	649	651	rBV3	357	249	0.02%	0.003%
14	3.214	673	676	678	rBV3	493	234	0.02%	0.003%
15	3.307	703	705	707	rBV3	472	229	0.02%	0.003%
16	3.371	721	725	727	rBV2	469	318	0.03%	0.004%
17	3.506	764	767	769	rVV3	452	257	0.02%	0.003%
18	3.641	806	809	811	rBV	614	391	0.03%	0.005%
19	3.715	827	832	834	rBV3	565	603	0.05%	0.007%
20	3.748	837	842	845	rBV2	463	334	0.03%	0.004%
21	3.818	862	864	867	rVB	618	310	0.03%	0.004%
22	3.879	872	883	911	rBV	83004	238117	20.58%	2.785%
23	4.233	990	993	998	rVB4	1033	630	0.05%	0.007%
24	4.346	1014	1028	1065	rVB	176901	463178	40.03%	5.417%
25	4.548	1089	1091	1094	rBV3	880	621	0.05%	0.007%
26	4.770	1159	1160	1163	rBV	535	263	0.02%	0.003%
27	4.815	1171	1174	1175	rBV2	426	257	0.02%	0.003%
28	4.825	1175	1177	1180	rVV2	780	393	0.03%	0.005%
29	4.844	1180	1183	1189	rVV4	843	724	0.06%	0.008%
30	5.043	1228	1245	1283	rBV2	424887	1157110	100.00%	13.534%
31	5.329	1332	1334	1338	rBV5	976	666	0.06%	0.008%
32	5.461	1373	1375	1381	rVB6	1166	891	0.08%	0.010%
33	5.490	1381	1384	1386	rBV3	803	525	0.05%	0.006%
34	5.612	1410	1422	1461	rBV	328529	718404	62.09%	8.403%
35	6.066	1551	1563	1594	rBV	250132	535989	46.32%	6.269%
36	6.345	1648	1650	1651	rBV	567	229	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027421.D
 Acq On : 17 Aug 2022 16:34
 Operator : SY/MD
 Sample : VV0818MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	6.381	1659	1661	1662	rBV2	617	234	0.02%	0.003%
38	6.391	1662	1664	1666	rVB4	705	284	0.02%	0.003%
39	6.429	1675	1676	1680	rVB3	1058	623	0.05%	0.007%
40	6.603	1728	1730	1734	rVB	422	296	0.03%	0.003%
41	6.754	1773	1777	1778	rBV3	406	286	0.02%	0.003%
42	6.776	1782	1784	1786	rVV	648	324	0.03%	0.004%
43	6.796	1789	1790	1795	rVB3	728	427	0.04%	0.005%
44	6.821	1795	1798	1801	rBV3	590	429	0.04%	0.005%
45	6.863	1806	1811	1815	rBV5	833	777	0.07%	0.009%
46	6.985	1838	1849	1874	rBV2	117237	233006	20.14%	2.725%
47	7.313	1939	1951	1980	rBV	453314	827708	71.53%	9.681%
48	7.622	2038	2047	2068	rBV	82977	155665	13.45%	1.821%
49	7.853	2116	2119	2123	rVB3	1289	850	0.07%	0.010%
50	7.979	2156	2158	2164	rVB4	955	806	0.07%	0.009%
51	8.088	2182	2192	2228	rBV	260403	539315	46.61%	6.308%
52	8.516	2324	2325	2326	rBV	745	247	0.02%	0.003%
53	8.612	2352	2355	2358	rBV3	861	574	0.05%	0.007%
54	8.693	2378	2380	2382	rBV2	658	306	0.03%	0.004%
55	8.738	2391	2394	2399	rVV5	631	649	0.06%	0.008%
56	8.850	2418	2429	2449	rBV	540731	884748	76.46%	10.348%
57	9.291	2564	2566	2571	rBV4	793	728	0.06%	0.009%
58	9.368	2586	2590	2592	rBV4	601	423	0.04%	0.005%
59	9.410	2598	2603	2606	rBV5	915	741	0.06%	0.009%
60	9.435	2608	2611	2613	rBV2	497	344	0.03%	0.004%
61	9.477	2621	2624	2626	rVB2	657	340	0.03%	0.004%
62	9.509	2630	2634	2635	rBV2	423	258	0.02%	0.003%
63	9.812	2725	2728	2733	rBV2	716	681	0.06%	0.008%
64	9.841	2735	2737	2741	rVB2	503	269	0.02%	0.003%
65	9.937	2764	2767	2770	rBV3	730	667	0.06%	0.008%
66	10.095	2813	2816	2818	rVB3	608	320	0.03%	0.004%
67	10.111	2818	2821	2823	rBV3	407	283	0.02%	0.003%
68	10.168	2836	2839	2841	rBV2	522	327	0.03%	0.004%
69	10.214	2841	2853	2870	rBV	345408	543277	46.95%	6.354%
70	10.451	2926	2927	2930	rVB	607	277	0.02%	0.003%
71	10.477	2933	2935	2938	rVB3	762	388	0.03%	0.005%
72	10.500	2938	2942	2945	rBV3	490	422	0.04%	0.005%
73	10.538	2951	2954	2959	rVB5	768	720	0.06%	0.008%
74	10.680	2996	2998	3000	rVV2	508	253	0.02%	0.003%
75	10.715	3007	3009	3012	rBV3	477	275	0.02%	0.003%
76	10.741	3015	3017	3020	rBV2	548	415	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027421.D
 Acq On : 17 Aug 2022 16:34
 Operator : SY/MD
 Sample : VV0818MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.789	3029	3032	3037	rVB4	890	675	0.06%	0.008%
78	10.815	3037	3040	3043	rBV4	817	654	0.06%	0.008%
79	10.918	3068	3072	3076	rBV5	1226	923	0.08%	0.011%
80	11.159	3145	3147	3151	rBV3	860	556	0.05%	0.007%
81	11.246	3162	3174	3196	rBV	503656	793133	68.54%	9.277%
82	11.551	3266	3269	3272	rBV3	872	537	0.05%	0.006%
83	11.622	3280	3291	3312	rBV	436981	689276	59.57%	8.062%
84	11.863	3364	3366	3368	rBV	587	258	0.02%	0.003%
85	12.117	3443	3445	3448	rBV2	591	284	0.02%	0.003%
86	12.291	3494	3499	3501	rBV3	419	355	0.03%	0.004%
87	12.307	3501	3504	3508	rBV2	585	448	0.04%	0.005%
88	12.336	3511	3513	3515	rBV2	598	295	0.03%	0.003%
89	12.384	3525	3528	3533	rBV6	790	614	0.05%	0.007%
90	12.651	3606	3611	3618	rVB6	1852	2350	0.20%	0.027%
91	13.011	3720	3723	3726	rBV2	762	457	0.04%	0.005%
92	13.149	3763	3766	3769	rVB3	524	330	0.03%	0.004%
93	13.165	3769	3771	3774	rBV	759	430	0.04%	0.005%
94	13.262	3798	3801	3813	rVB8	2673	3697	0.32%	0.043%
95	13.506	3870	3877	3886	rBV2	8570	13691	1.18%	0.160%
96	13.737	3946	3949	3950	rBV2	2684	1384	0.12%	0.016%
97	13.786	3962	3964	3967	rVB3	776	261	0.02%	0.003%
98	13.914	4002	4004	4009	rVB3	785	369	0.03%	0.004%
99	13.972	4018	4022	4023	rBV3	759	517	0.04%	0.006%
100	14.490	4181	4183	4186	rBV2	538	436	0.04%	0.005%




Sum of corrected areas: 8549695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027421.D
Acq On : 17 Aug 2022 16:34
Operator : SY/MD
Sample : VV0818MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

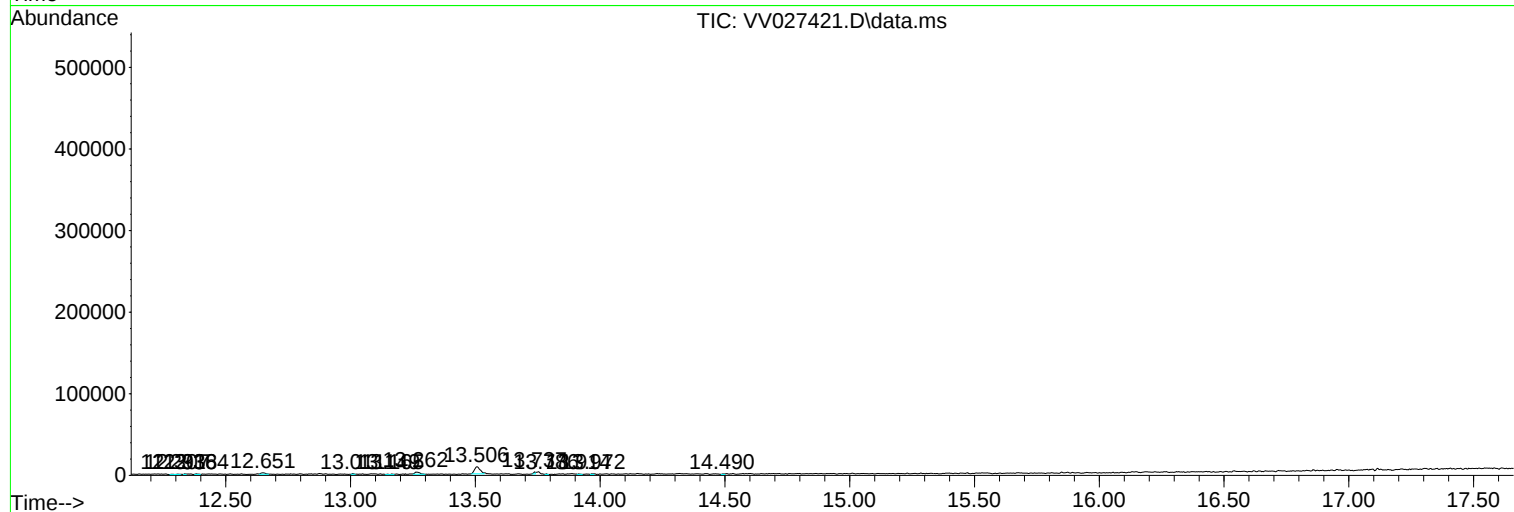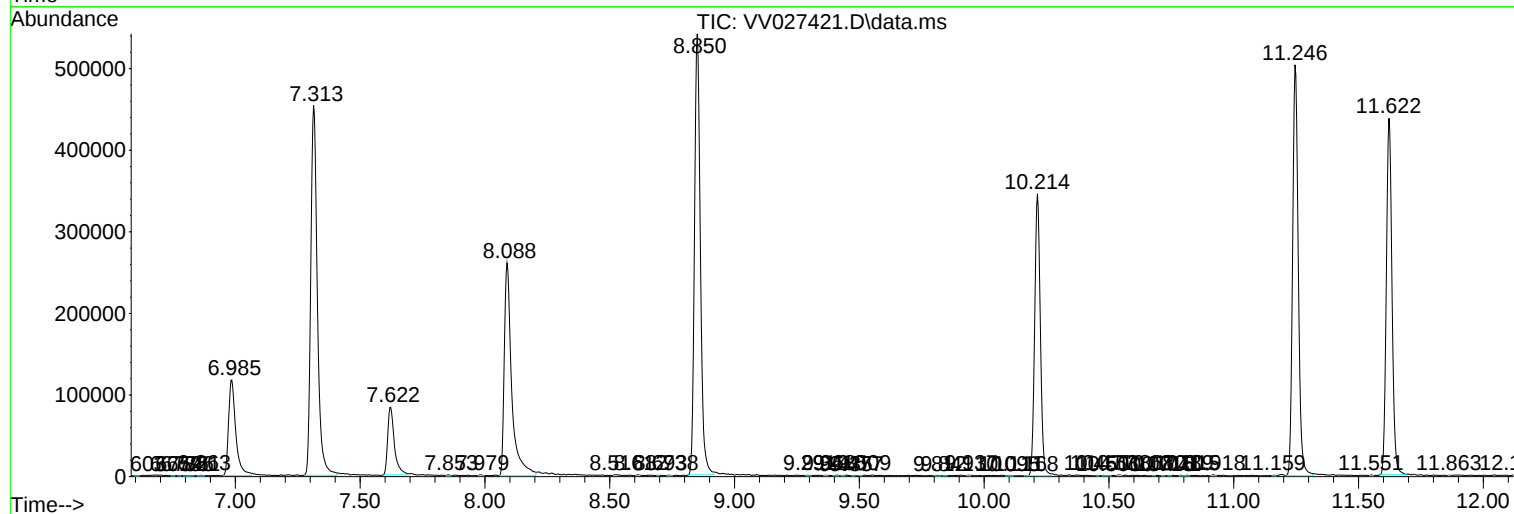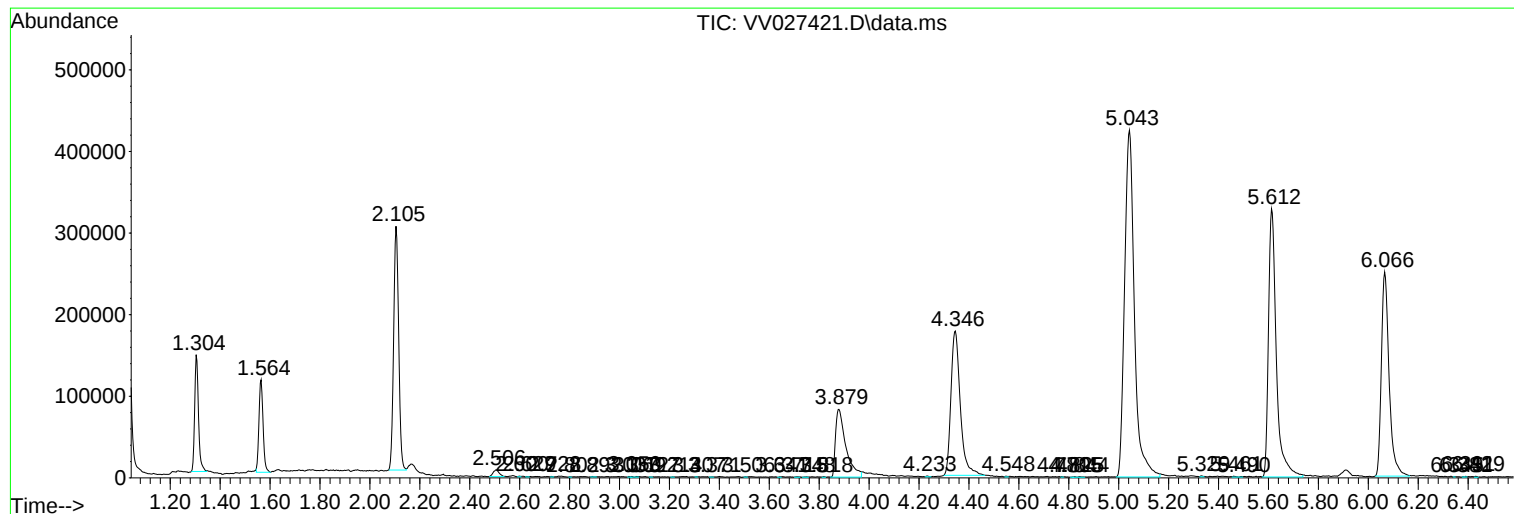

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027421.D
Acq On : 17 Aug 2022 16:34
Operator : SY/MD
Sample : VV0818MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027421.D
Acq On : 17 Aug 2022 16:34
Operator : SY/MD
Sample : VV0818MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK260

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc