

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027422.D
 Acq On : 17 Aug 2022 16:59
 Operator : SY/MD
 Sample : VV0818WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VV027422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	131909	140830	13.01%	1.748%
2	1.564	157	163	177	rVB	115135	132728	12.26%	1.647%
3	2.105	322	331	345	rVB	273456	385771	35.63%	4.788%
4	2.709	516	519	522	rBV3	772	482	0.04%	0.006%
5	2.728	523	525	531	rVB3	573	454	0.04%	0.006%
6	2.757	531	534	537	rBV4	923	787	0.07%	0.010%
7	2.812	548	551	554	rBV3	1047	790	0.07%	0.010%
8	2.838	557	559	562	rVV2	535	270	0.02%	0.003%
9	2.879	570	572	575	rBV4	759	466	0.04%	0.006%
10	2.921	583	585	589	rVB3	968	574	0.05%	0.007%
11	2.976	599	602	608	rVB4	1128	954	0.09%	0.012%
12	3.079	630	634	636	rVB3	661	462	0.04%	0.006%
13	3.105	636	642	644	rBV5	783	812	0.07%	0.010%
14	3.117	644	646	649	rVB2	745	327	0.03%	0.004%
15	3.137	649	652	654	rBV3	637	443	0.04%	0.005%
16	3.185	665	667	669	rBV2	465	318	0.03%	0.004%
17	3.233	678	682	687	rBV3	822	639	0.06%	0.008%
18	3.288	696	699	700	rBV3	560	338	0.03%	0.004%
19	3.416	735	739	742	rBV3	370	271	0.03%	0.003%
20	3.561	779	784	786	rBV3	895	693	0.06%	0.009%
21	3.600	791	796	799	rBV4	634	687	0.06%	0.009%
22	3.674	815	819	822	rVV4	472	394	0.04%	0.005%
23	3.738	836	839	842	rBV3	379	312	0.03%	0.004%
24	3.789	853	855	857	rBV2	697	377	0.03%	0.005%
25	3.818	861	864	866	rBV	488	324	0.03%	0.004%
26	3.879	873	883	915	rBV	82724	241989	22.35%	3.003%
27	4.265	1000	1003	1005	rBV2	1083	729	0.07%	0.009%
28	4.346	1013	1028	1048	rBV	166703	430237	39.73%	5.340%
29	4.773	1159	1161	1166	rVB2	732	404	0.04%	0.005%
30	4.796	1166	1168	1170	rBV2	578	305	0.03%	0.004%
31	4.921	1200	1207	1210	rBV6	726	922	0.09%	0.011%
32	4.966	1219	1221	1223	rBV	492	274	0.03%	0.003%
33	5.043	1227	1245	1280	rBV2	397659	1082825	100.00%	13.439%
34	5.397	1353	1355	1359	rVB4	827	492	0.05%	0.006%
35	5.497	1383	1386	1390	rBV3	710	570	0.05%	0.007%
36	5.612	1411	1422	1463	rBV	301153	656833	60.66%	8.152%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027422.D
 Acq On : 17 Aug 2022 16:59
 Operator : SY/MD
 Sample : VV0818WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

37	5.911	1506	1515	1530	rVB	6781	14232	1.31%	0.177%
38	6.011	1544	1546	1549	rVB3	1025	556	0.05%	0.007%
39	6.066	1549	1563	1588	rBV	242390	514707	47.53%	6.388%
40	6.329	1643	1645	1649	rVB3	760	431	0.04%	0.005%
41	6.368	1655	1657	1659	rBV3	704	471	0.04%	0.006%
42	6.432	1675	1677	1680	rVV3	761	418	0.04%	0.005%
43	6.526	1704	1706	1710	rBV4	402	328	0.03%	0.004%
44	6.564	1715	1718	1721	rBV3	550	353	0.03%	0.004%
45	6.645	1741	1743	1744	rBV2	730	282	0.03%	0.003%
46	6.664	1745	1749	1751	rBV5	692	586	0.05%	0.007%
47	6.699	1757	1760	1761	rBV3	845	450	0.04%	0.006%
48	6.828	1798	1800	1804	rVB2	710	451	0.04%	0.006%
49	6.863	1804	1811	1815	rBV5	681	769	0.07%	0.010%
50	6.899	1820	1822	1827	rVB4	778	466	0.04%	0.006%
51	6.944	1831	1836	1837	rBV2	573	399	0.04%	0.005%
52	6.985	1838	1849	1868	rBV	112012	215664	19.92%	2.677%
53	7.313	1940	1951	1971	rBV	411883	757038	69.91%	9.396%
54	7.561	2025	2028	2032	rBV4	945	681	0.06%	0.008%
55	7.622	2037	2047	2070	rBV2	81822	152937	14.12%	1.898%
56	7.854	2116	2119	2120	rBV2	918	544	0.05%	0.007%
57	7.892	2127	2131	2132	rBV	454	312	0.03%	0.004%
58	7.918	2137	2139	2142	rBV3	865	597	0.06%	0.007%
59	7.947	2146	2148	2152	rVB3	920	572	0.05%	0.007%
60	7.969	2152	2155	2157	rBV2	776	438	0.04%	0.005%
61	8.088	2182	2192	2227	rBV	254804	523302	48.33%	6.495%
62	8.741	2391	2395	2397	rBV2	940	648	0.06%	0.008%
63	8.776	2402	2406	2407	rBV3	526	404	0.04%	0.005%
64	8.850	2417	2429	2454	rVV	503424	836279	77.23%	10.379%
65	9.088	2500	2503	2504	rBV2	658	362	0.03%	0.004%
66	9.262	2555	2557	2559	rBV2	731	404	0.04%	0.005%
67	9.291	2565	2566	2569	rBV	577	270	0.02%	0.003%
68	9.477	2620	2624	2627	rBV2	727	398	0.04%	0.005%
69	9.734	2701	2704	2706	rVB3	543	294	0.03%	0.004%
70	9.789	2720	2721	2728	rVB4	478	353	0.03%	0.004%
71	9.837	2732	2736	2739	rBV3	883	831	0.08%	0.010%
72	9.953	2770	2772	2775	rVB4	573	295	0.03%	0.004%
73	9.972	2775	2778	2780	rBV3	505	354	0.03%	0.004%
74	10.017	2789	2792	2795	rVB4	749	450	0.04%	0.006%
75	10.050	2800	2802	2805	rBV3	477	298	0.03%	0.004%
76	10.062	2805	2806	2809	rVB2	679	280	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
 Data File : VV027422.D
 Acq On : 17 Aug 2022 16:59
 Operator : SY/MD
 Sample : VV0818WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
 Title : VOC Analysis

77	10.082	2809	2812	2815	rBV3	526	504	0.05%	0.006%
78	10.117	2818	2823	2827	rBV2	771	673	0.06%	0.008%
79	10.214	2841	2853	2872	rBV	337060	527978	48.76%	6.553%
80	10.542	2952	2955	2956	rBV	926	457	0.04%	0.006%
81	10.689	2997	3001	3002	rBV2	534	376	0.03%	0.005%
82	10.738	3014	3016	3020	rVB2	577	348	0.03%	0.004%
83	10.873	3055	3058	3062	rVB3	450	262	0.02%	0.003%
84	11.050	3109	3113	3115	rBV2	796	503	0.05%	0.006%
85	11.072	3118	3120	3124	rVV5	702	603	0.06%	0.007%
86	11.246	3164	3174	3196	rBV	473163	742562	68.58%	9.216%
87	11.487	3247	3249	3253	rBV4	746	763	0.07%	0.009%
88	11.622	3279	3291	3311	rBV	418615	656395	60.62%	8.147%
89	11.808	3347	3349	3350	rBV	670	274	0.03%	0.003%
90	11.924	3383	3385	3390	rVB2	824	360	0.03%	0.004%
91	12.374	3523	3525	3528	rBV2	949	538	0.05%	0.007%
92	12.619	3598	3601	3605	rBV5	901	631	0.06%	0.008%
93	12.889	3683	3685	3690	rVB2	645	454	0.04%	0.006%
94	12.972	3706	3711	3715	rBV3	967	794	0.07%	0.010%
95	13.213	3785	3786	3790	rBV4	535	362	0.03%	0.004%
96	13.265	3798	3802	3803	rBV2	1200	722	0.07%	0.009%
97	13.506	3872	3877	3884	rBV4	3330	4948	0.46%	0.061%
98	13.599	3903	3906	3908	rBV2	720	475	0.04%	0.006%
99	13.615	3909	3911	3915	rVV4	721	502	0.05%	0.006%
100	15.046	4352	4356	4358	rBV2	985	758	0.07%	0.009%




Sum of corrected areas: 8057229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027422.D
Acq On : 17 Aug 2022 16:59
Operator : SY/MD
Sample : VV0818WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

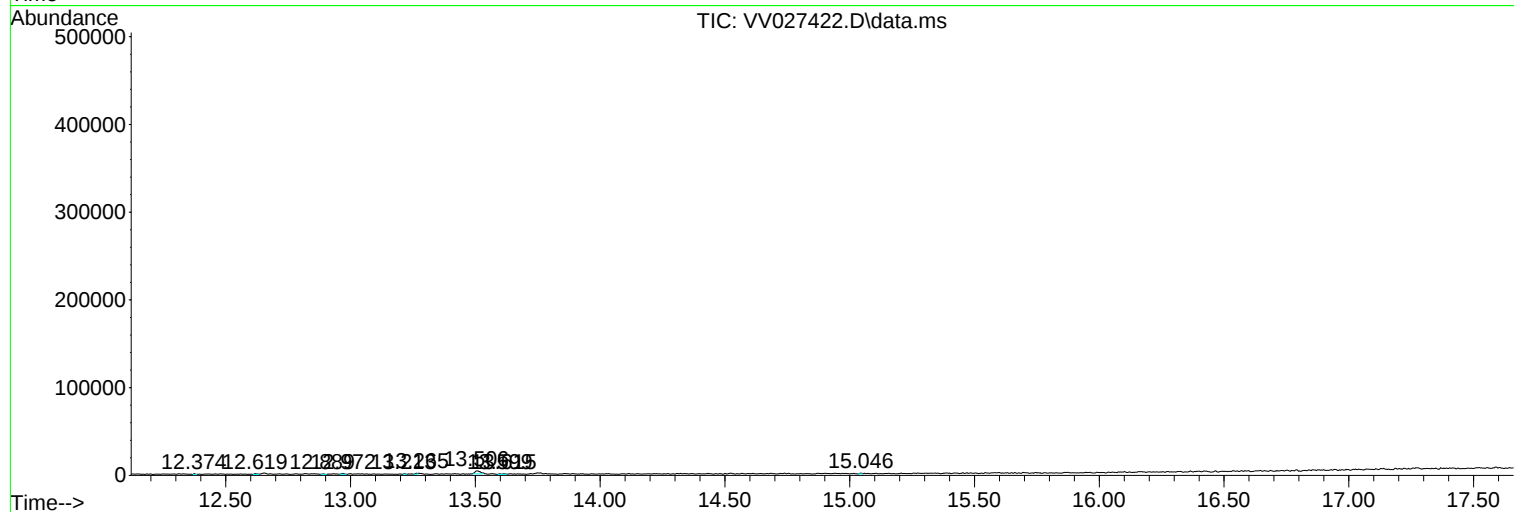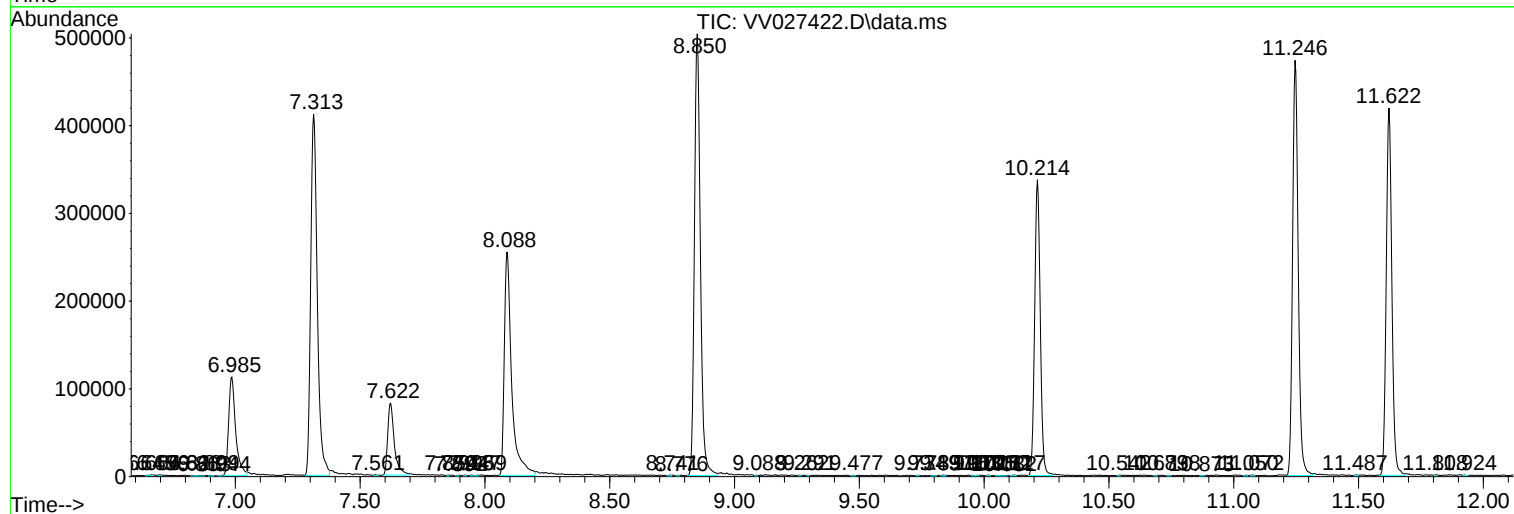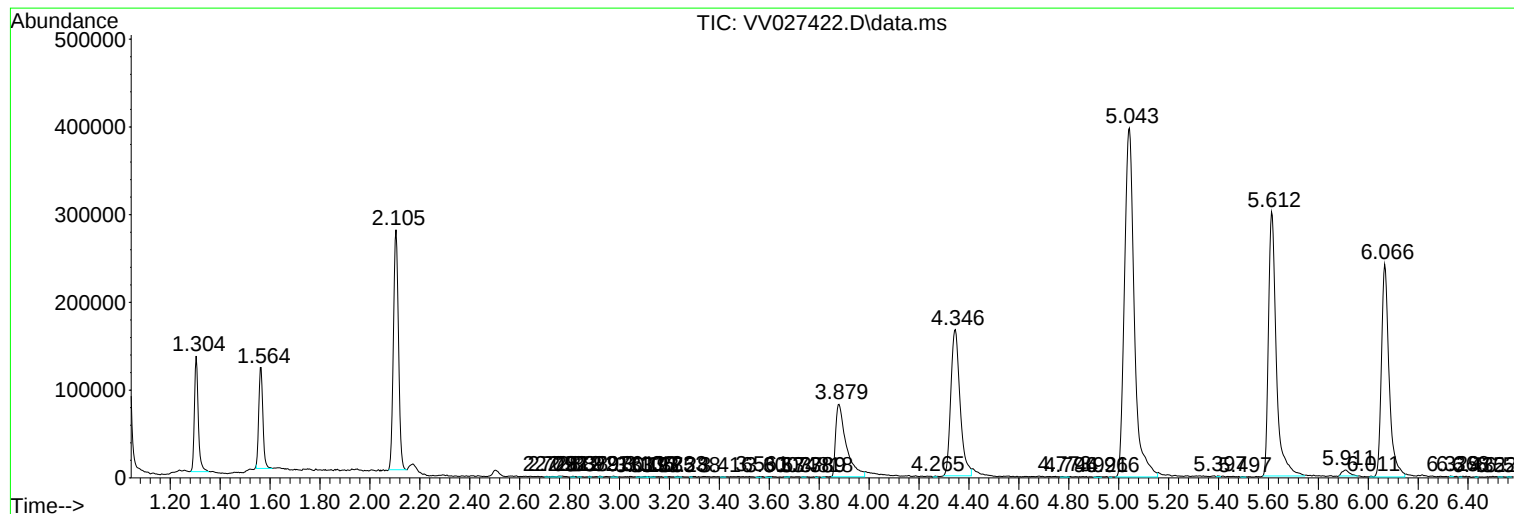

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027422.D
Acq On : 17 Aug 2022 16:59
Operator : SY/MD
Sample : VV0818WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081822\
Data File : VV027422.D
Acq On : 17 Aug 2022 16:59
Operator : SY/MD
Sample : VV0818WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc